

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024098.D
 Acq On : 26 Jul 2022 13:46
 Operator : SY/VA
 Sample : N3790-14RE
 Misc : 3.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK8RE

Quant Time: Jul 26 23:42:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	207695	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	131498	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	31188	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	127625	28.667	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	114.680%
7) Chloroethane-d5	2.581	69	280	0.093	ug/L	-0.29
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.360%#
11) 1,1-Dichloroethene-d2	4.007	63	59037	15.060	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.240%
21) 2-Butanone-d5	7.080	46	9043	11.429	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	22.860%
24) Chloroform-d	7.647	84	148944	26.085	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.360%
26) 1,2-Dichloroethane-d4	8.305	65	88556	26.995	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.960%
32) Benzene-d6	8.275	84	214941	35.187	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	140.760%#
36) 1,2-Dichloropropane-d6	9.275	67	79976	41.509	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	166.040%#
41) Toluene-d8	10.323	98	158920	26.014	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.040%
43) trans-1,3-Dichloroprop...	10.573	79	5321	6.229	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	24.920%#
47) 2-Hexanone-d5	10.927	63	1669	4.143	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	8.280%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	52640	23.678	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.720%
66) 1,2-Dichlorobenzene-d4	13.853	152	23246	23.015	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.040%
Target Compounds					Qvalue	
13) Acetone	4.129	43	10710	19.075	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024098.D
Acq On : 26 Jul 2022 13:46
Operator : SY/VA
Sample : N3790-14RE
Misc : 3.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK8RE

Quant Time: Jul 26 23:42:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

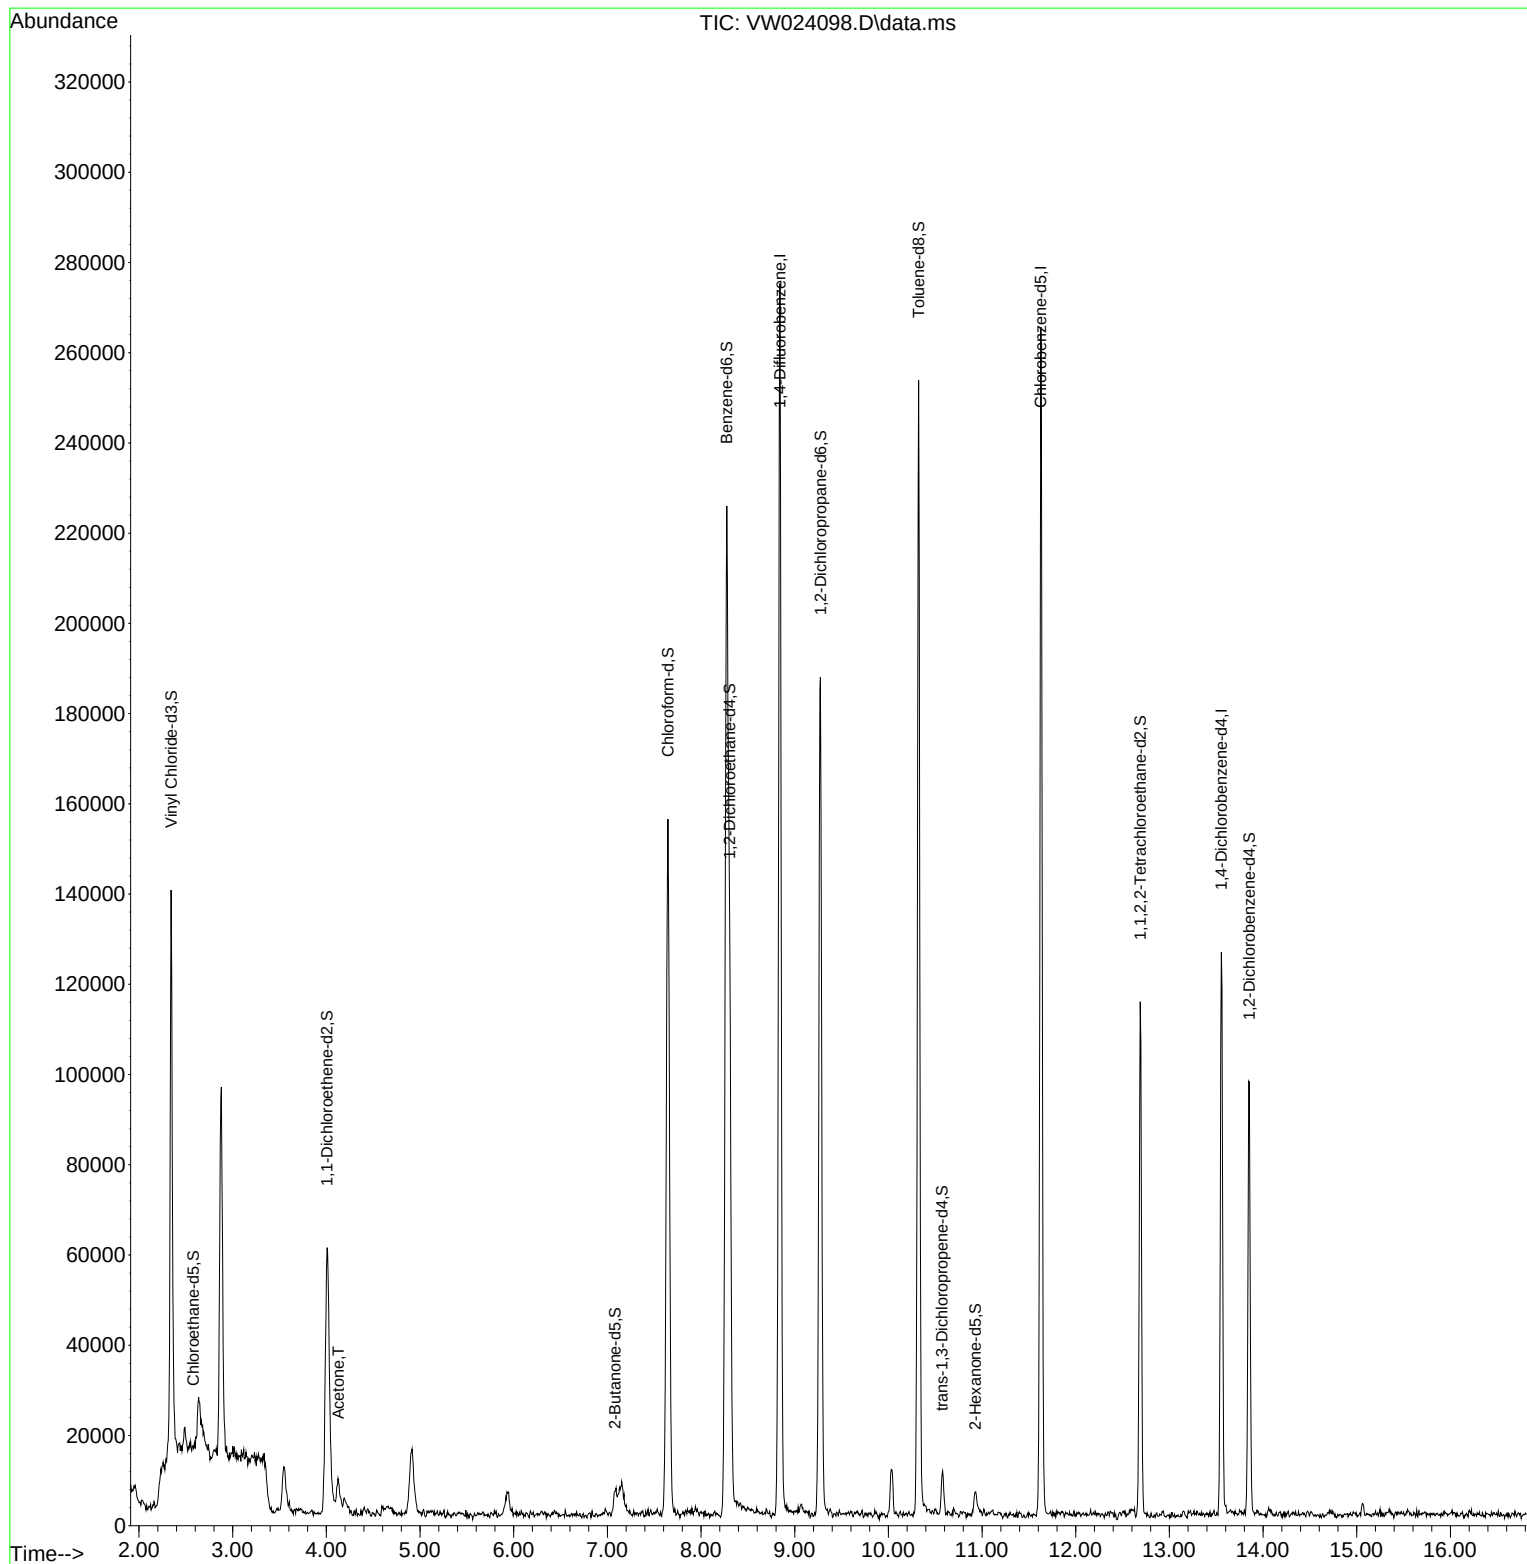

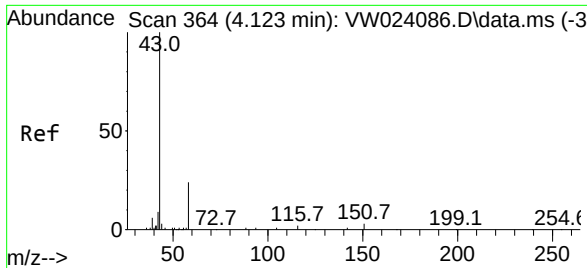

#13
 Acetone
 Concen: 19.075 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW024098.D
 Acq: 26 Jul 2022 13:46

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK8RE

Tgt Ion: 43 Resp: 10710
 Ion Ratio Lower Upper
 43 100
 58 22.1 0.0 60.0

