

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024089.D
 Acq On : 26 Jul 2022 10:06
 Operator : SY/VA
 Sample : N3795-06
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Supervised By :Mahesh
 Dadoda
 07/27/2022

Quant Time: Jul 26 23:40:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

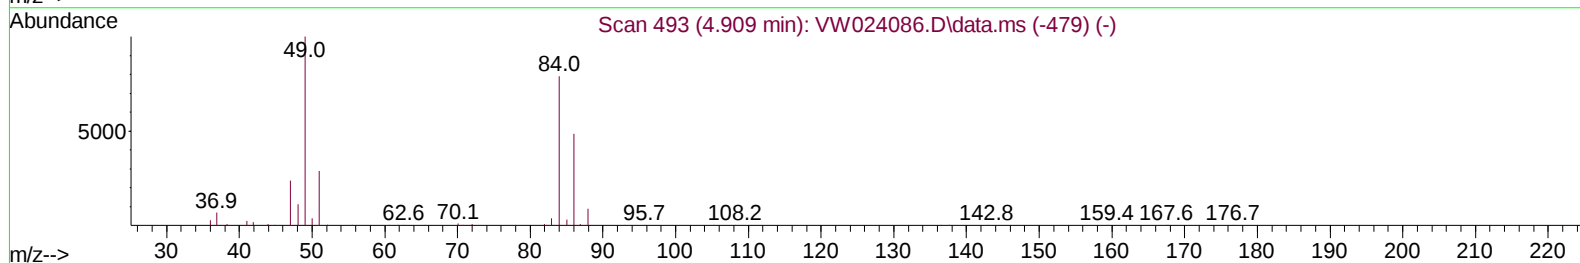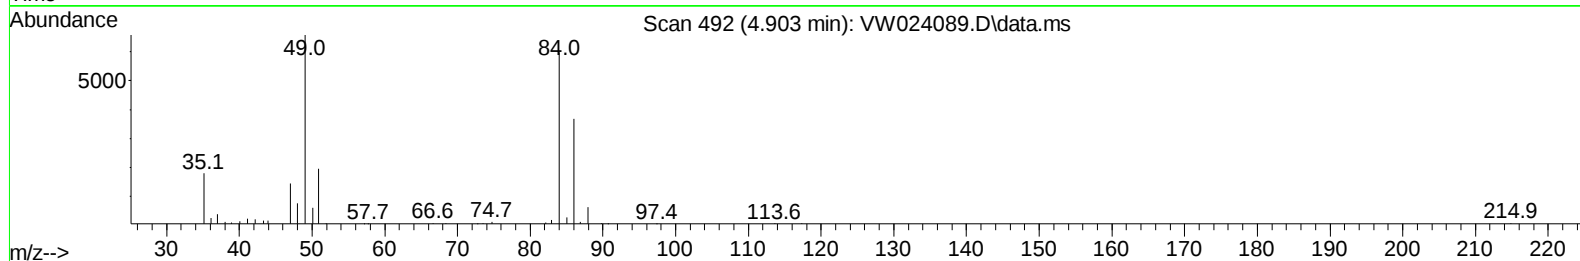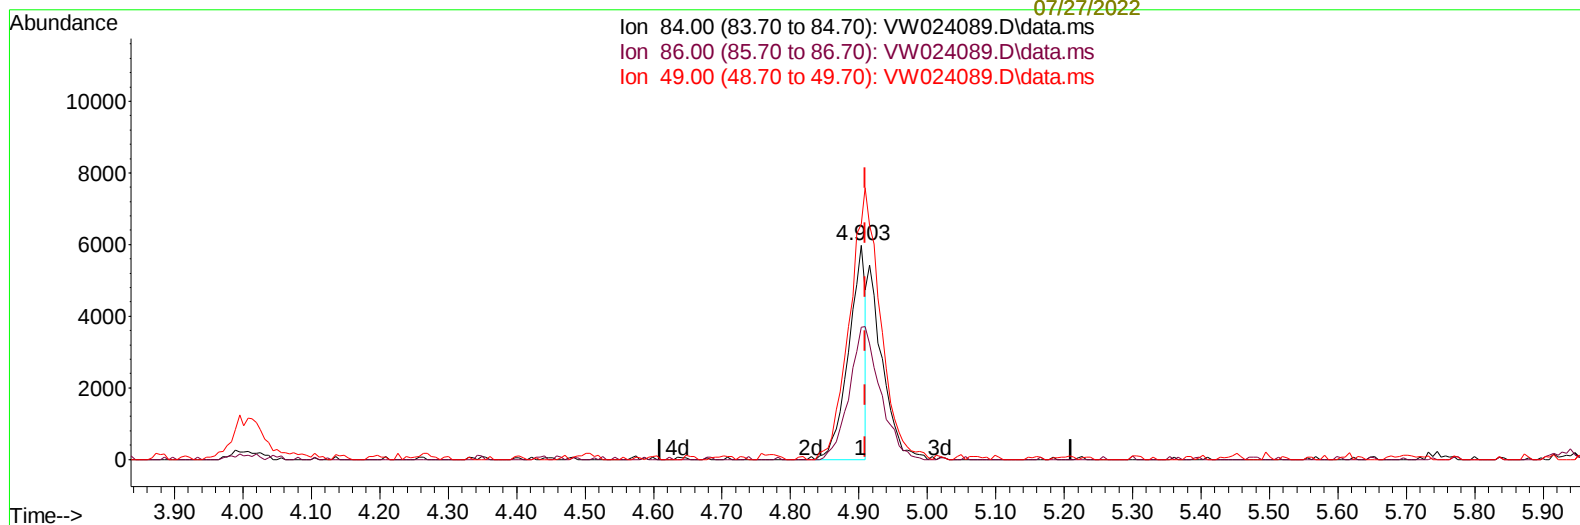

TIC: VW024089.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.006) 2.91 ug/L

response 10331

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	61.72
49.00	119.50	109.98
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024089.D
Acq On : 26 Jul 2022 10:06
Operator : SY/VA
Sample : N3795-06
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Supervised By :Mahesh
Dadoda
07/27/2022

Quant Time: Jul 26 23:40:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

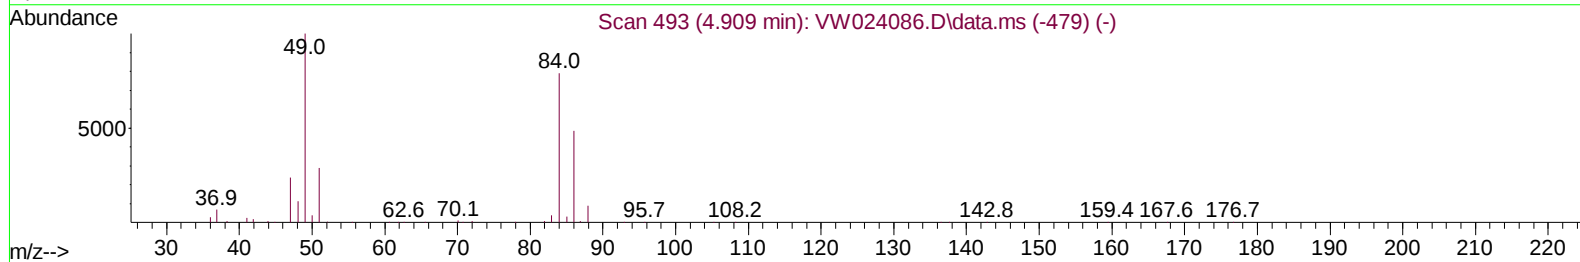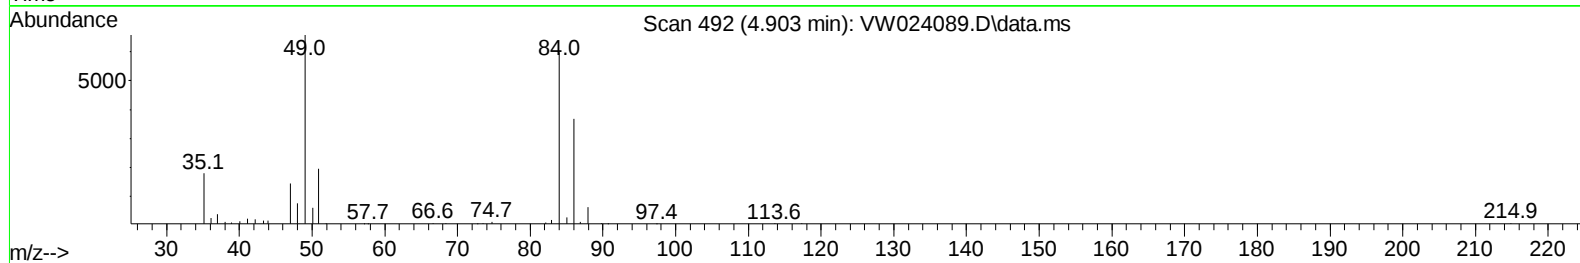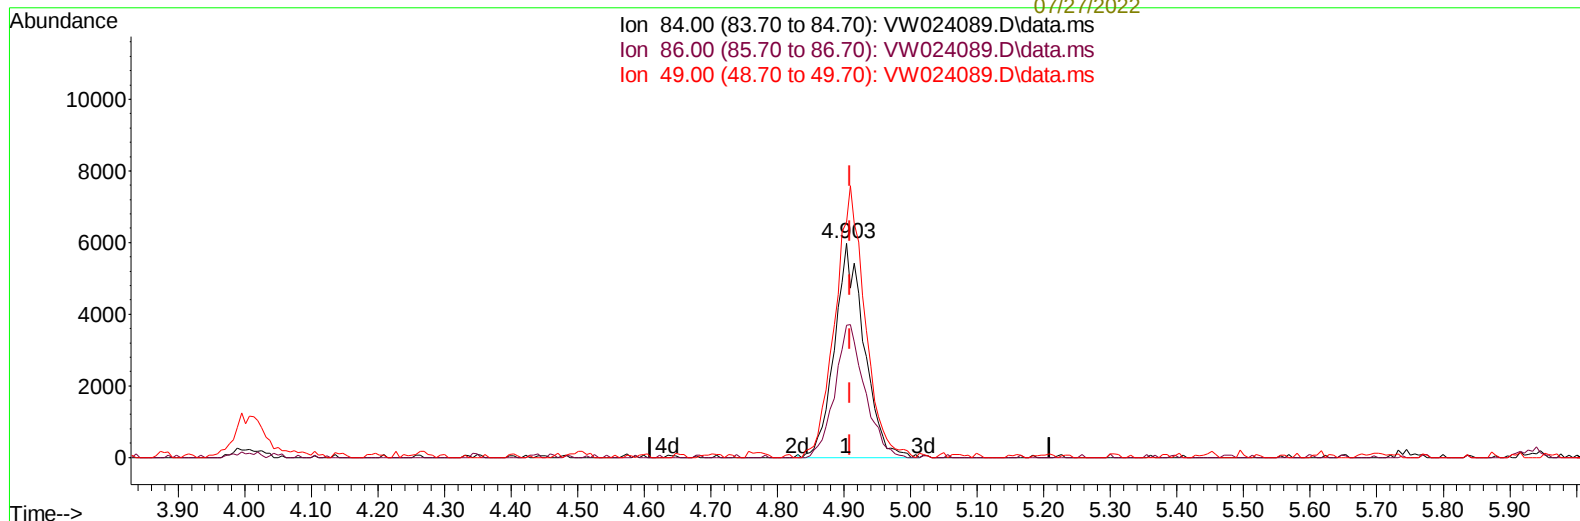

TIC: VW024089.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.006) 5.21 ug/L m

response 18479

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	61.72
49.00	119.50	109.98
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024089.D
 Acq On : 26 Jul 2022 10:06
 Operator : SY/VA
 Sample : N3795-06
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Supervised By :Mahesh
 Dadoda
 07/27/2022

Quant Time: Jul 26 23:40:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	232973	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	234247	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	102283	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	131030	26.239	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	104.960%	
7) Chloroethane-d5	2.873	69	73473	21.775	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.120%	
11) 1,1-Dichloroethene-d2	4.007	63	77764	17.685	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	70.760%	
21) 2-Butanone-d5	7.074	46	33767	38.047	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	76.100%	
24) Chloroform-d	7.641	84	143429	22.394	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	89.560%	
26) 1,2-Dichloroethane-d4	8.299	65	83747	22.759	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	91.040%	
32) Benzene-d6	8.269	84	277505	25.503	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	102.000%	
36) 1,2-Dichloropropane-d6	9.275	67	81209	23.661	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	94.640%	
41) Toluene-d8	10.323	98	259819	23.875	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	95.520%	
43) trans-1,3-Dichloroprop...	10.573	79	33887	22.268	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.080%	
47) 2-Hexanone-d5	10.921	63	28614	39.878	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	79.760%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	73597	18.584	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	74.320%	
66) 1,2-Dichlorobenzene-d4	13.853	152	85783	25.897	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	103.600%	
Target Compounds						
16) Methylene chloride	4.903	84	18479m	5.211	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024089.D
Acq On : 26 Jul 2022 10:06
Operator : SY/VA
Sample : N3795-06
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Supervised By :Mahesh
Dadoda
07/27/2022

Quant Time: Jul 26 23:40:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

