




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024091.D
 Acq On : 26 Jul 2022 10:55
 Operator : SY/VA
 Sample : N3766-05
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:40:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

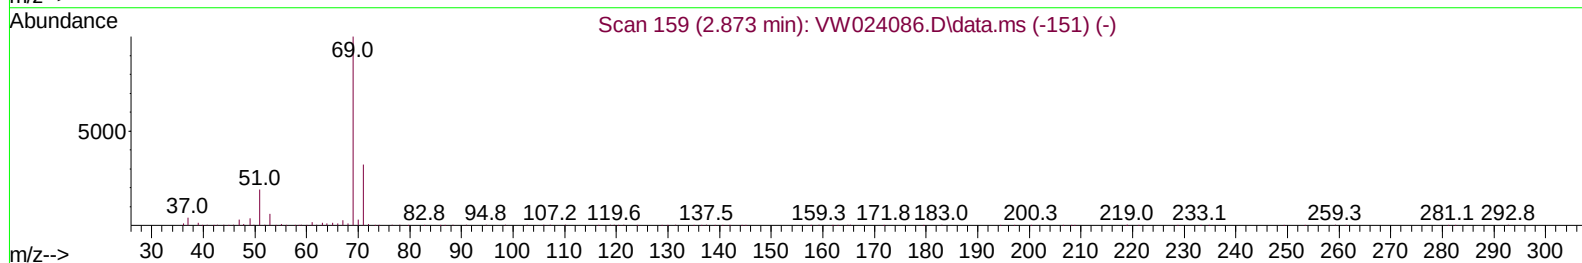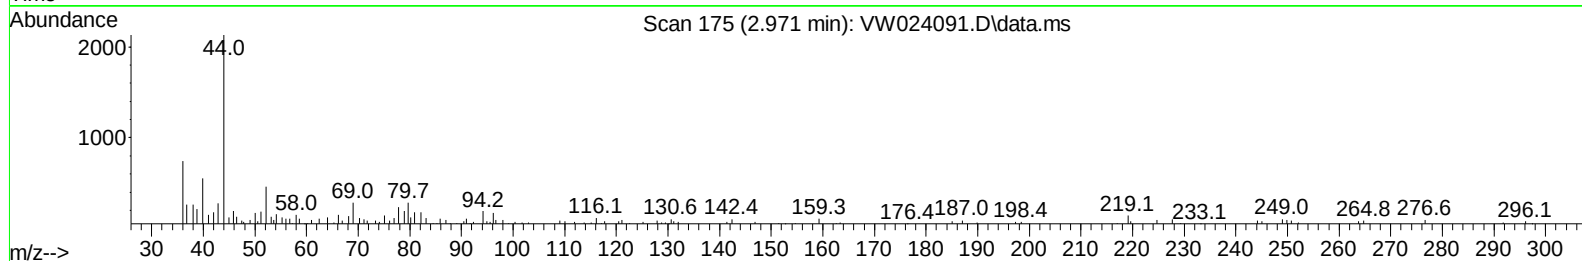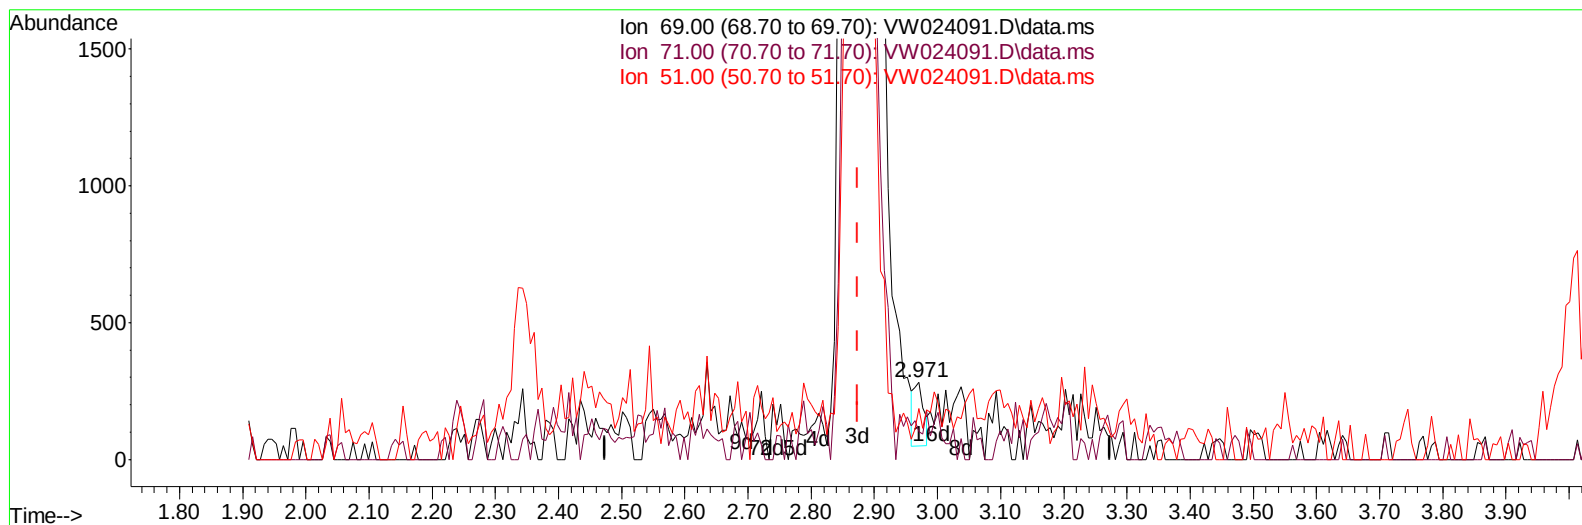

TIC: VW024091.D\data.ms

(7) Chloroethane-d5 (S)

2.971min (+ 0.098) 0.08 ug/L

response 252

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	31.75
51.00	27.90	27.78
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024091.D
Acq On : 26 Jul 2022 10:55
Operator : SY/VA
Sample : N3766-05
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:40:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

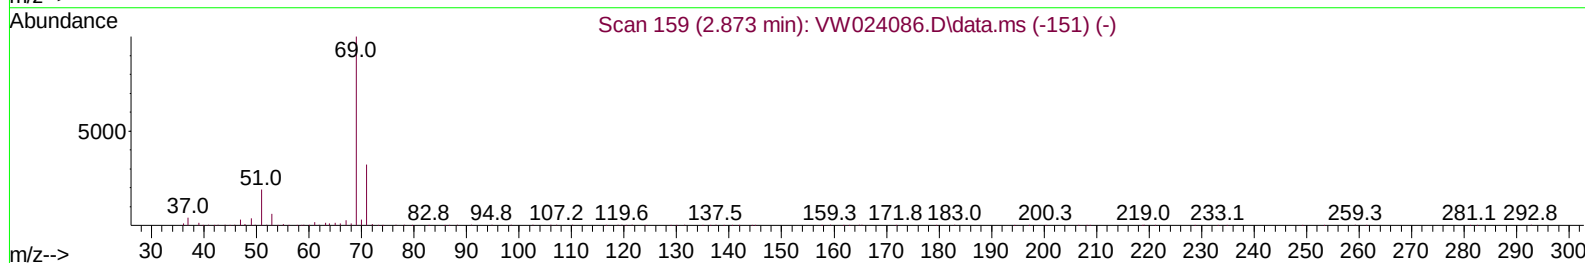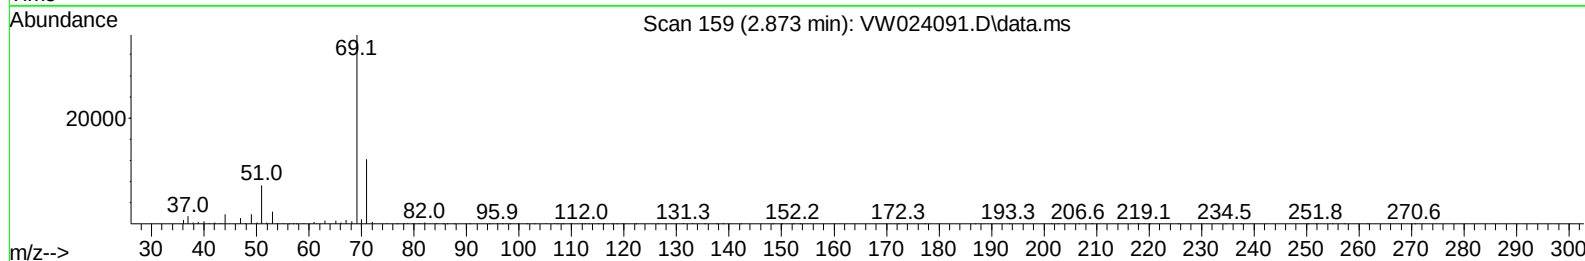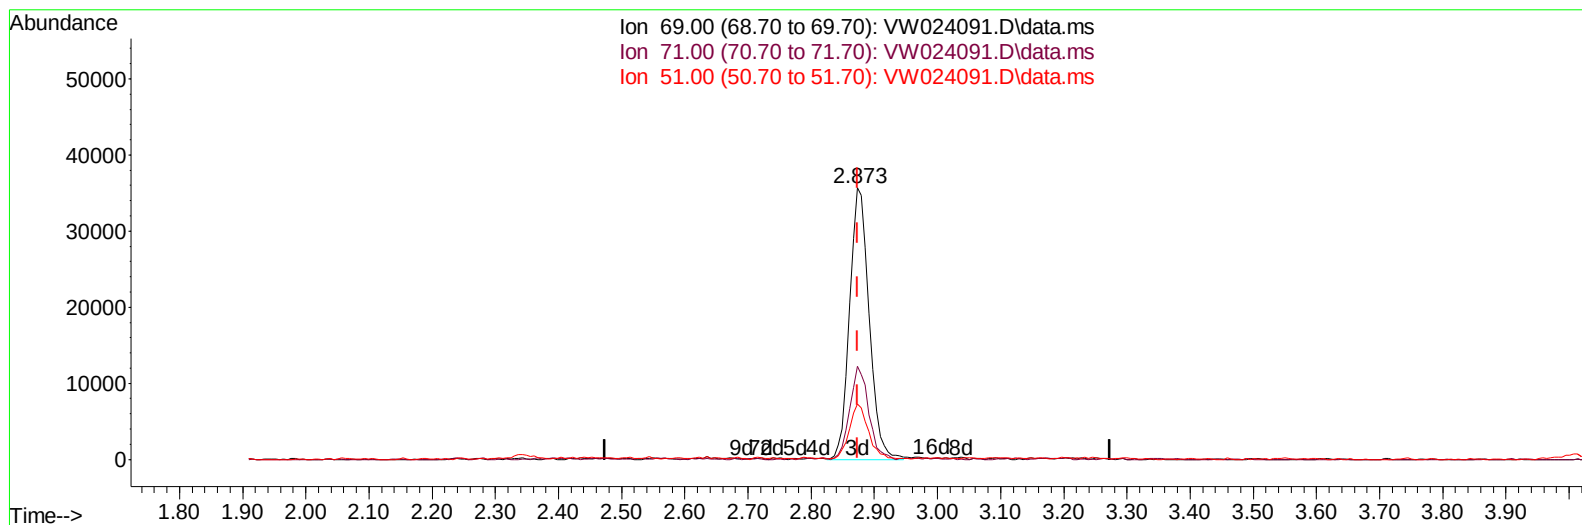

TIC: VW024091.D\data.ms

(7) Chloroethane-d5 (S)

2.873min (+ 0.000) 23.57 ug/L m

response 76960

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	0.10#
51.00	27.90	0.09#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024091.D
Acq On : 26 Jul 2022 10:55
Operator : SY/VA
Sample : N3766-05
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:40:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

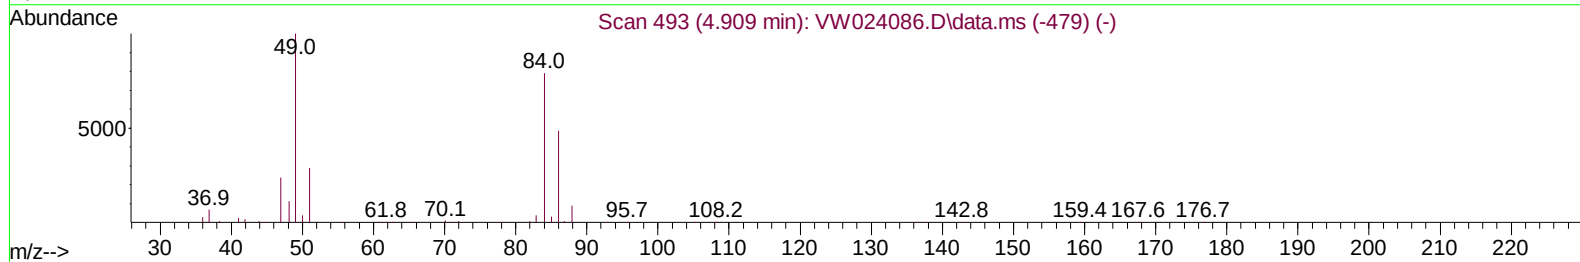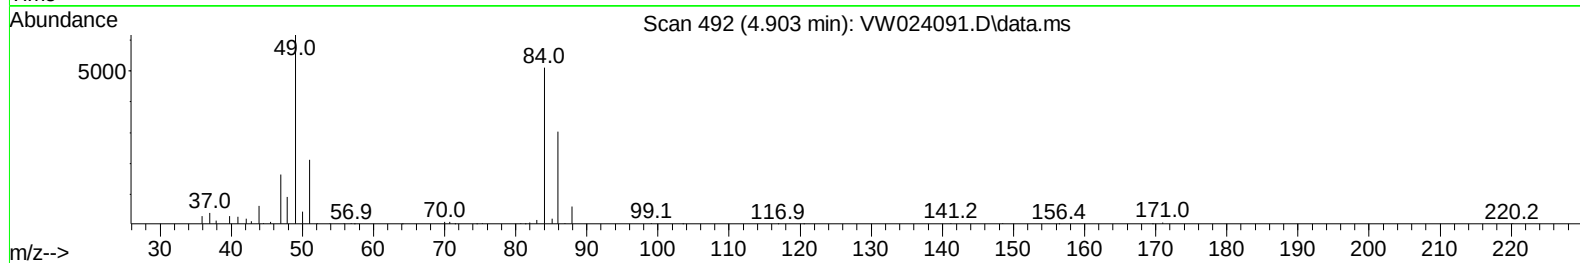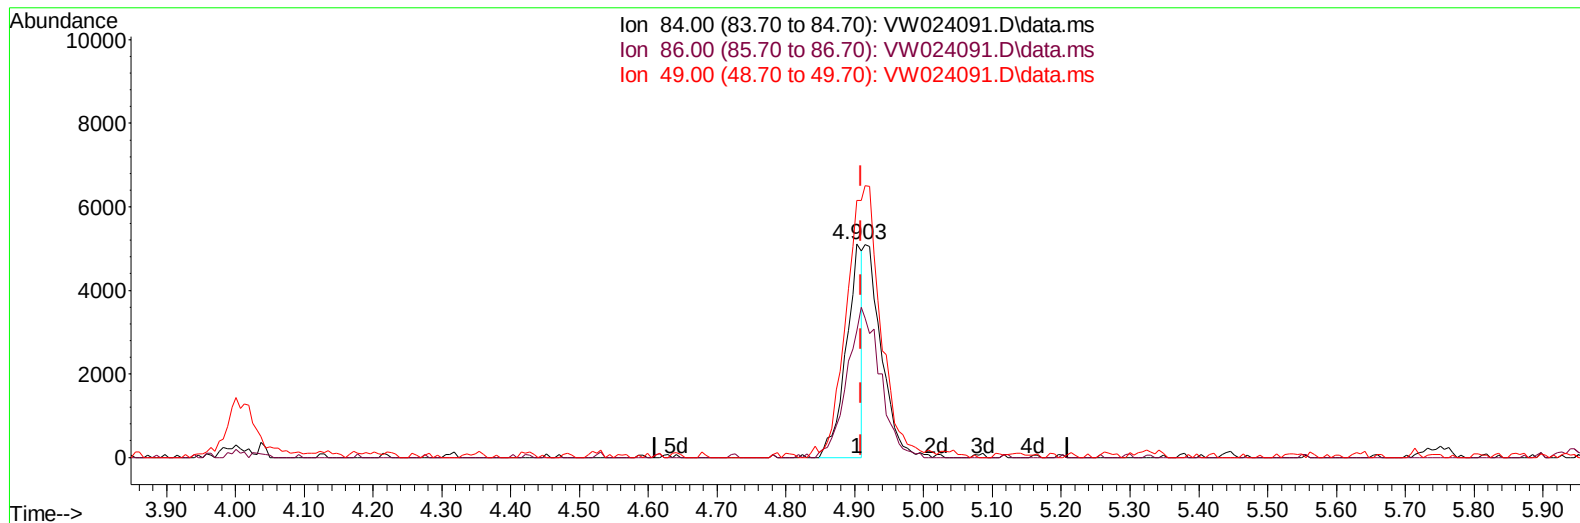

TIC: VW024091.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.006) 2.43 ug/L

response 8343

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	59.15
49.00	119.50	120.51
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024091.D
Acq On : 26 Jul 2022 10:55
Operator : SY/VA
Sample : N3766-05
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:40:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

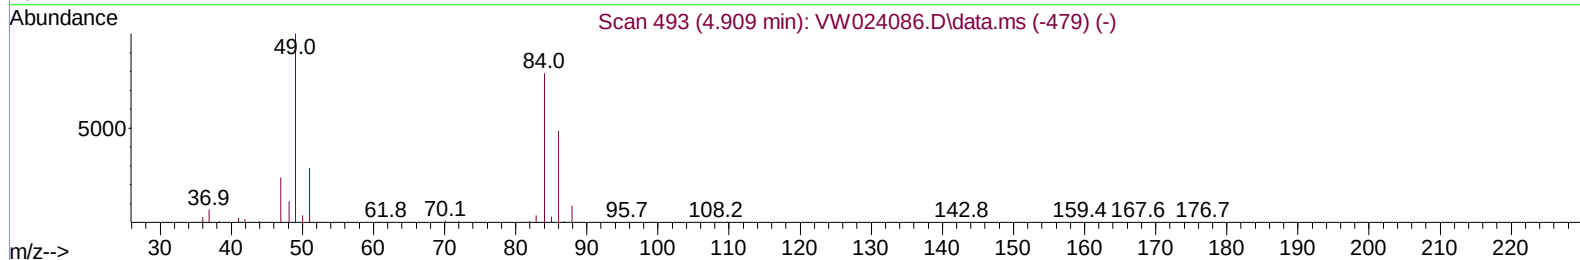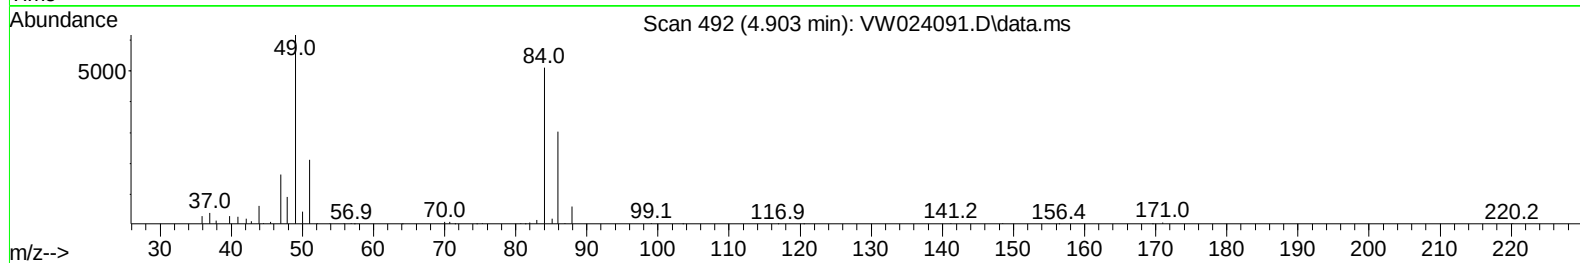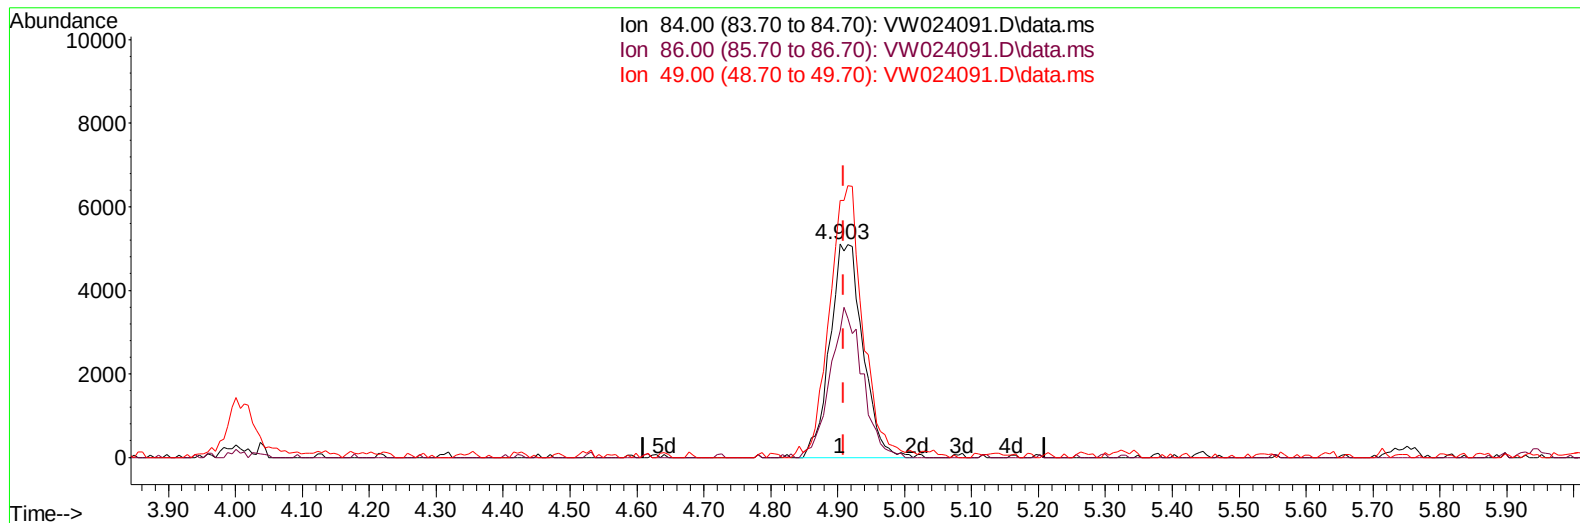

TIC: VW024091.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.006) 5.07 ug/L m

response 17413

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	59.15
49.00	119.50	120.51
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024091.D
 Acq On : 26 Jul 2022 10:55
 Operator : SY/VA
 Sample : N3766-05
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:40:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		225450	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		236623	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		103191	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		124680	25.800	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.200%	
7) Chloroethane-d5	2.873	69		76960m	23.570	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.280%	
11) 1,1-Dichloroethene-d2	4.007	63		72606	17.063	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.240%	
21) 2-Butanone-d5	7.074	46		39283	45.739	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.480%	
24) Chloroform-d	7.647	84		134594	21.715	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.880%	
26) 1,2-Dichloroethane-d4	8.305	65		81100	22.775	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.080%	
32) Benzene-d6	8.269	84		264024	24.020	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.080%	
36) 1,2-Dichloropropane-d6	9.274	67		76273	22.000	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.000%	
41) Toluene-d8	10.323	98		243821	22.180	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.720%	
43) trans-1,3-Dichloroprop...	10.579	79		32268	20.991	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.960%	
47) 2-Hexanone-d5	10.920	63		31030	42.811	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.620%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		76268	19.065	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.280%	
66) 1,2-Dichlorobenzene-d4	13.853	152		83420	24.962	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.840%	
Target Compounds							
16) Methylene chloride	4.903	84		17413m	5.075	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024091.D
Acq On : 26 Jul 2022 10:55
Operator : SY/VA
Sample : N3766-05
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:40:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

