




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024096.D
Acq On : 26 Jul 2022 12:57
Operator : SY/VA
Sample : N3790-12RE
Misc : 4.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:41:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

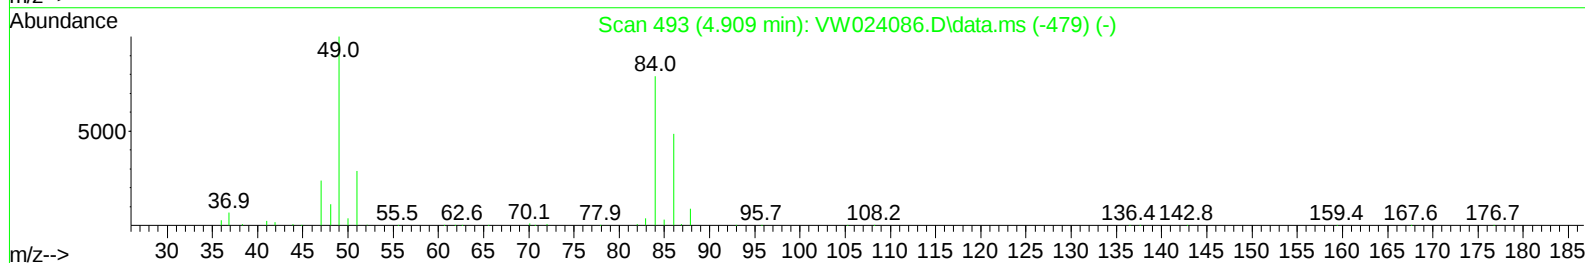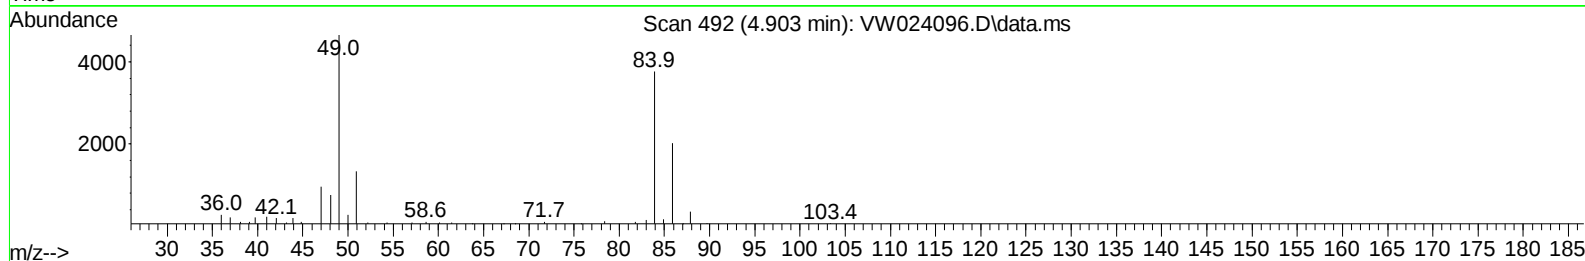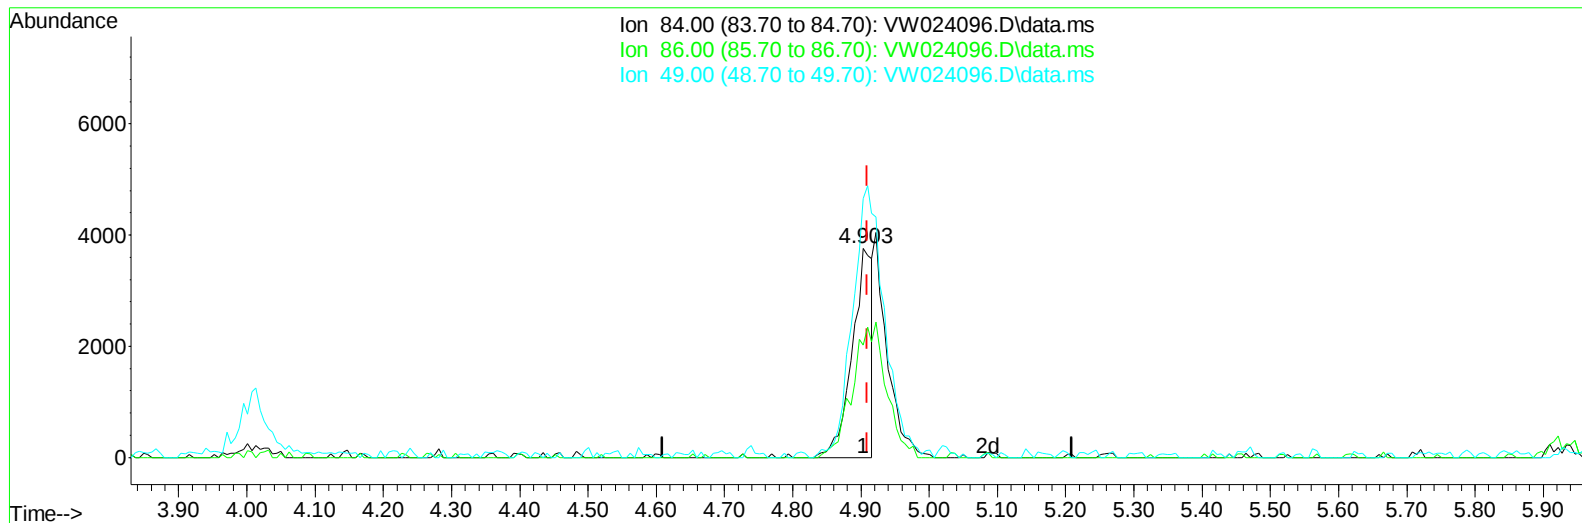

TIC: VW024096.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.006) 2.37 ug/L

response 7659

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	53.85
49.00	119.50	123.74
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024096.D
Acq On : 26 Jul 2022 12:57
Operator : SY/VA
Sample : N3790-12RE
Misc : 4.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:41:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

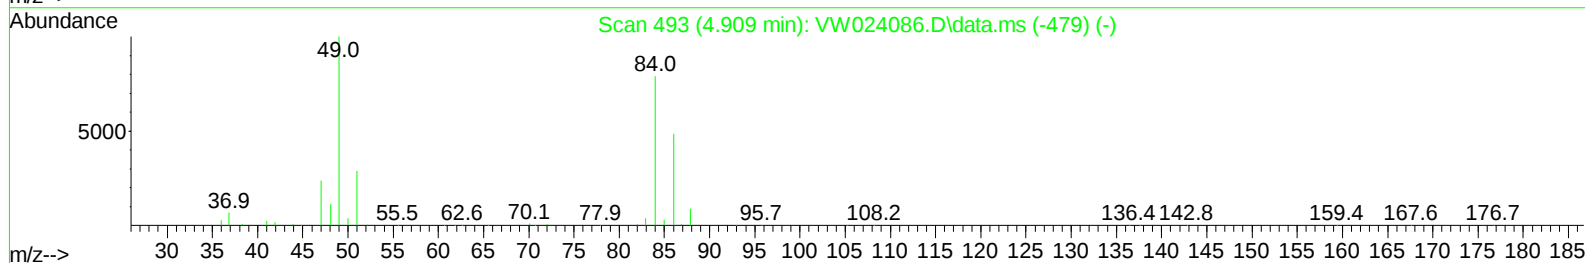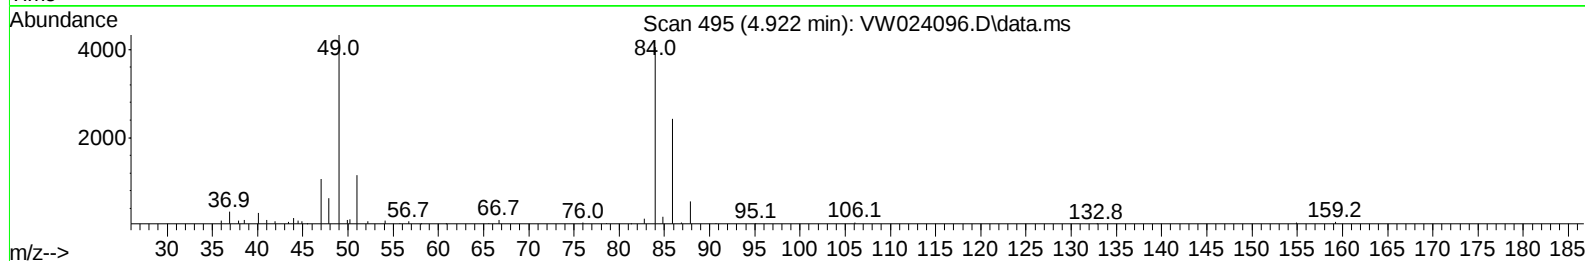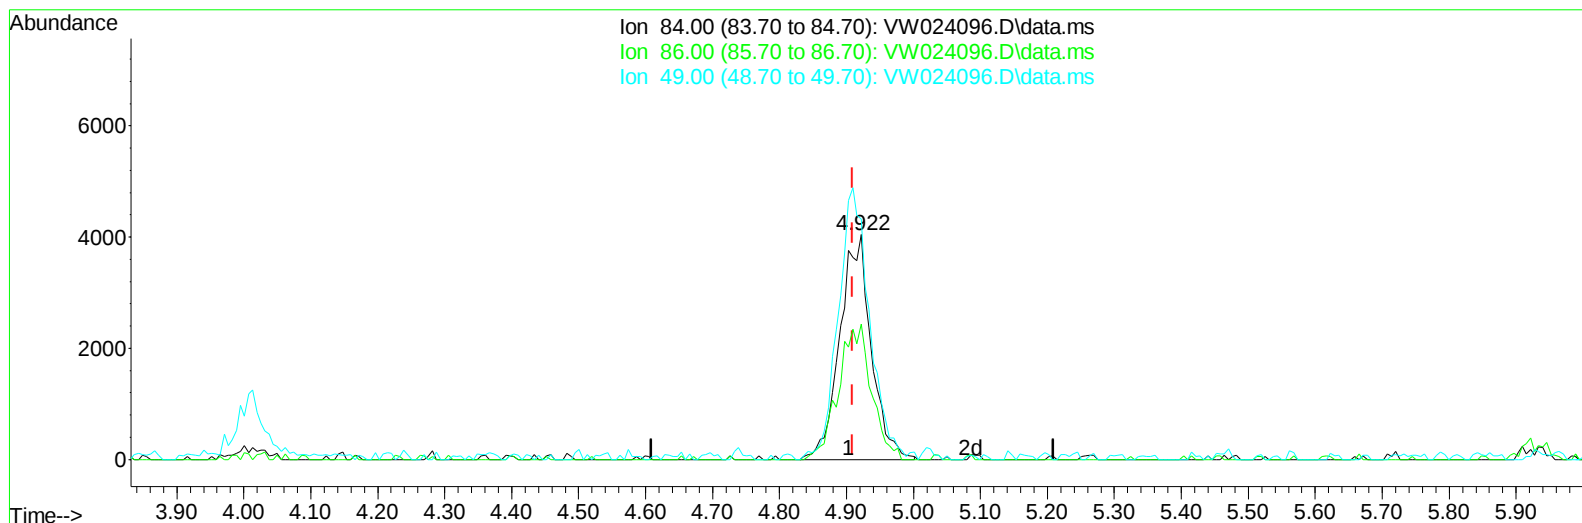

TIC: VW024096.D\data.ms

(16) Methylene chloride (T)

4.922min (+ 0.012) 4.05 ug/L m

response 13087

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	60.14
49.00	119.50	106.89
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024096.D
Acq On : 26 Jul 2022 12:57
Operator : SY/VA
Sample : N3790-12RE
Misc : 4.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:41:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

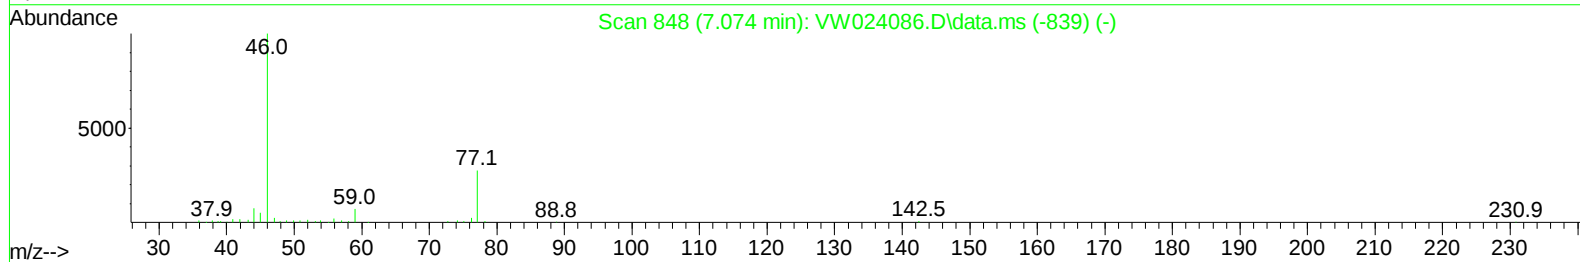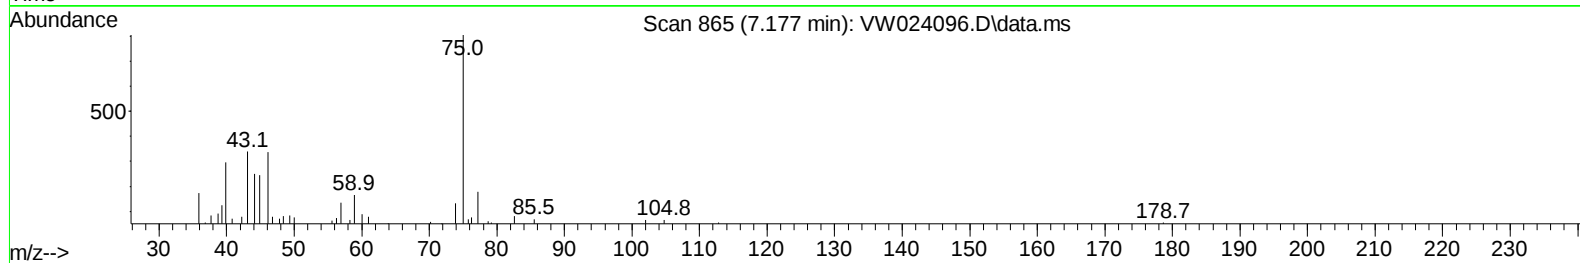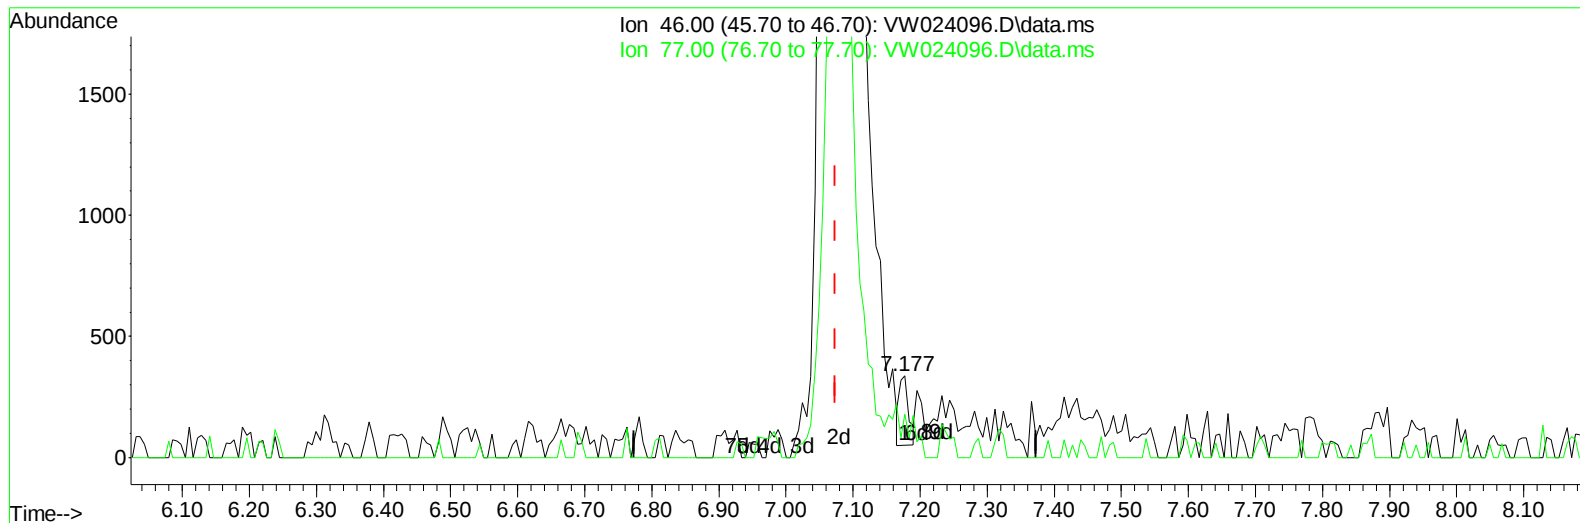

TIC: VW024096.D\data.ms

(21) 2-Butanone-d5 (S)

7.177min (+ 0.104) 0.33 ug/L

response 270

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.90	19.26
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024096.D
Acq On : 26 Jul 2022 12:57
Operator : SY/VA
Sample : N3790-12RE
Misc : 4.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:41:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

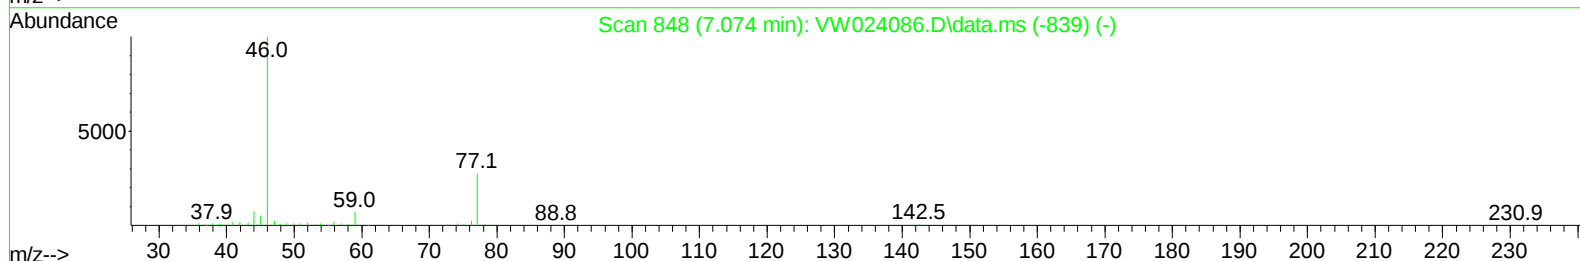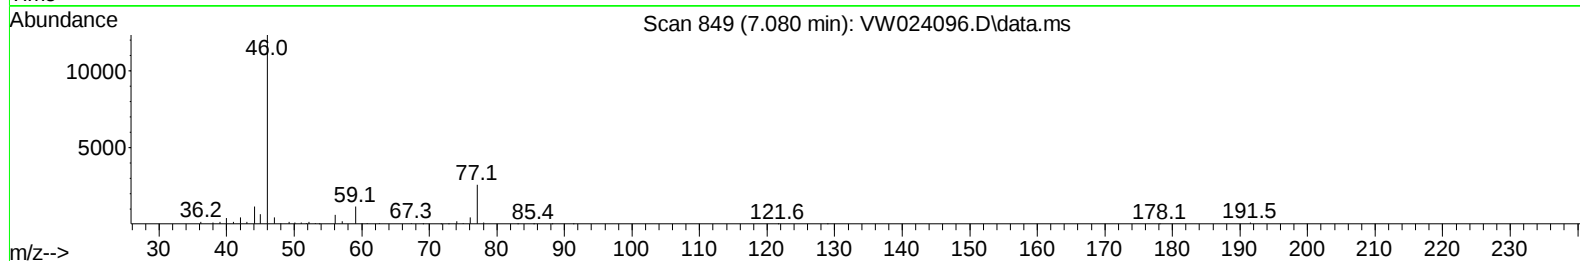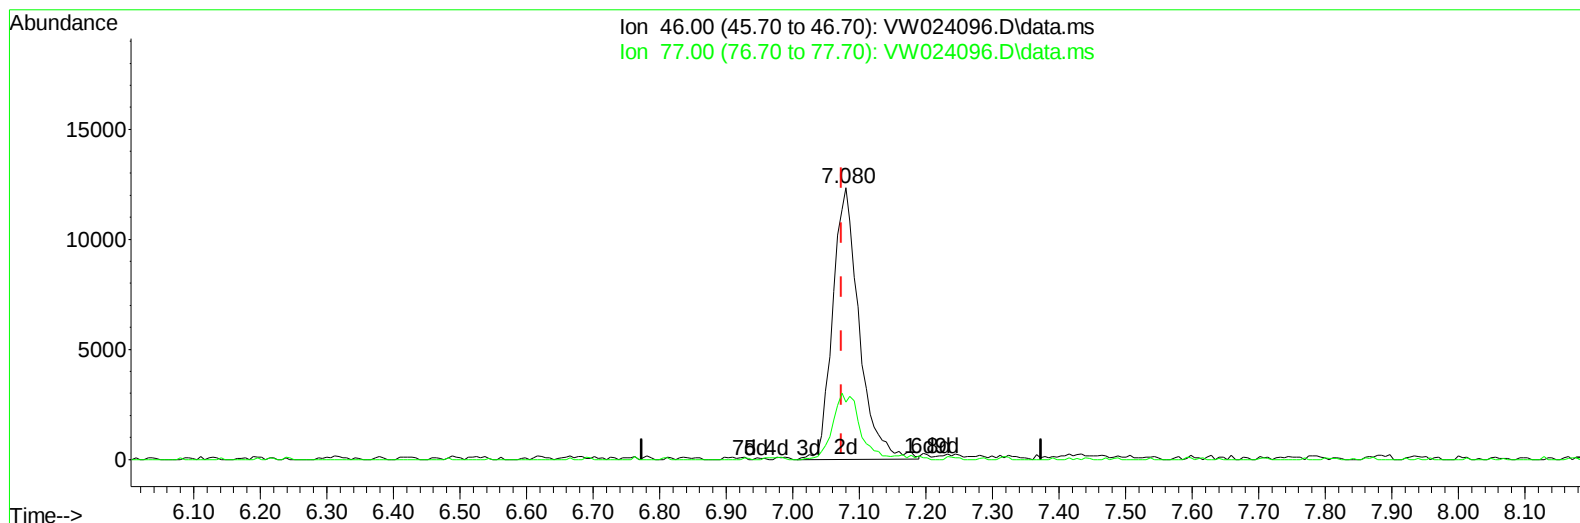

TIC: VW024096.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 42.18 ug/L m

response 34108

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.90	0.15#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024096.D
 Acq On : 26 Jul 2022 12:57
 Operator : SY/VA
 Sample : N3790-12RE
 Misc : 4.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:41:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		212256	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		164108	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		47187	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		125968	27.687	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	110.760%	
7) Chloroethane-d5	2.873	69		95132	30.946	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	123.800%	
11) 1,1-Dichloroethene-d2	4.013	63		64156	16.014	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	64.040%	
21) 2-Butanone-d5	7.080	46		34108m	42.182	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	84.360%	
24) Chloroform-d	7.647	84		156049	26.742	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	106.960%	
26) 1,2-Dichloroethane-d4	8.305	65		100447	29.961	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	119.840%	
32) Benzene-d6	8.275	84		200312	26.276	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	105.120%	
36) 1,2-Dichloropropane-d6	9.268	67		88688	36.884	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	147.520%#	
41) Toluene-d8	10.323	98		156930	20.584	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	82.320%	
43) trans-1,3-Dichloroprop...	10.579	79		15958	14.968	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	59.880%	
47) 2-Hexanone-d5	10.927	63		8912	17.729	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	35.460%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		82887	29.875	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	119.520%	
66) 1,2-Dichlorobenzene-d4	13.853	152		40281	26.359	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	105.440%	
Target Compounds							
13) Acetone	4.123	43		2351	4.097	ug/L	76
16) Methylene chloride	4.922	84		13087m	4.051	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024096.D
Acq On : 26 Jul 2022 12:57
Operator : SY/VA
Sample : N3790-12RE
Misc : 4.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:41:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

