




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024098.D
Acq On : 26 Jul 2022 13:46
Operator : SY/VA
Sample : N3790-14RE
Misc : 3.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK8RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:42:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

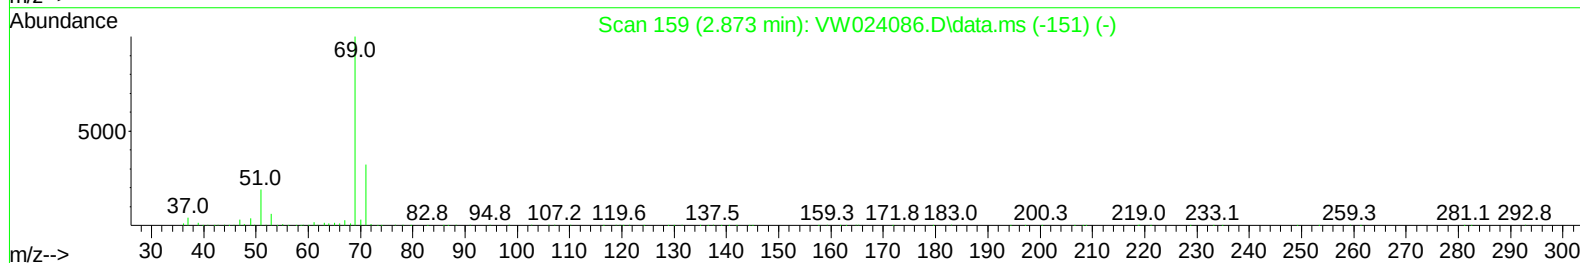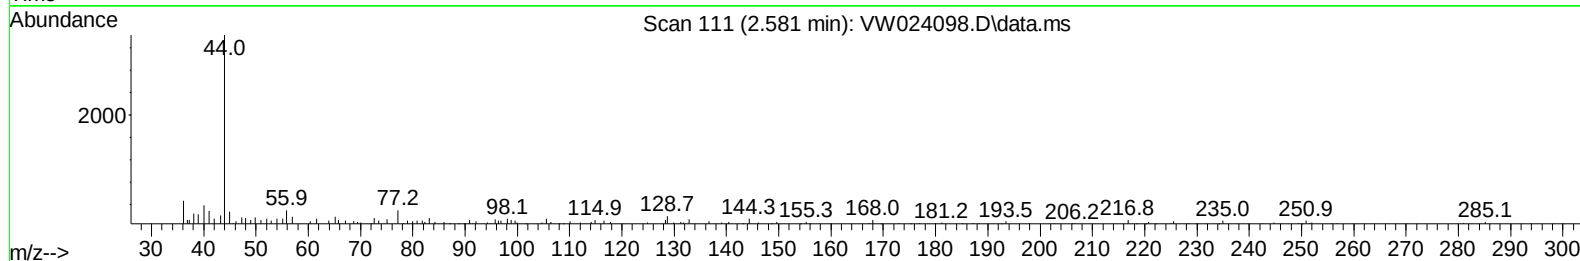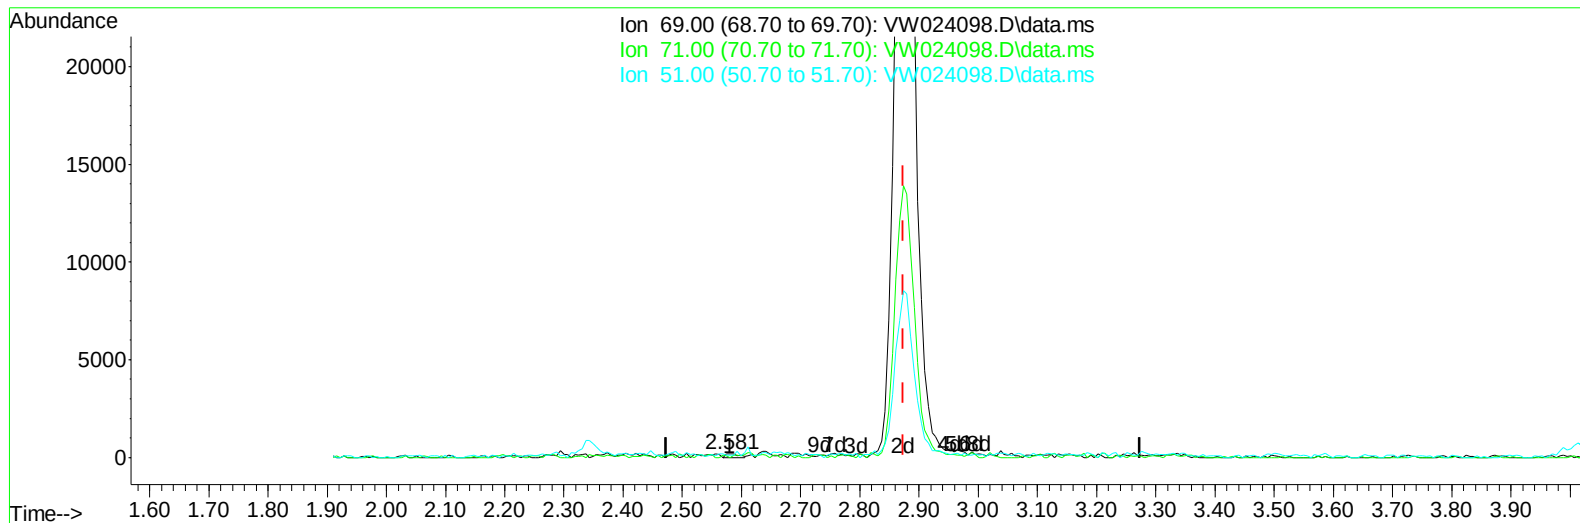

TIC: VW024098.D\data.ms

(7) Chloroethane-d5 (S)

2.581min (-0.292) 0.09 ug/L

response 280

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	41.07
51.00	27.90	31.43
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024098.D
Acq On : 26 Jul 2022 13:46
Operator : SY/VA
Sample : N3790-14RE
Misc : 3.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK8RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:42:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

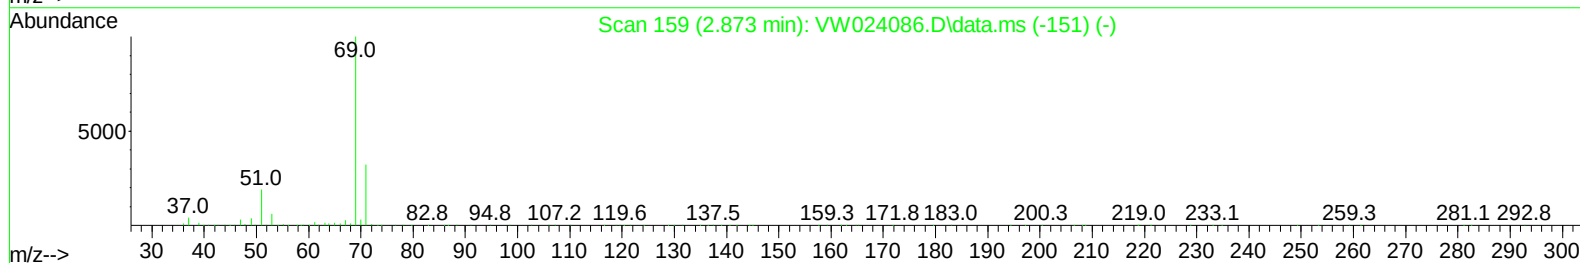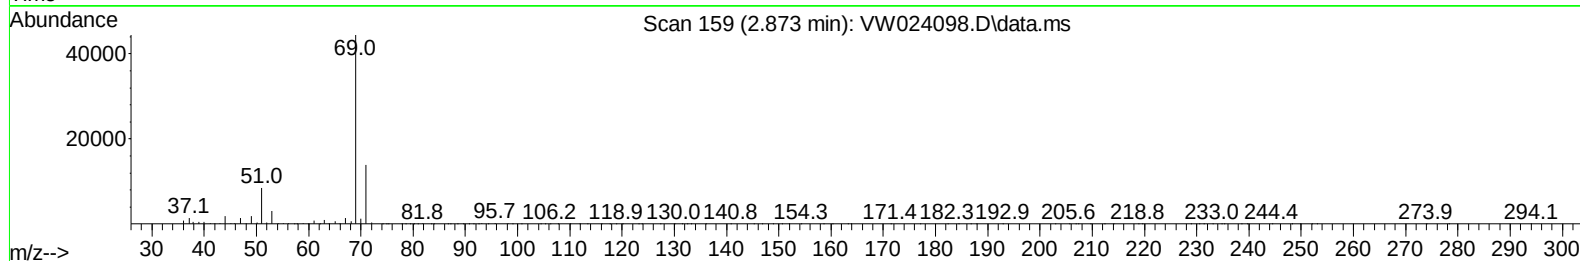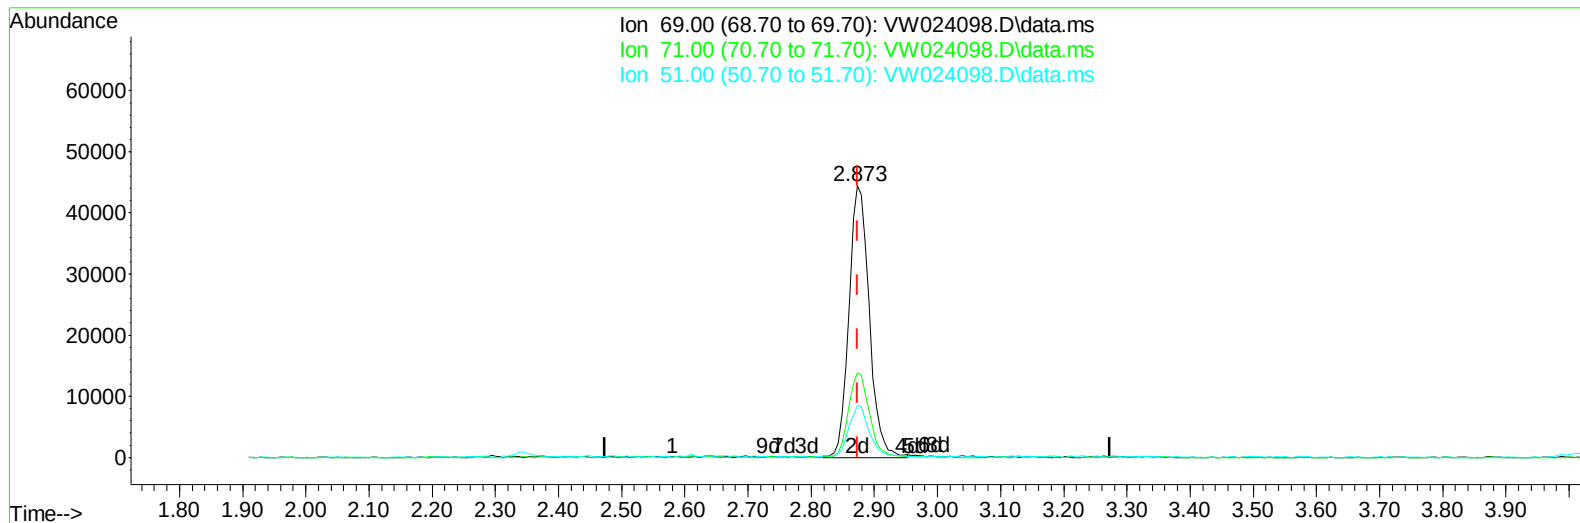

TIC: VW024098.D\data.ms

(7) Chloroethane-d5 (S)

2.873min (+ 0.000) 33.05 ug/L m

response 99426

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	0.12#
51.00	27.90	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024098.D
 Acq On : 26 Jul 2022 13:46
 Operator : SY/VA
 Sample : N3790-14RE
 Misc : 3.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK8RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:42:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound		R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards								
1) 1,4-Difluorobenzene		8.842	114		207695	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117		131498	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152		31188	25.000	ug/L	0.00
System Monitoring Compounds								
4) Vinyl Chloride-d3		2.343	65		127625	28.667	ug/L	0.00
Spiked Amount	25.000	Range	30	- 150	Recovery	=	114.680%	
7) Chloroethane-d5		2.873	69		99426m	33.053	ug/L	0.00
Spiked Amount	25.000	Range	30	- 150	Recovery	=	132.200%	
11) 1,1-Dichloroethene-d2		4.007	63		59037	15.060	ug/L	0.00
Spiked Amount	25.000	Range	45	- 110	Recovery	=	60.240%	
21) 2-Butanone-d5		7.080	46		9043	11.429	ug/L	0.00
Spiked Amount	50.000	Range	20	- 135	Recovery	=	22.860%	
24) Chloroform-d		7.647	84		148944	26.085	ug/L	0.00
Spiked Amount	25.000	Range	40	- 150	Recovery	=	104.360%	
26) 1,2-Dichloroethane-d4		8.305	65		88556	26.995	ug/L	0.00
Spiked Amount	25.000	Range	70	- 130	Recovery	=	107.960%	
32) Benzene-d6		8.275	84		214941	35.187	ug/L	0.00
Spiked Amount	25.000	Range	20	- 135	Recovery	=	140.760%#	
36) 1,2-Dichloropropane-d6		9.275	67		79976	41.509	ug/L	0.00
Spiked Amount	25.000	Range	70	- 120	Recovery	=	166.040%#	
41) Toluene-d8		10.323	98		158920	26.014	ug/L	0.00
Spiked Amount	25.000	Range	30	- 130	Recovery	=	104.040%	
43) trans-1,3-Dichloroprop...		10.573	79		5321	6.229	ug/L	0.00
Spiked Amount	25.000	Range	30	- 135	Recovery	=	24.920%#	
47) 2-Hexanone-d5		10.927	63		1669	4.143	ug/L	0.00
Spiked Amount	50.000	Range	20	- 135	Recovery	=	8.280%#	
56) 1,1,2,2-Tetrachloroeth...		12.689	84		52640	23.678	ug/L	0.00
Spiked Amount	25.000	Range	45	- 120	Recovery	=	94.720%	
66) 1,2-Dichlorobenzene-d4		13.853	152		23246	23.015	ug/L	0.00
Spiked Amount	25.000	Range	75	- 120	Recovery	=	92.040%	
Target Compounds								
13) Acetone		4.129	43		10710	19.075	ug/L	Qvalue 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024098.D
Acq On : 26 Jul 2022 13:46
Operator : SY/VA
Sample : N3790-14RE
Misc : 3.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK8RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:42:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

