

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024088.D
 Acq On : 26 Jul 2022 09:05
 Operator : SY/VA
 Sample : N3790-02
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUJ7

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:40:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Supervised By :Mahesh
 Dadoda
 07/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	226089	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	236753	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	125556	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	123990	25.585	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 102.320%			
7) Chloroethane-d5	2.873	69	86652m	26.463	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 105.840%			
11) 1,1-Dichloroethene-d2	4.013	63	104885	24.579	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 98.320%			
21) 2-Butanone-d5	7.074	46	31531	36.609	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 73.220%			
24) Chloroform-d	7.647	84	138016	22.205	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 88.800%			
26) 1,2-Dichloroethane-d4	8.305	65	80514m	22.546	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 90.200%			
32) Benzene-d6	8.269	84	268063	24.374	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 97.480%			
36) 1,2-Dichloropropane-d6	9.274	67	78641	22.670	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 90.680%			
41) Toluene-d8	10.323	98	251653	22.880	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 91.520%			
43) trans-1,3-Dichloroprop...	10.573	79	35824	23.292	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 93.160%			
47) 2-Hexanone-d5	10.921	63	30216	41.665	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 83.320%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	78733	19.671	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 78.680%			
66) 1,2-Dichlorobenzene-d4	13.847	152	92912	22.850	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 91.400%			
Target Compounds						Qvalue
3) Chloromethane	2.215	50	82338	18.993	ug/L	98
6) Bromomethane	2.770	94	36825	9.865	ug/L	100
9) Trichlorofluoromethane	3.245	101	59075	18.781	ug/L	99
12) 1,1-Dichloroethene	4.025	96	52736	22.086	ug/L	94
13) Acetone	4.123	43	33341	54.552	ug/L	100
15) Methyl Acetate	4.659	43	47056	31.916	ug/L	96
16) Methylene chloride	4.903	84	37538	10.908	ug/L	94
17) trans-1,2-Dichloroethene	5.422	96	32481	11.118	ug/L	98
18) Methyl tert-butyl Ether	5.428	73	138368	31.951	ug/L #	88
20) cis-1,2-Dichloroethene	7.165	96	84399	26.308	ug/L	96
23) Bromochloromethane	7.507	128	23549	14.264	ug/L	93
27) 1,2-Dichloroethane	8.397	62	43551	9.576	ug/L	96
29) Cyclohexane	7.952	56	43648	10.006	ug/L	100
30) 1,1,1-Trichloroethane	7.872	97	53664	10.141	ug/L	99
31) Carbon tetrachloride	8.067	117	62929	12.900	ug/L	96
34) Trichloroethene	9.085	95	144725	39.960	ug/L	97
35) Methylcyclohexane	9.329	83	153838	27.959	ug/L	98
37) 1,2-Dichloropropane	9.366	63	44252	12.798	ug/L	99
38) Bromodichloromethane	9.640	83	98071	19.893	ug/L	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024088.D
 Acq On : 26 Jul 2022 09:05
 Operator : SY/VA
 Sample : N3790-02
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUJ7

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:40:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Supervised By :Mahesh
 Dadoda
 07/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

39) cis-1,3-Dichloropropene	10.067	75	79854	15.851	ug/L	100
42) Toluene	10.384	91	324838	20.997	ug/L	95
44) trans-1,3-Dichloropropene	10.604	75	35446	7.430	ug/L	93
46) Tetrachloroethene	10.860	164	111878	39.468	ug/L	88
48) 2-Hexanone	10.969	43	45162	25.901	ug/L	99
49) Dibromochloromethane	11.128	129	66794	18.924	ug/L	93
52) Ethylbenzene	11.725	91	270477	15.865	ug/L	99
53) m,p-Xylene	11.841	106	68759	10.390	ug/L	94
54) o-Xylene	12.164	106	77024	12.171	ug/L	93
60) Isopropylbenzene	12.463	105	211275	13.285	ug/L	98
64) 1,3-Dichlorobenzene	13.493	146	148377	19.507	ug/L	96
67) 1,2-Dichlorobenzene	13.865	146	72272	10.158	ug/L	96
68) 1,2-Dibromo-3-chloropr...	14.481	75	10083	15.990	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024088.D
Acq On : 26 Jul 2022 09:05
Operator : SY/VA
Sample : N3790-02
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBUJ7


Quant Time: Jul 26 23:40:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 07/27/2022
Supervised By : Mahesh Dadoda 07/27/2022


Supervised By : Mahesh
Dadoda
07/27/2022

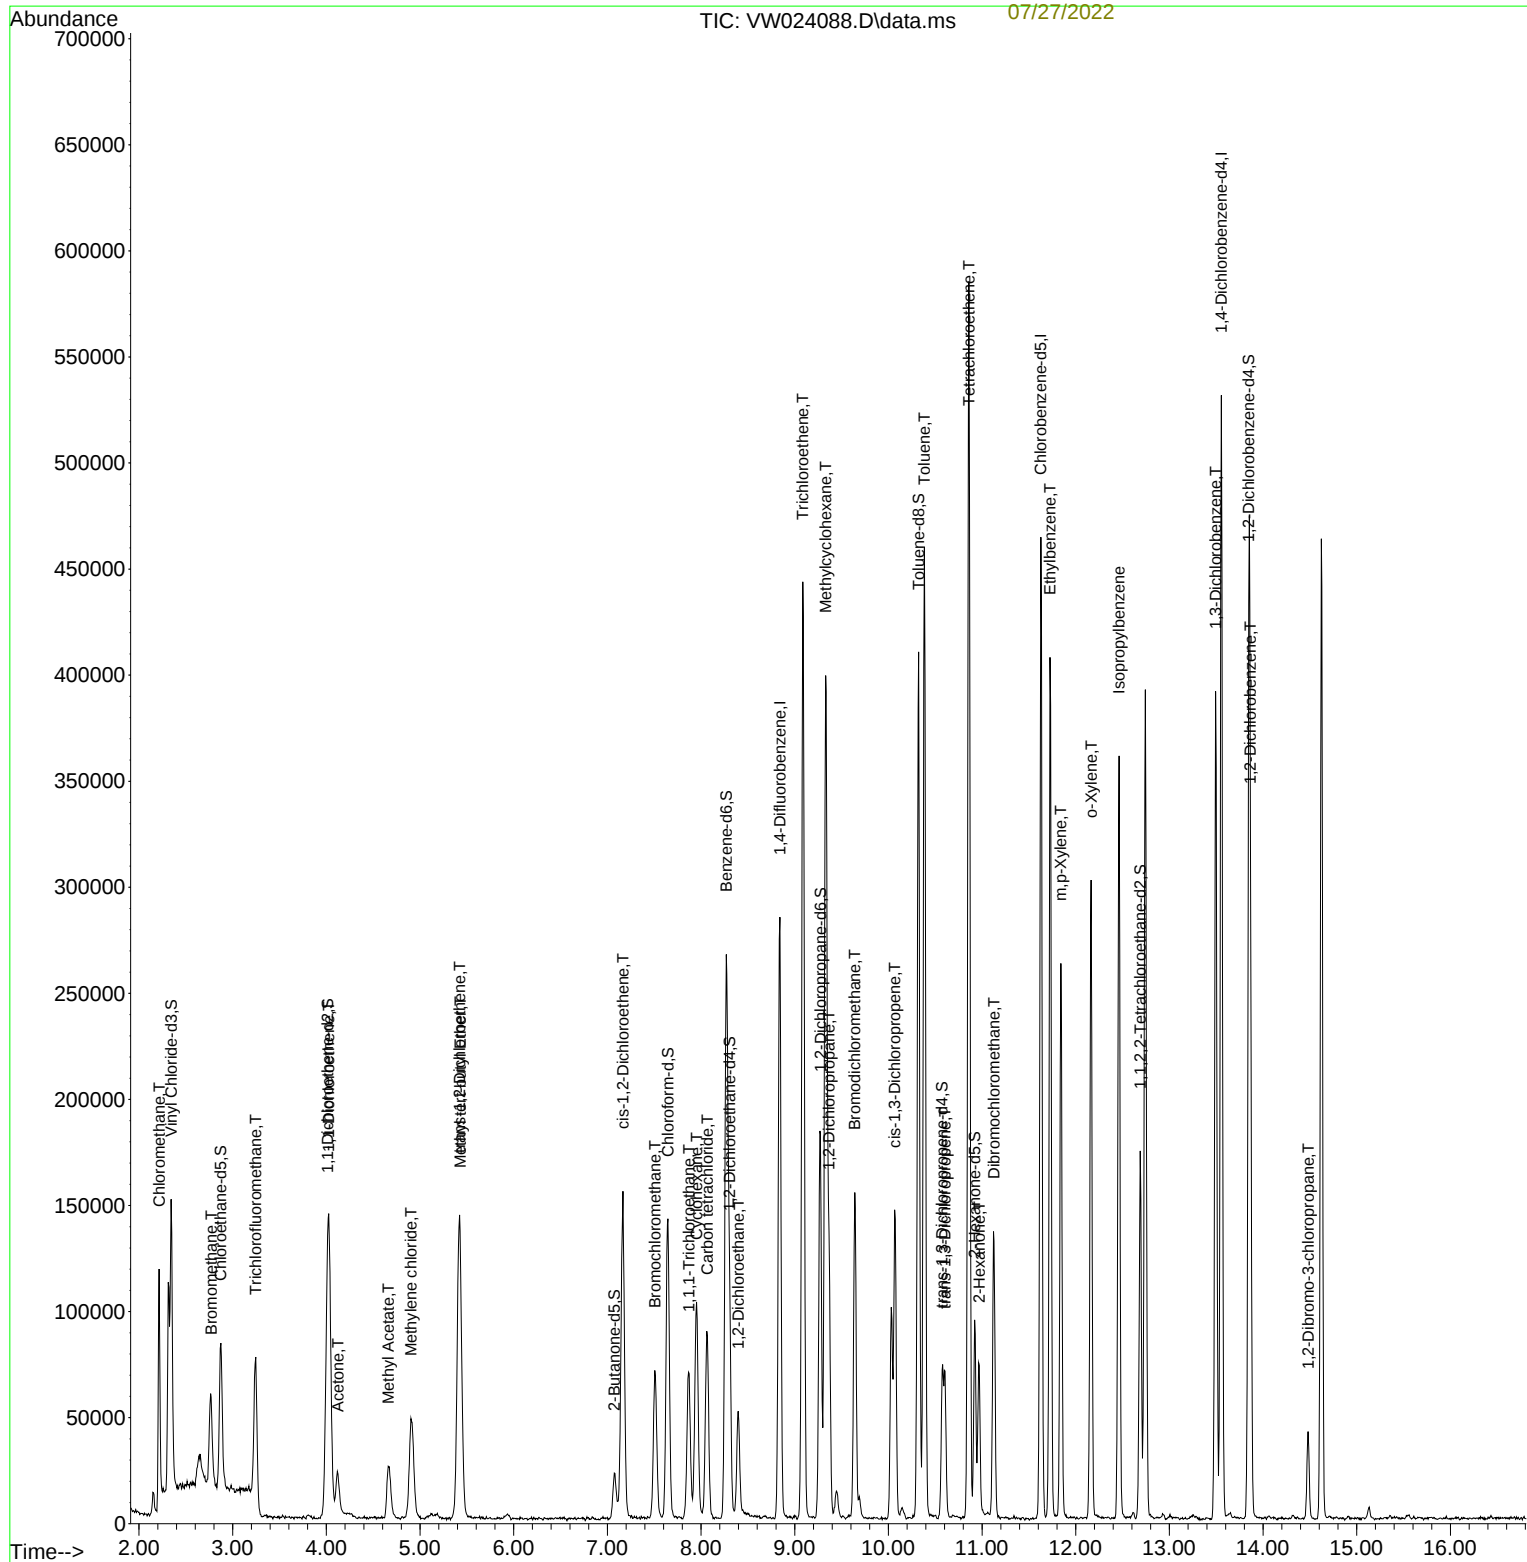



#3
Chloromethane
Concen: 18.993 ug/L
RT: 2.215 min Scan# 51
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05



Instrument :
MSVOA_W
ClientSampleId :
DBUJ7

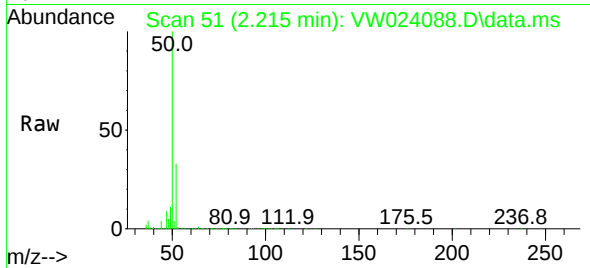


Tgt Ion: 50 Resp: 82338
Ion Ratio Lower Upper
50 100
52 33.2 23.9 44.5

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

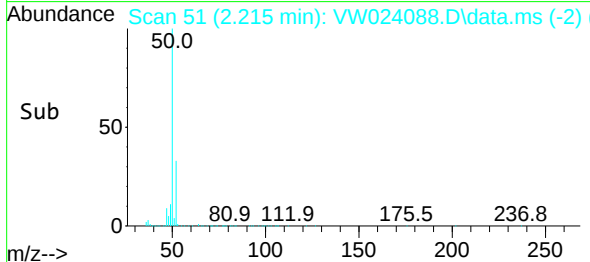



Supervised By :Mahesh
Dadoda
07/27/2022




#6
Bromomethane
Concen: 9.865 ug/L
RT: 2.770 min Scan# 142
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

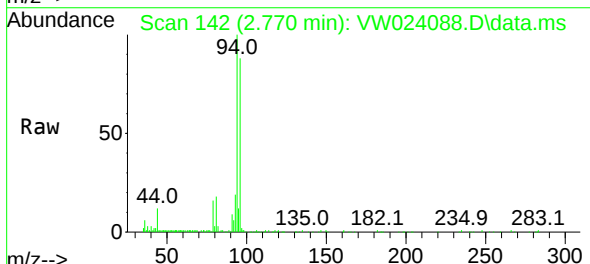


Tgt Ion: 94 Resp: 36825
Ion Ratio Lower Upper
94 100
96 88.0 61.9 114.9

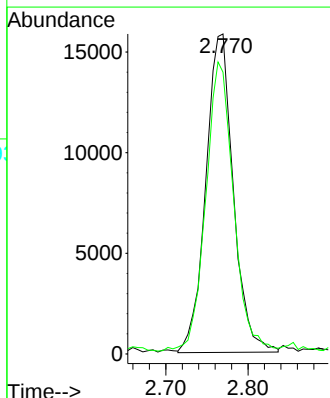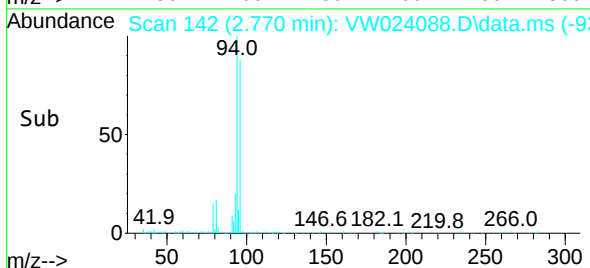



#9
Trichlorofluoromethane
Concen: 18.781 ug/L
RT: 3.245 min Scan# 219
Delta R.T. 0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7






Tgt Ion:101 Resp: 5907
Ion Ratio Lower Upper
101 100
103 65.0 52.4 78.6

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

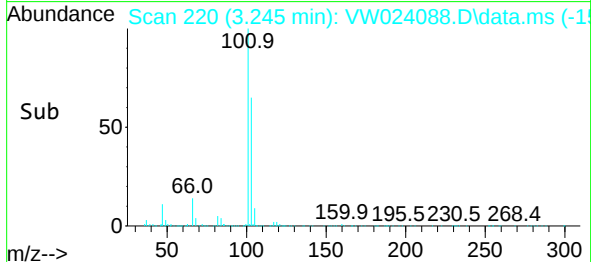

#12
1,1-Dichloroethene
Concen: 22.086 ug/L
RT: 4.025 min Scan# 348
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05


Tgt Ion: 96 Resp: 52736
Ion Ratio Lower Upper
96 100
61 184.2 128.4 238.4
63 148.7 93.1 172.9

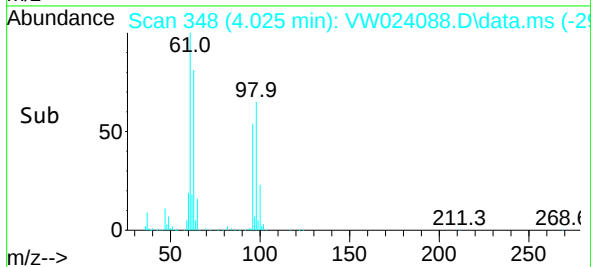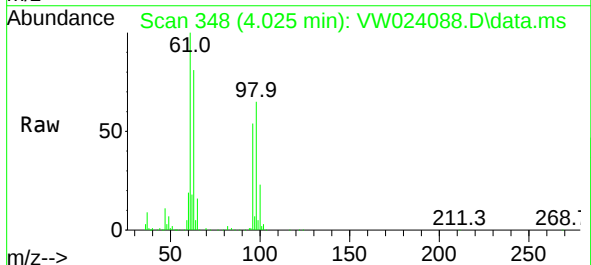



#13
Acetone
Concen: 54.552 ug/L
RT: 4.123 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05



Instrument :
MSVOA_W
ClientSampleId :
DBUJ7

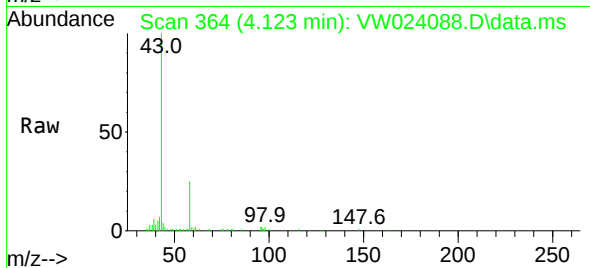


Tgt Ion: 43 Resp: 3334
Ion Ratio Lower Upper
43 100
58 29.8 0.0 60.0

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022

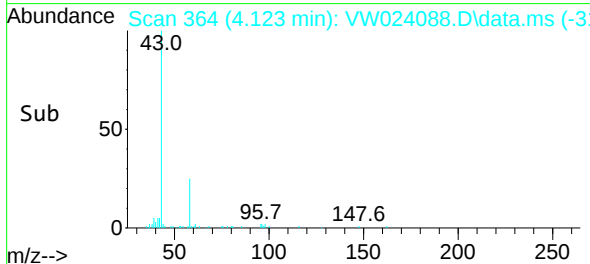



Supervised By :Mahesh
Dadoda
07/27/2022

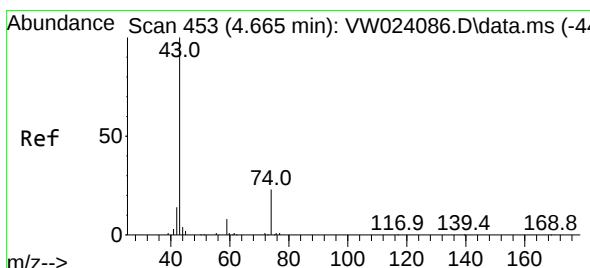


#15
Methyl Acetate
Concen: 31.916 ug/L
RT: 4.659 min Scan# 452
Delta R.T. -0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05




Tgt Ion: 43 Resp: 47056
Ion Ratio Lower Upper
43 100
74 24.5 21.1 31.7

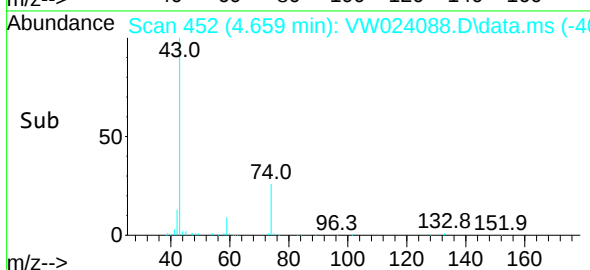



#16
Methylene chloride
Concen: 10.908 ug/L
RT: 4.903 min Scan# 493
Delta R.T. -0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05



Instrument :
MSVOA_W
ClientSampleId :
DBUJ7

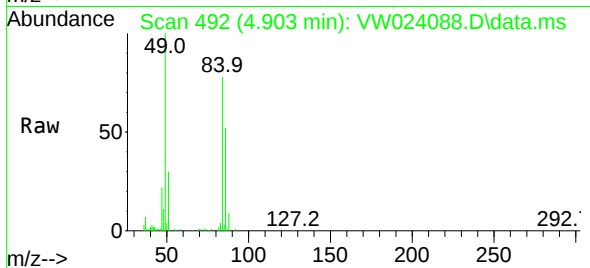


Tgt Ion: 84 Resp: 37538
Ion Ratio Lower Upper
84 100
86 66.3 44.7 83.1
49 128.6 83.7 155.4

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022







Supervised By :Mahesh
Dadoda
07/27/2022

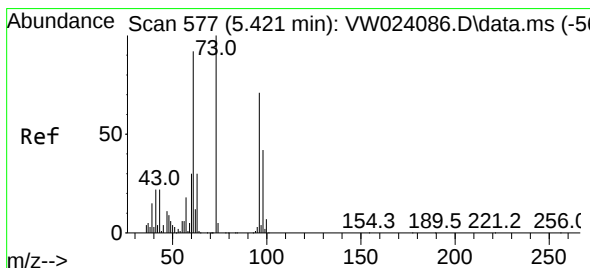

#17
trans-1,2-Dichloroethene
Concen: 11.118 ug/L
RT: 5.422 min Scan# 577
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05


Tgt Ion: 96 Resp: 32481
Ion Ratio Lower Upper
96 100
61 135.5 92.7 172.1
98 64.4 44.1 81.9

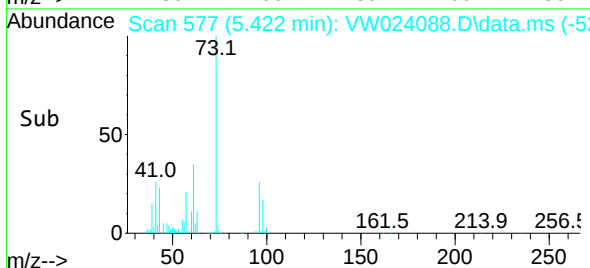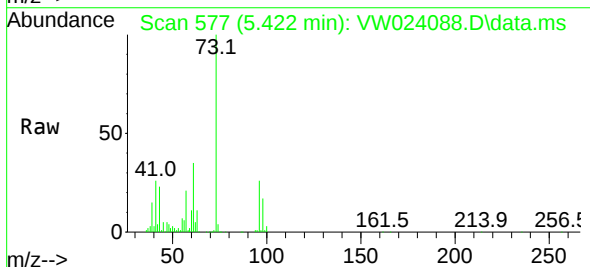



#18
Methyl tert-butyl Ether
Concen: 31.951 ug/L
RT: 5.428 min Scan# 51
Delta R.T. 0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7






Tgt Ion: 73 Resp: 138368
Ion Ratio Lower Upper
73 100
43 21.9 17.3 25.9
57 9.3 16.6 25.0

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

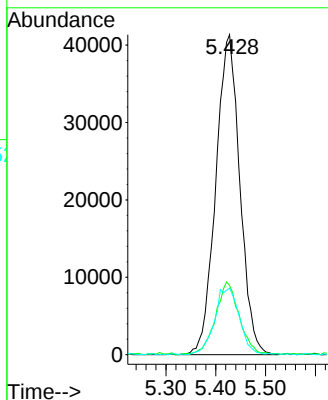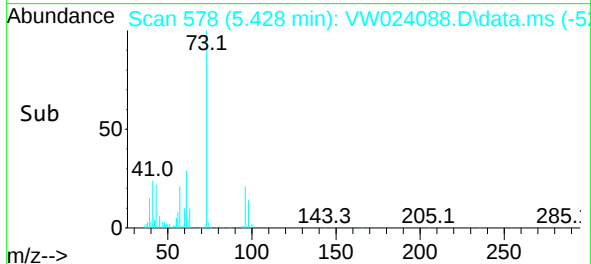

#20
cis-1,2-Dichloroethene
Concen: 26.308 ug/L
RT: 7.165 min Scan# 863
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05


Tgt Ion: 96 Resp: 84399
Ion Ratio Lower Upper
96 100
61 125.9 85.3 158.3
68 0.0 0.0 0.0

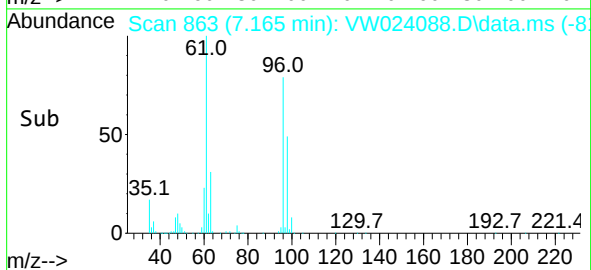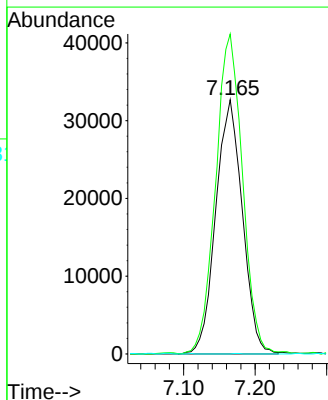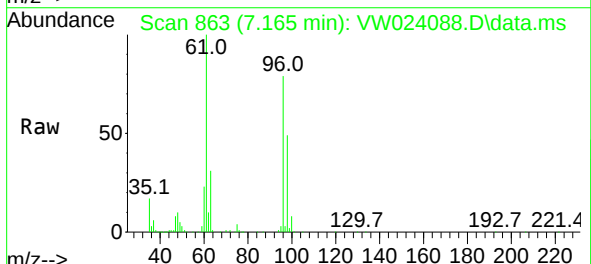



#23
Bromochloromethane
Concen: 14.264 ug/L
RT: 7.507 min Scan# 919
Delta R.T. -0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7






Tgt Ion:128 Resp: 23549
Ion Ratio Lower Upper
128 100
49 164.8 119.8 222.4
130 118.3 90.7 168.5
51 53.8 40.1 60.1

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

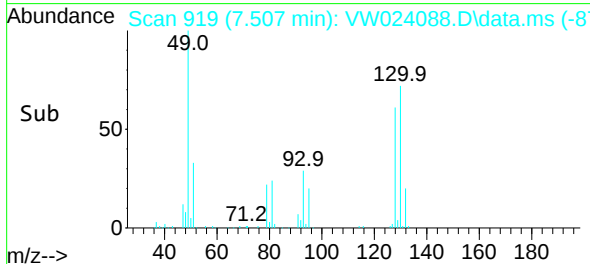

#27
1,2-Dichloroethane
Concen: 9.576 ug/L
RT: 8.397 min Scan# 1065
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05


Tgt Ion: 62 Resp: 43551
Ion Ratio Lower Upper
62 100
98 7.6 7.1 10.7

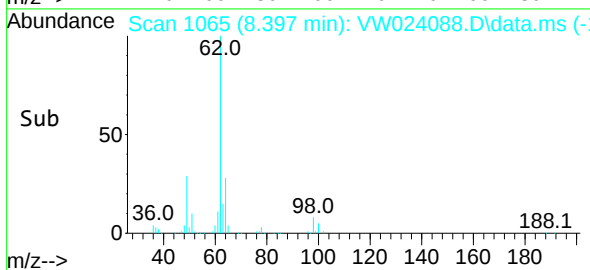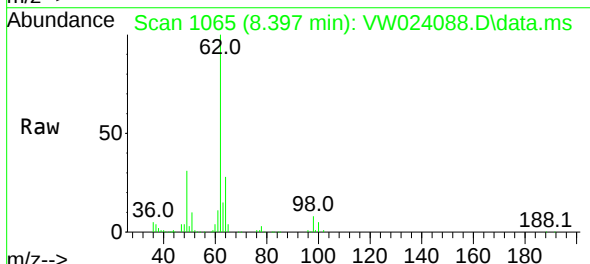



#29
Cyclohexane
Concen: 10.006 ug/L
RT: 7.952 min Scan# 992
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7



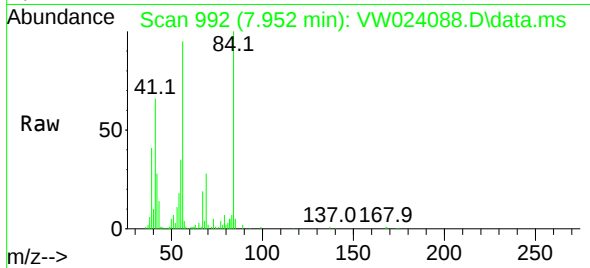


Tgt Ion: 56 Resp: 43648
Ion Ratio Lower Upper
56 100
69 30.5 24.1 36.1
84 95.5 76.2 114.4

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

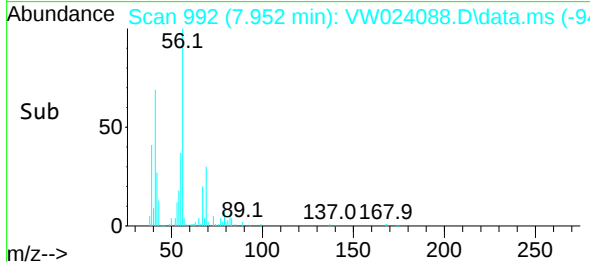

#30
1,1,1-Trichloroethane
Concen: 10.141 ug/L
RT: 7.872 min Scan# 979
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05


Tgt Ion: 97 Resp: 53664
Ion Ratio Lower Upper
97 100
99 65.5 51.7 77.5
61 47.0 37.8 56.6

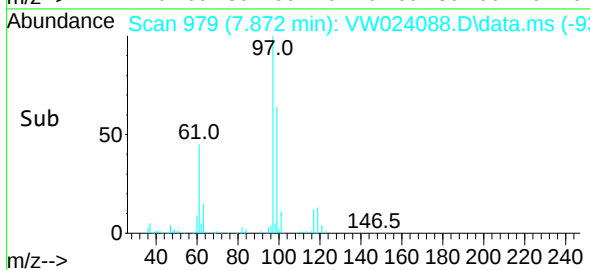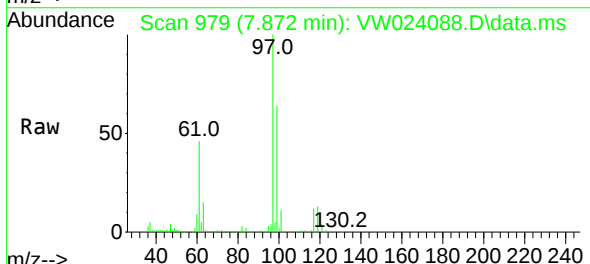



#31
Carbon tetrachloride
Concen: 12.900 ug/L
RT: 8.067 min Scan# 1011
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7



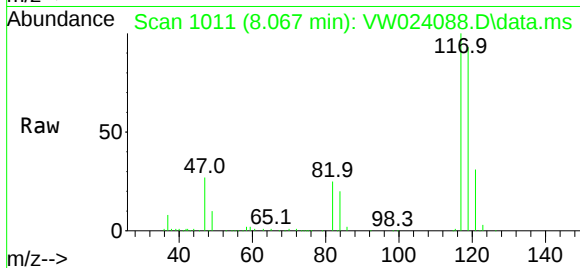


Tgt Ion:117 Resp: 62925
Ion Ratio Lower Upper
117 100
119 97.2 75.0 112.4

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

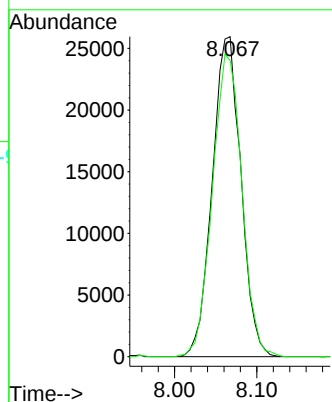

#34
Trichloroethene
Concen: 39.960 ug/L
RT: 9.085 min Scan# 1178
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05


Tgt Ion: 95 Resp: 144725
Ion Ratio Lower Upper
95 100
97 66.3 46.5 86.3
132 90.7 65.8 122.2
130 99.3 66.2 123.0

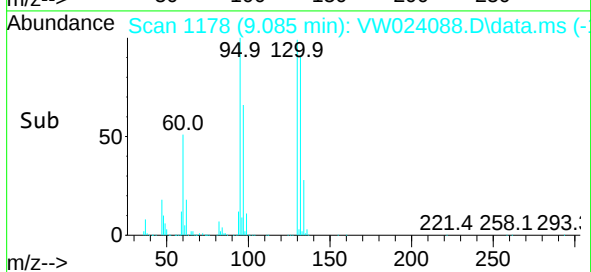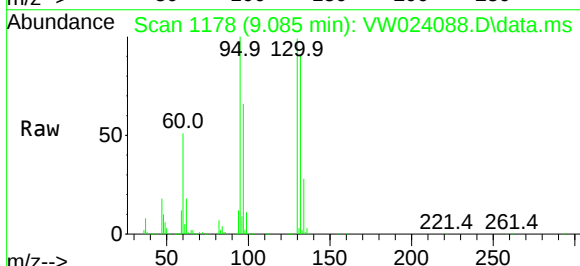



#35
Methylcyclohexane
Concen: 27.959 ug/L
RT: 9.329 min Scan# 1218
Delta R.T. -0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7






Tgt Ion: 83 Resp: 15383
Ion Ratio Lower Upper
83 100
55 74.5 57.3 85.9
98 48.9 38.9 58.3

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

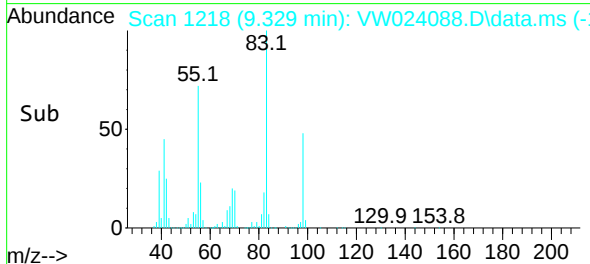

#37
1,2-Dichloropropane
Concen: 12.798 ug/L
RT: 9.366 min Scan# 1224
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05


Tgt Ion: 63 Resp: 44252
Ion Ratio Lower Upper
63 100
112 5.3 3.9 5.9

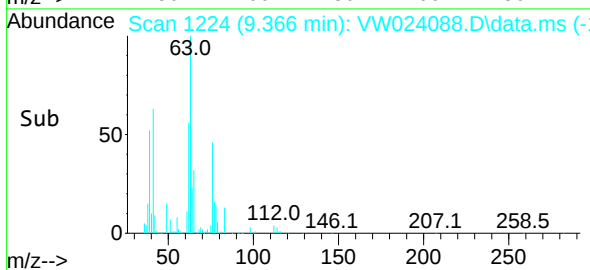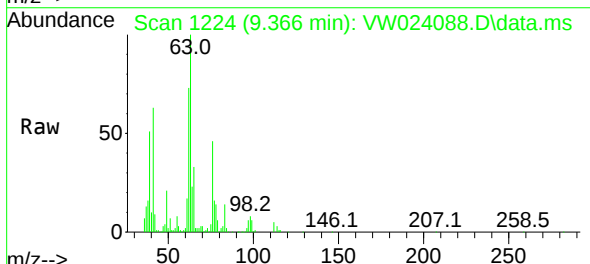



#38
Bromodichloromethane
Concen: 19.893 ug/L
RT: 9.640 min Scan# 1269
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7






Tgt Ion: 83 Resp: 9807
Ion Ratio Lower Upper
83 100
85 58.0 45.1 83.7
127 8.2 6.4 9.6

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

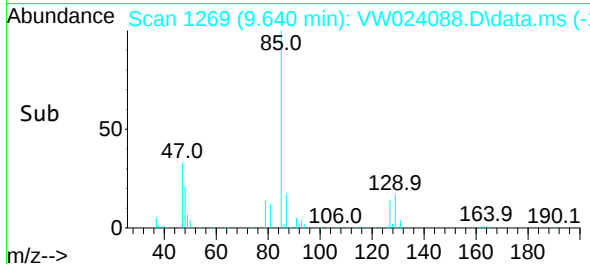

#39
cis-1,3-Dichloropropene
Concen: 15.851 ug/L
RT: 10.067 min Scan# 1339
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Tgt Ion: 75 Resp: 79854
Ion Ratio Lower Upper
75 100
77 31.0 21.8 40.6

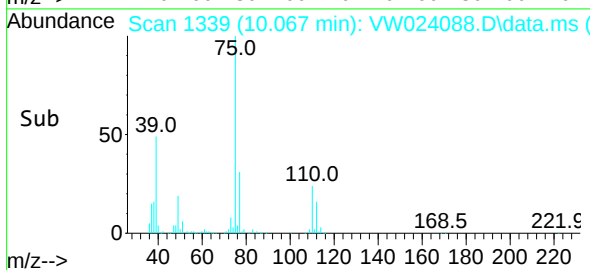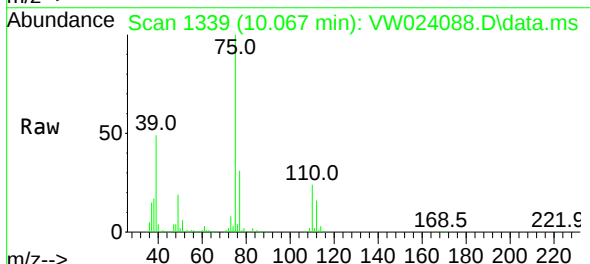



#42

Toluene

Concen: 20.997 ug/L

RT: 10.384 min Scan# 1391

Delta R.T. 0.000 min

Lab File: VW024088.D

Acq: 26 Jul 2022 09:05

Instrument :

MSVOA_W

ClientSampleId :

DBUJ7

Tgt Ion: 91 Resp: 324838

Ion Ratio Lower Upper

91 100





92 61.4 40.3 74.9

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022

Supervised By :Mahesh Dadoda 07/27/2022

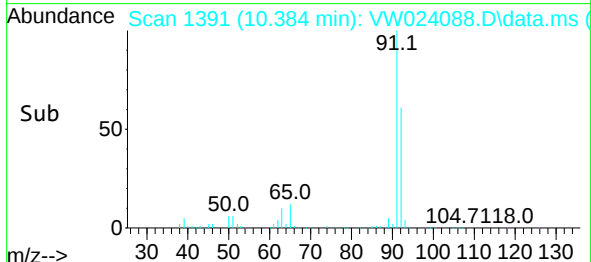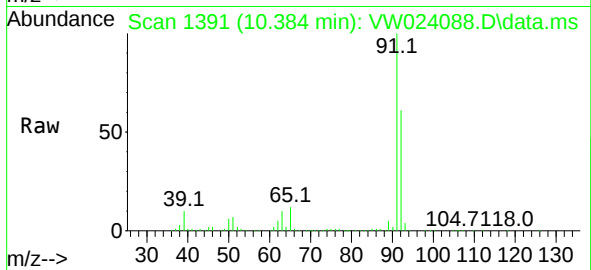

#44

trans-1,3-Dichloropropene

Concen: 7.430 ug/L

RT: 10.604 min Scan# 1427

Delta R.T. 0.000 min

Lab File: VW024088.D




Acq: 26 Jul 2022 09:05


Tgt Ion: 75 Resp: 35446

Ion Ratio Lower Upper

75 100


77 34.1 21.3 39.6

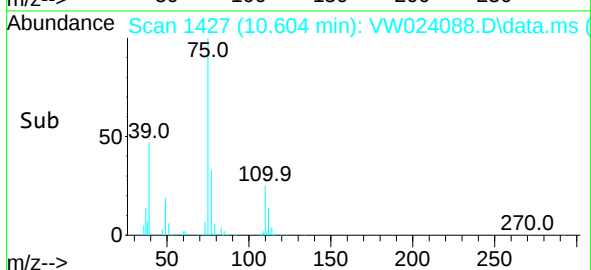



#46
Tetrachloroethene
Concen: 39.468 ug/L
RT: 10.860 min Scan# 1468
Delta R.T. 0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7






Tgt Ion:164 Resp: 111878
Ion Ratio Lower Upper
164 100
129 106.8 65.7 122.1
131 101.4 69.2 128.4
166 152.4 92.8 172.4

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

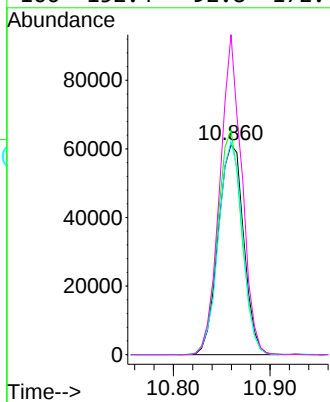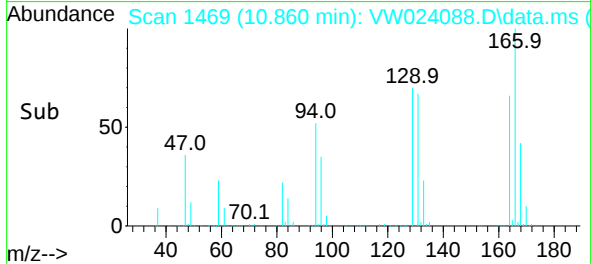

#48
2-Hexanone
Concen: 25.901 ug/L
RT: 10.969 min Scan# 1487
Delta R.T. 0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Tgt Ion: 43 Resp: 45162
Ion Ratio Lower Upper
43 100
58 52.4 41.0 61.6
57 18.1 14.5 21.7
100 13.0 10.9 16.3

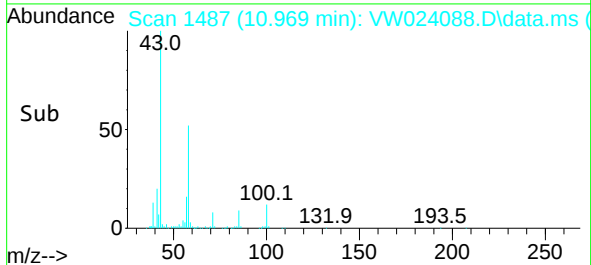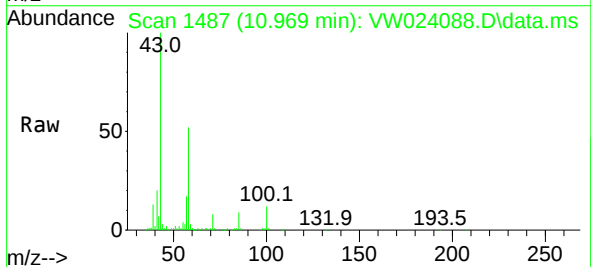



#49

Dibromochloromethane

Concen: 18.924 ug/L

RT: 11.128 min Scan# 1513

Delta R.T. 0.000 min

Lab File: VW024088.D

Acq: 26 Jul 2022 09:05

Instrument :

MSVOA_W

ClientSampleId :

DBUJ7

Tgt Ion:129 Resp: 66794

Ion Ratio Lower Upper

129 100





127 72.3 55.0 102.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022

Supervised By :Mahesh Dadoda 07/27/2022

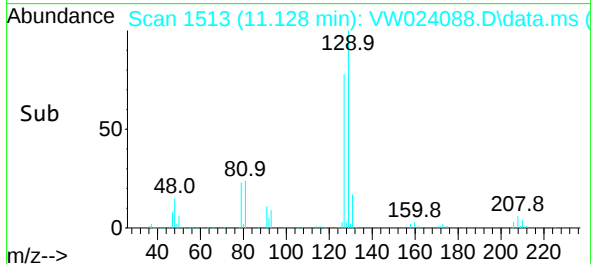

#52

Ethylbenzene

Concen: 15.865 ug/L

RT: 11.725 min Scan# 1611

Delta R.T. 0.000 min

Lab File: VW024088.D




Acq: 26 Jul 2022 09:05


Tgt Ion: 91 Resp: 270477

Ion Ratio Lower Upper

91 100


106 29.6 21.0 39.0

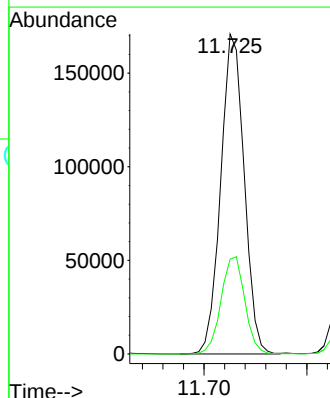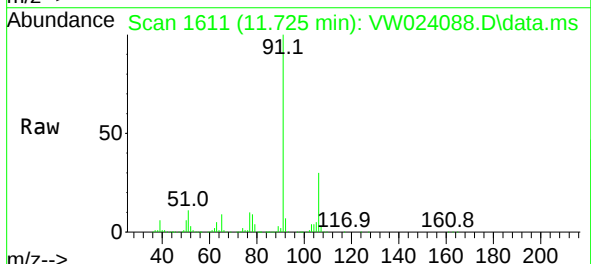



#53
m,p-Xylene
Concen: 10.390 ug/L
RT: 11.841 min Scan# 1630
Delta R.T. 0.006 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7






Tgt Ion:106 Resp: 68759
Ion Ratio Lower Upper
106 100
91 194.8 142.9 265.3

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Supervised By :Mahesh
Dadoda
07/27/2022

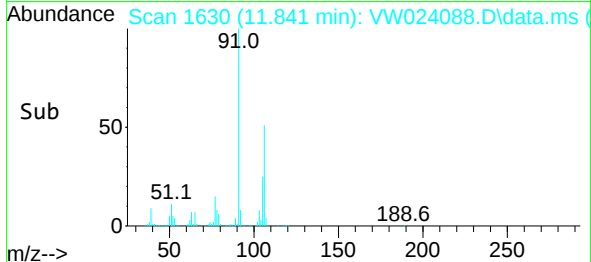

#54
o-Xylene
Concen: 12.171 ug/L
RT: 12.164 min Scan# 1683
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05


Tgt Ion:106 Resp: 77024
Ion Ratio Lower Upper
106 100
91 204.7 150.6 279.6

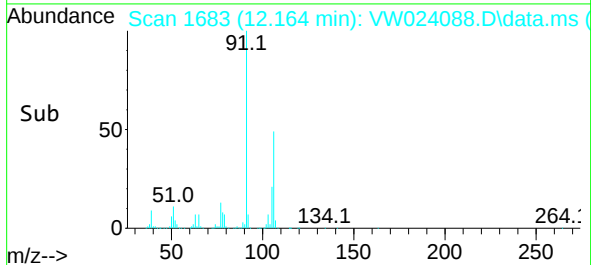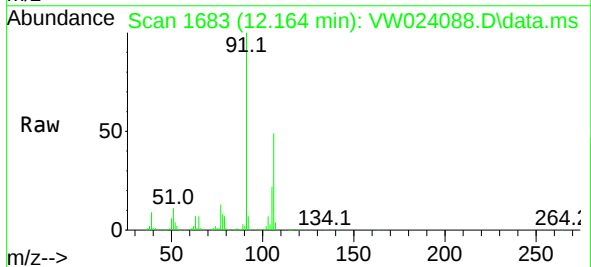



#60
Isopropylbenzene
Concen: 13.285 ug/L
RT: 12.463 min Scan# 1732
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

Instrument :
MSVOA_W
ClientSampleId :
DBUJ7






Tgt Ion:105 Resp: 211279
Ion Ratio Lower Upper
105 100
120 25.5 21.1 31.7
77 17.0 12.8 19.2


Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022



Supervised By :Mahesh
Dadoda
07/27/2022

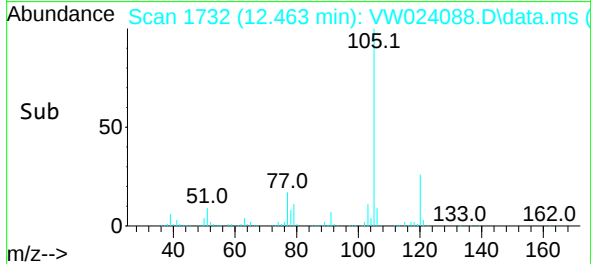


#64
1,3-Dichlorobenzene
Concen: 19.507 ug/L
RT: 13.493 min Scan# 1901
Delta R.T. 0.000 min
Lab File: VW024088.D
Acq: 26 Jul 2022 09:05

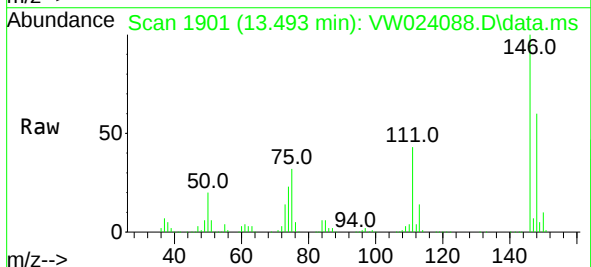

Tgt Ion:146 Resp: 148377
Ion Ratio Lower Upper
146 100
111 42.6 26.4 49.0
148 60.0 41.4 77.0

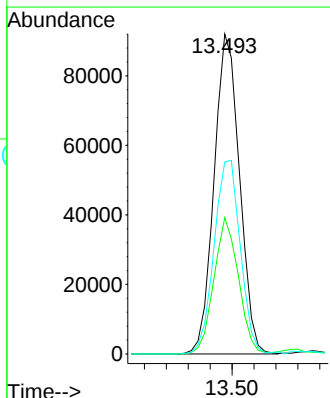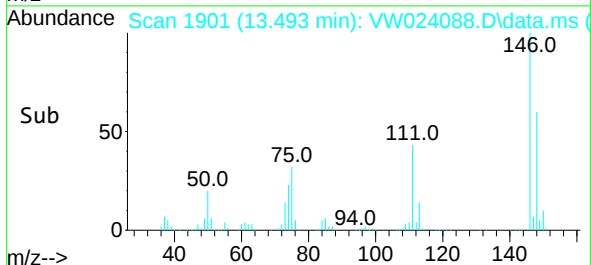



#67

1,2-Dichlorobenzene

Concen: 10.158 ug/L

RT: 13.865 min Scan# 1962

Delta R.T. 0.000 min

Lab File: VW024088.D

Acq: 26 Jul 2022 09:05

Instrument :

MSVOA_W

ClientSampleId :

DBUJ7

Tgt Ion:	146	Resp:	7227
Ion Ratio	Lower	Upper	
146	100		
111	47.1	33.9	50.9
148	68.4	53.0	79.6

Manual Integrations

APPROVED





Reviewed By :Semsettin Yesilyurt 07/27/2022

Supervised By :Mahesh Dadoda 07/27/2022

Supervised By :Mahesh

Dadoda

07/27/2022

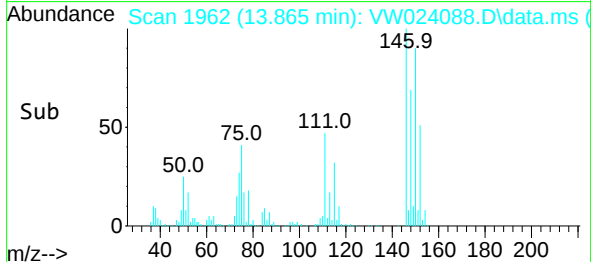

#68

1,2-Dibromo-3-chloropropane

Concen: 15.990 ug/L

RT: 14.481 min Scan# 2063

Delta R.T. 0.006 min

Lab File: VW024088.D

Acq: 26 Jul 2022 09:05

Tgt Ion:	75	Resp:	10083
Ion Ratio	Lower	Upper	
75	100		
155	64.7	58.6	88.0
157	87.1	64.0	96.0

