

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024090.D
 Acq On : 26 Jul 2022 10:30
 Operator : SY/VA
 Sample : N3745-07
 Misc : 5.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jul 26 23:40:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	222493	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	227318	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	101668	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	126305	26.484	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.920%
7) Chloroethane-d5	2.873	69	79998	24.826	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.320%
11) 1,1-Dichloroethene-d2	4.001	63	73604	17.527	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.120%
21) 2-Butanone-d5	7.080	46	35776	42.209	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.420%
24) Chloroform-d	7.647	84	137940	22.551	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.200%
26) 1,2-Dichloroethane-d4	8.305	65	83067	23.637	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.560%
32) Benzene-d6	8.268	84	268345	25.412	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.640%
36) 1,2-Dichloropropane-d6	9.274	67	79263	23.798	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.200%
41) Toluene-d8	10.323	98	253065	23.963	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.840%
43) trans-1,3-Dichloroprop...	10.579	79	33208	22.487	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.960%
47) 2-Hexanone-d5	10.920	63	29483	42.342	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.680%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	76897	20.009	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	86938	26.404	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.600%
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	17226	5.087	ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024090.D
Acq On : 26 Jul 2022 10:30
Operator : SY/VA
Sample : N3745-07
Misc : 5.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001


Quant Time: Jul 26 23:40:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

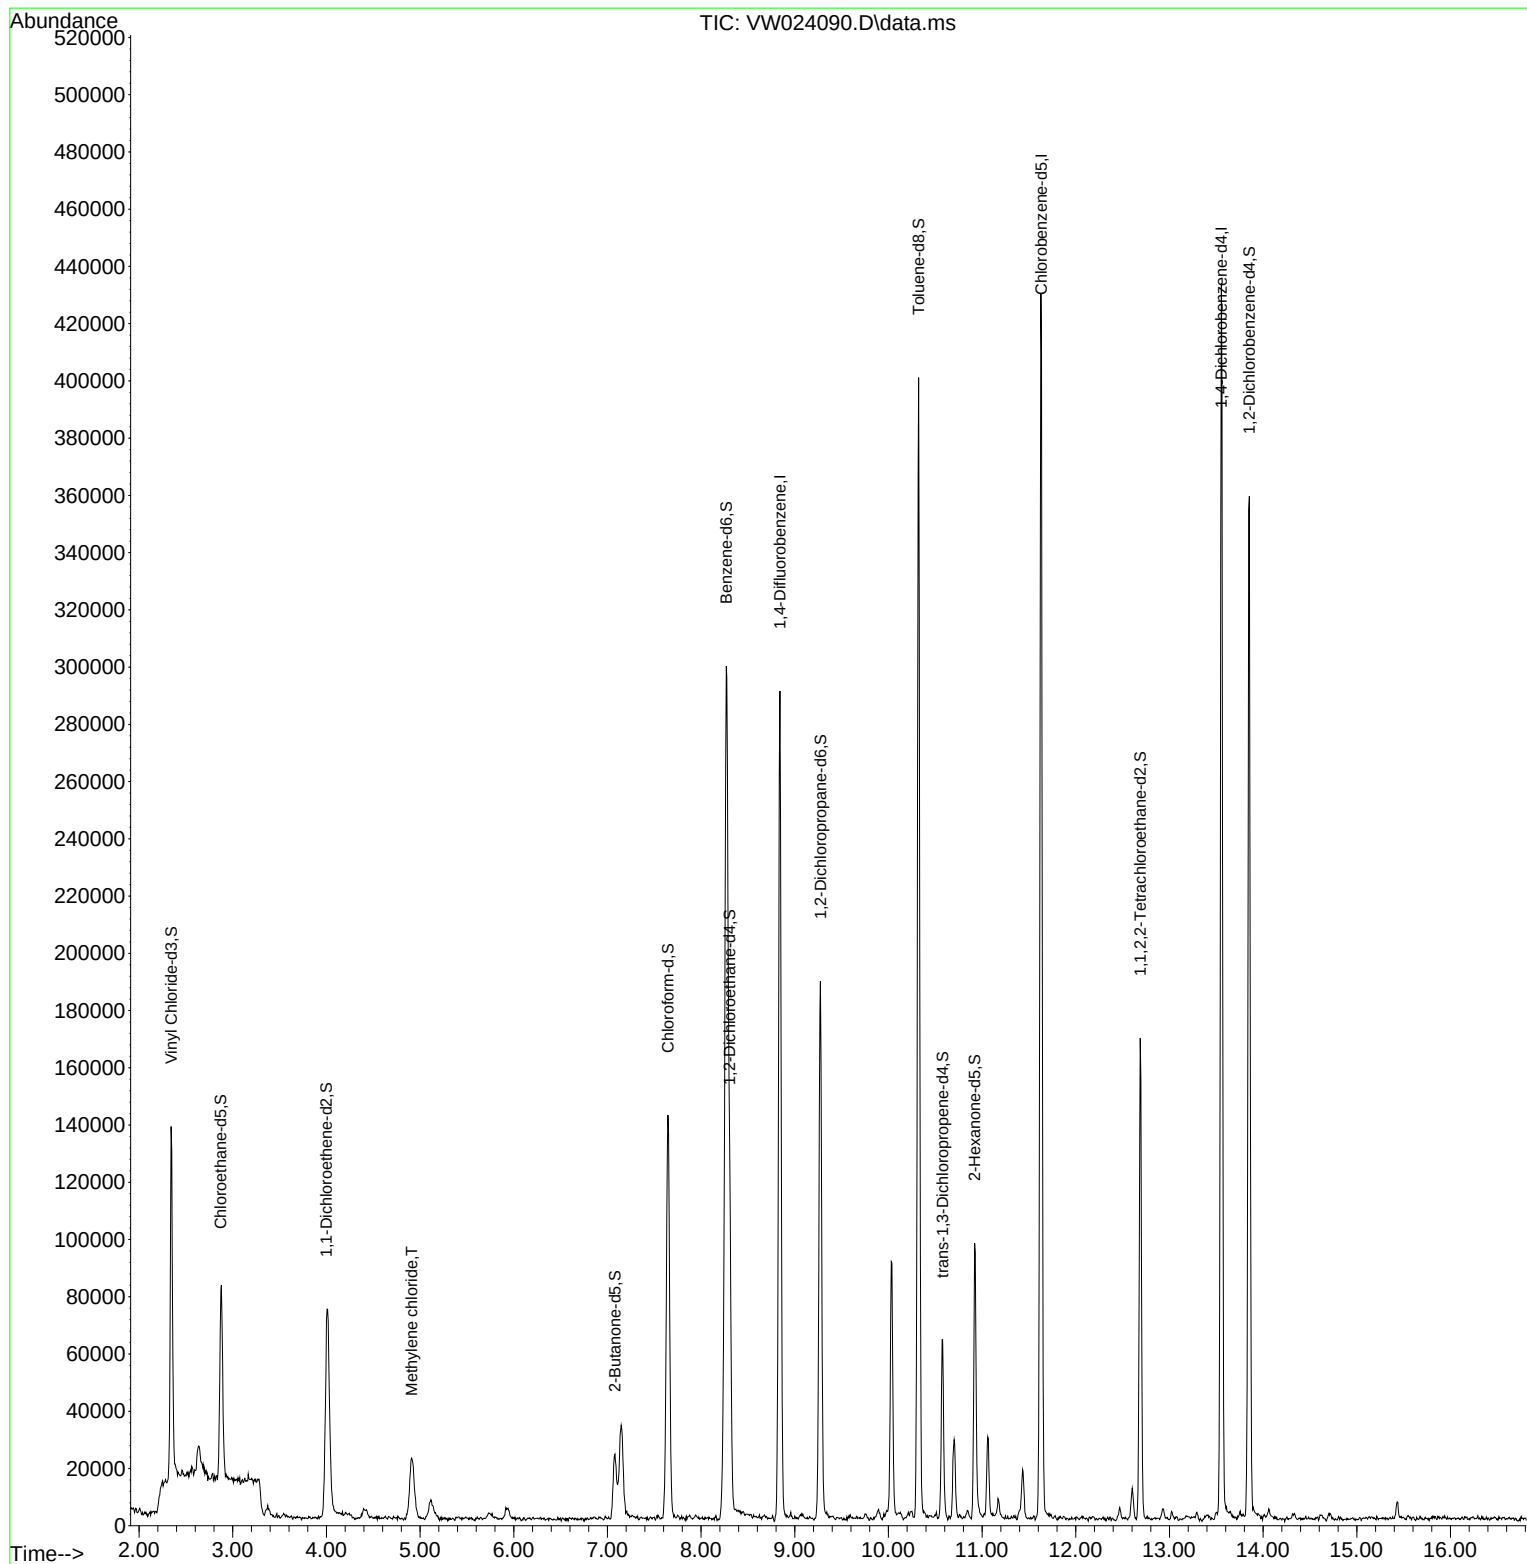

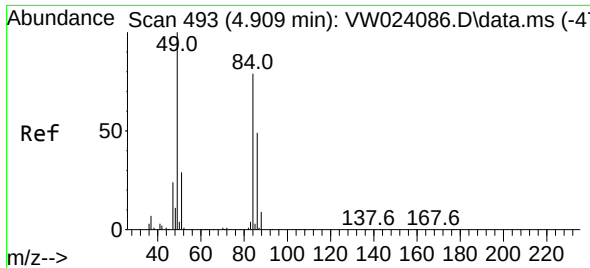

#16
Methylene chloride
Concen: 5.087 ug/L
RT: 4.909 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW024090.D
Acq: 26 Jul 2022 10:30

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

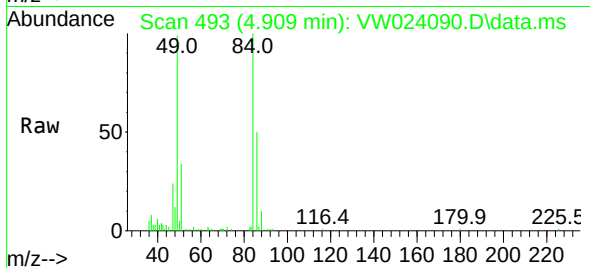

Tgt Ion: 84 Resp: 17226

Ion	Ratio	Lower	Upper
84	100		
86	50.4	44.7	83.1
49	98.6	83.7	155.4

