

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024094.D
 Acq On : 26 Jul 2022 12:08
 Operator : SY/VA
 Sample : N3743-22
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Jul 26 23:41:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	218046	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	221119	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	96048	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	120933	25.874	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.480%
7) Chloroethane-d5	2.873	69	78490	24.855	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.400%
11) 1,1-Dichloroethene-d2	4.013	63	69748	16.948	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.800%
21) 2-Butanone-d5	7.074	46	38688	46.576	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.160%
24) Chloroform-d	7.647	84	131164	21.881	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.520%
26) 1,2-Dichloroethane-d4	8.305	65	81310	23.609	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.440%
32) Benzene-d6	8.269	84	254644	24.791	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.160%
36) 1,2-Dichloropropane-d6	9.274	67	75628	23.343	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.360%
41) Toluene-d8	10.323	98	239678	23.332	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.320%
43) trans-1,3-Dichloroprop...	10.579	79	31345	21.821	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.280%
47) 2-Hexanone-d5	10.927	63	32107	47.403	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.800%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	78188	20.916	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.680%
66) 1,2-Dichlorobenzene-d4	13.853	152	82926	26.659	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.640%
Target Compounds						
16) Methylene chloride	4.916	84	24117	7.267	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024094.D
Acq On : 26 Jul 2022 12:08
Operator : SY/VA
Sample : N3743-22
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Jul 26 23:41:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

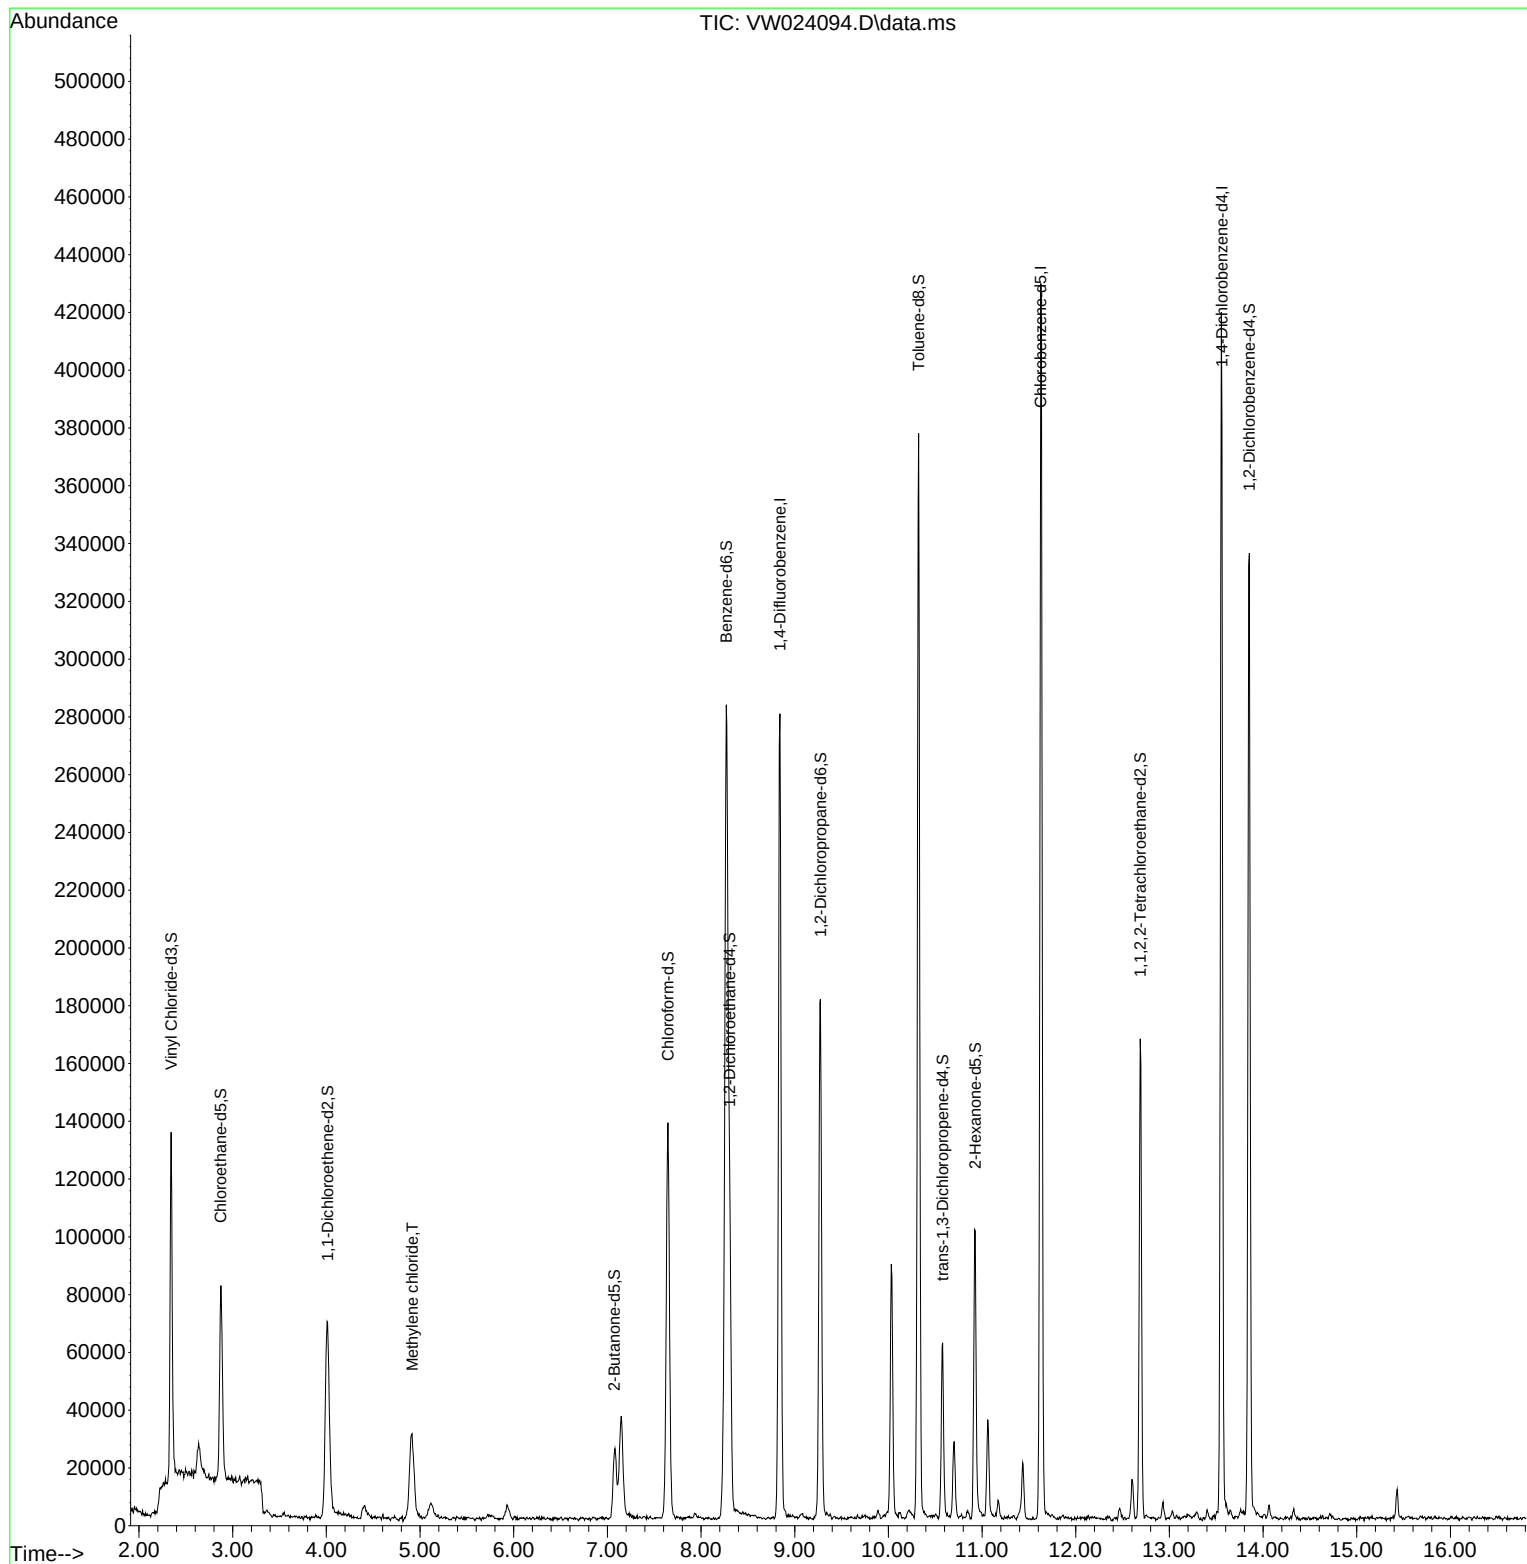

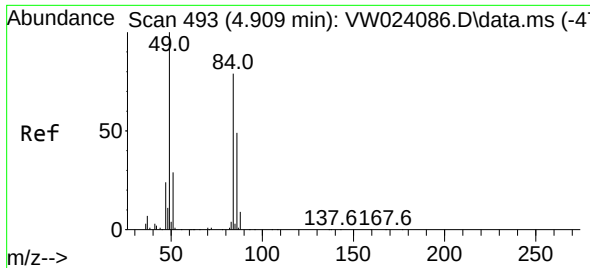

#16

Methylene chloride

Concen: 7.267 ug/L

RT: 4.916 min Scan# 49

Delta R.T. 0.006 min

Lab File: VW024094.D


Acq: 26 Jul 2022 12:08

Instrument :

MSVOA_W

ClientSampleId :

VHBLK002

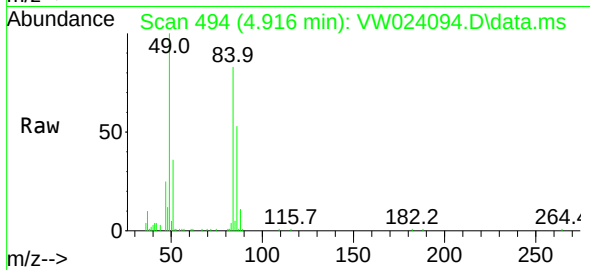

Tgt Ion: 84 Resp: 24117

Ion Ratio Lower Upper

84 100

86 64.0 44.7 83.1

49 120.2 83.7 155.4

