

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024098.D
 Acq On : 26 Jul 2022 13:46
 Operator : SY/VA
 Sample : N3790-14RE
 Misc : 3.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK8RE

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 07/27/2022
 Supervised By : Mahesh Dadoda 07/27/2022

Quant Time: Jul 26 23:42:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	207695	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	131498	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	31188	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	127625	28.667	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 114.680%			
7) Chloroethane-d5	2.873	69	99426m	33.053	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 132.200%			
11) 1,1-Dichloroethene-d2	4.007	63	59037	15.060	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 60.240%			
21) 2-Butanone-d5	7.080	46	9043	11.429	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 22.860%			
24) Chloroform-d	7.647	84	148944	26.085	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 104.360%			
26) 1,2-Dichloroethane-d4	8.305	65	88556	26.995	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 107.960%			
32) Benzene-d6	8.275	84	214941	35.187	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 140.760%#			
36) 1,2-Dichloropropane-d6	9.275	67	79976	41.509	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 166.040%#			
41) Toluene-d8	10.323	98	158920	26.014	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 104.040%			
43) trans-1,3-Dichloroprop...	10.573	79	5321	6.229	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 24.920%#			
47) 2-Hexanone-d5	10.927	63	1669	4.143	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 8.280%#			
56) 1,1,2,2-Tetrachloroeth...	12.689	84	52640	23.678	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 94.720%			
66) 1,2-Dichlorobenzene-d4	13.853	152	23246	23.015	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 92.040%			
Target Compounds					Qvalue	
13) Acetone	4.129	43	10710	19.075	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024098.D
Acq On : 26 Jul 2022 13:46
Operator : SY/VA
Sample : N3790-14RE
Misc : 3.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBUK8RE

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
Supervised By :Mahesh Dadoda 07/27/2022


Quant Time: Jul 26 23:42:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

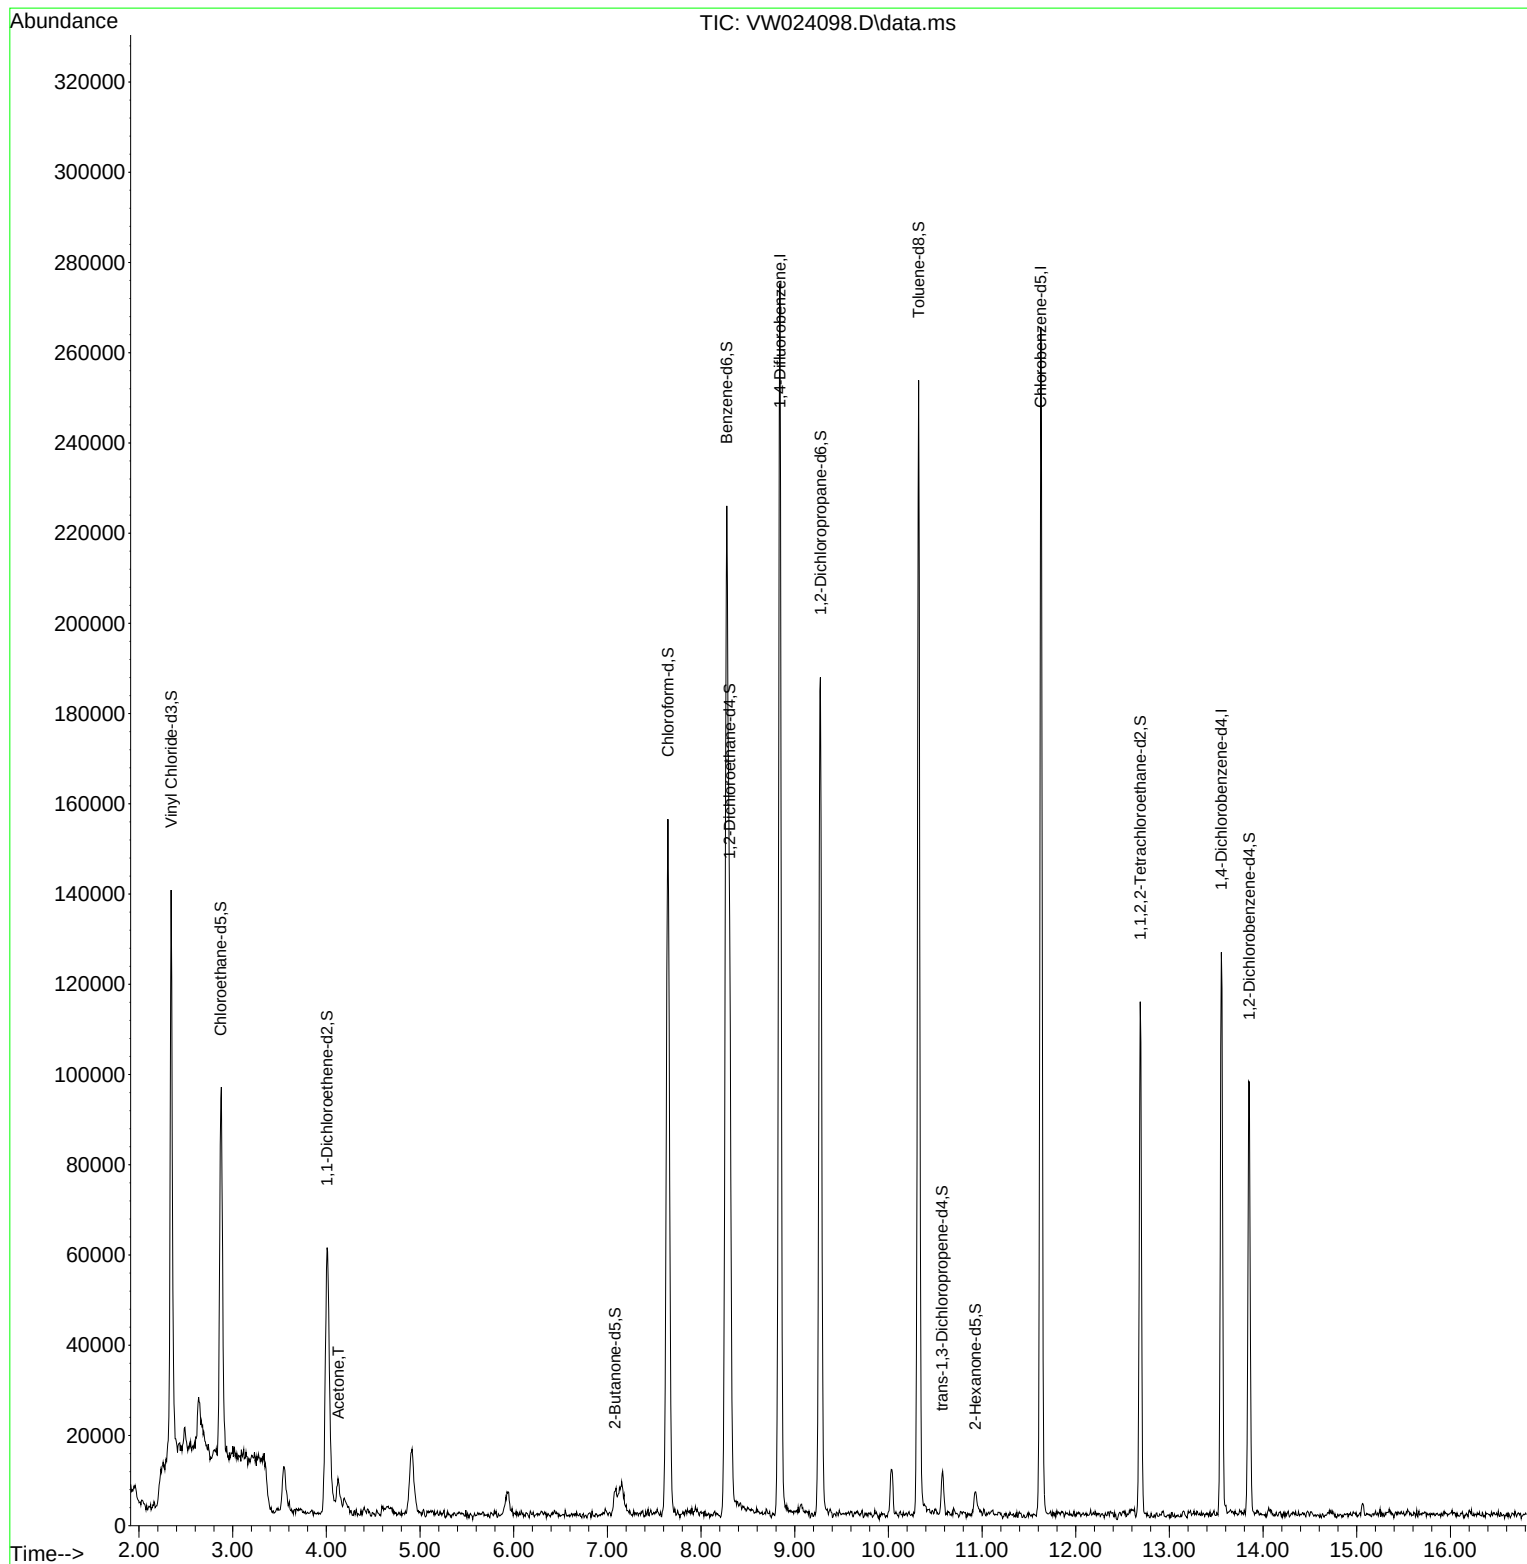

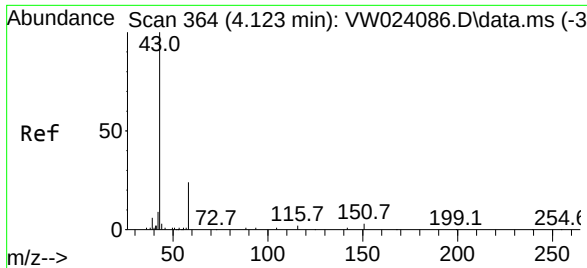

#13
 Acetone
 Concen: 19.075 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW024098.D
 Acq: 26 Jul 2022 13:46

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK8RE

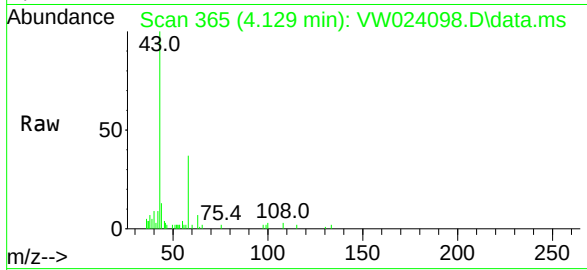

Tgt Ion: 43 Resp: 10710
 Ion Ratio Lower Upper
 43 100
 58 22.1 0.0 60.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2022
 Supervised By :Mahesh Dadoda 07/27/2022

