

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024103.D
 Acq On : 26 Jul 2022 16:14
 Operator : SY/VA
 Sample : VIBLK517
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK517

Quant Time: Jul 26 23:43:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.836	114	204151	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	207375	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	89827	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	126746	28.964	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.840%
7) Chloroethane-d5	2.873	69	84010	28.413	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	113.640%
11) 1,1-Dichloroethene-d2	4.007	63	69809	18.117	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.480%
21) 2-Butanone-d5	7.074	46	31198	40.115	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.220%
24) Chloroform-d	7.641	84	122896	21.897	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	8.299	65	70802	21.957	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.840%
32) Benzene-d6	8.269	84	224913	23.348	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.400%
36) 1,2-Dichloropropane-d6	9.268	67	69445	22.855	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.440%
41) Toluene-d8	10.323	98	209199	21.715	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.840%
43) trans-1,3-Dichloroprop...	10.573	79	28110	20.865	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.480%
47) 2-Hexanone-d5	10.927	63	24760	38.978	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.960%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	65449	18.668	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.680%
66) 1,2-Dichlorobenzene-d4	13.853	152	68021	23.382	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.520%
Target Compounds						Qvalue
16) Methylene chloride	4.903	84	41583	13.383	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024103.D
Acq On : 26 Jul 2022 16:14
Operator : SY/VA
Sample : VIBLK517
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK517

Quant Time: Jul 26 23:43:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

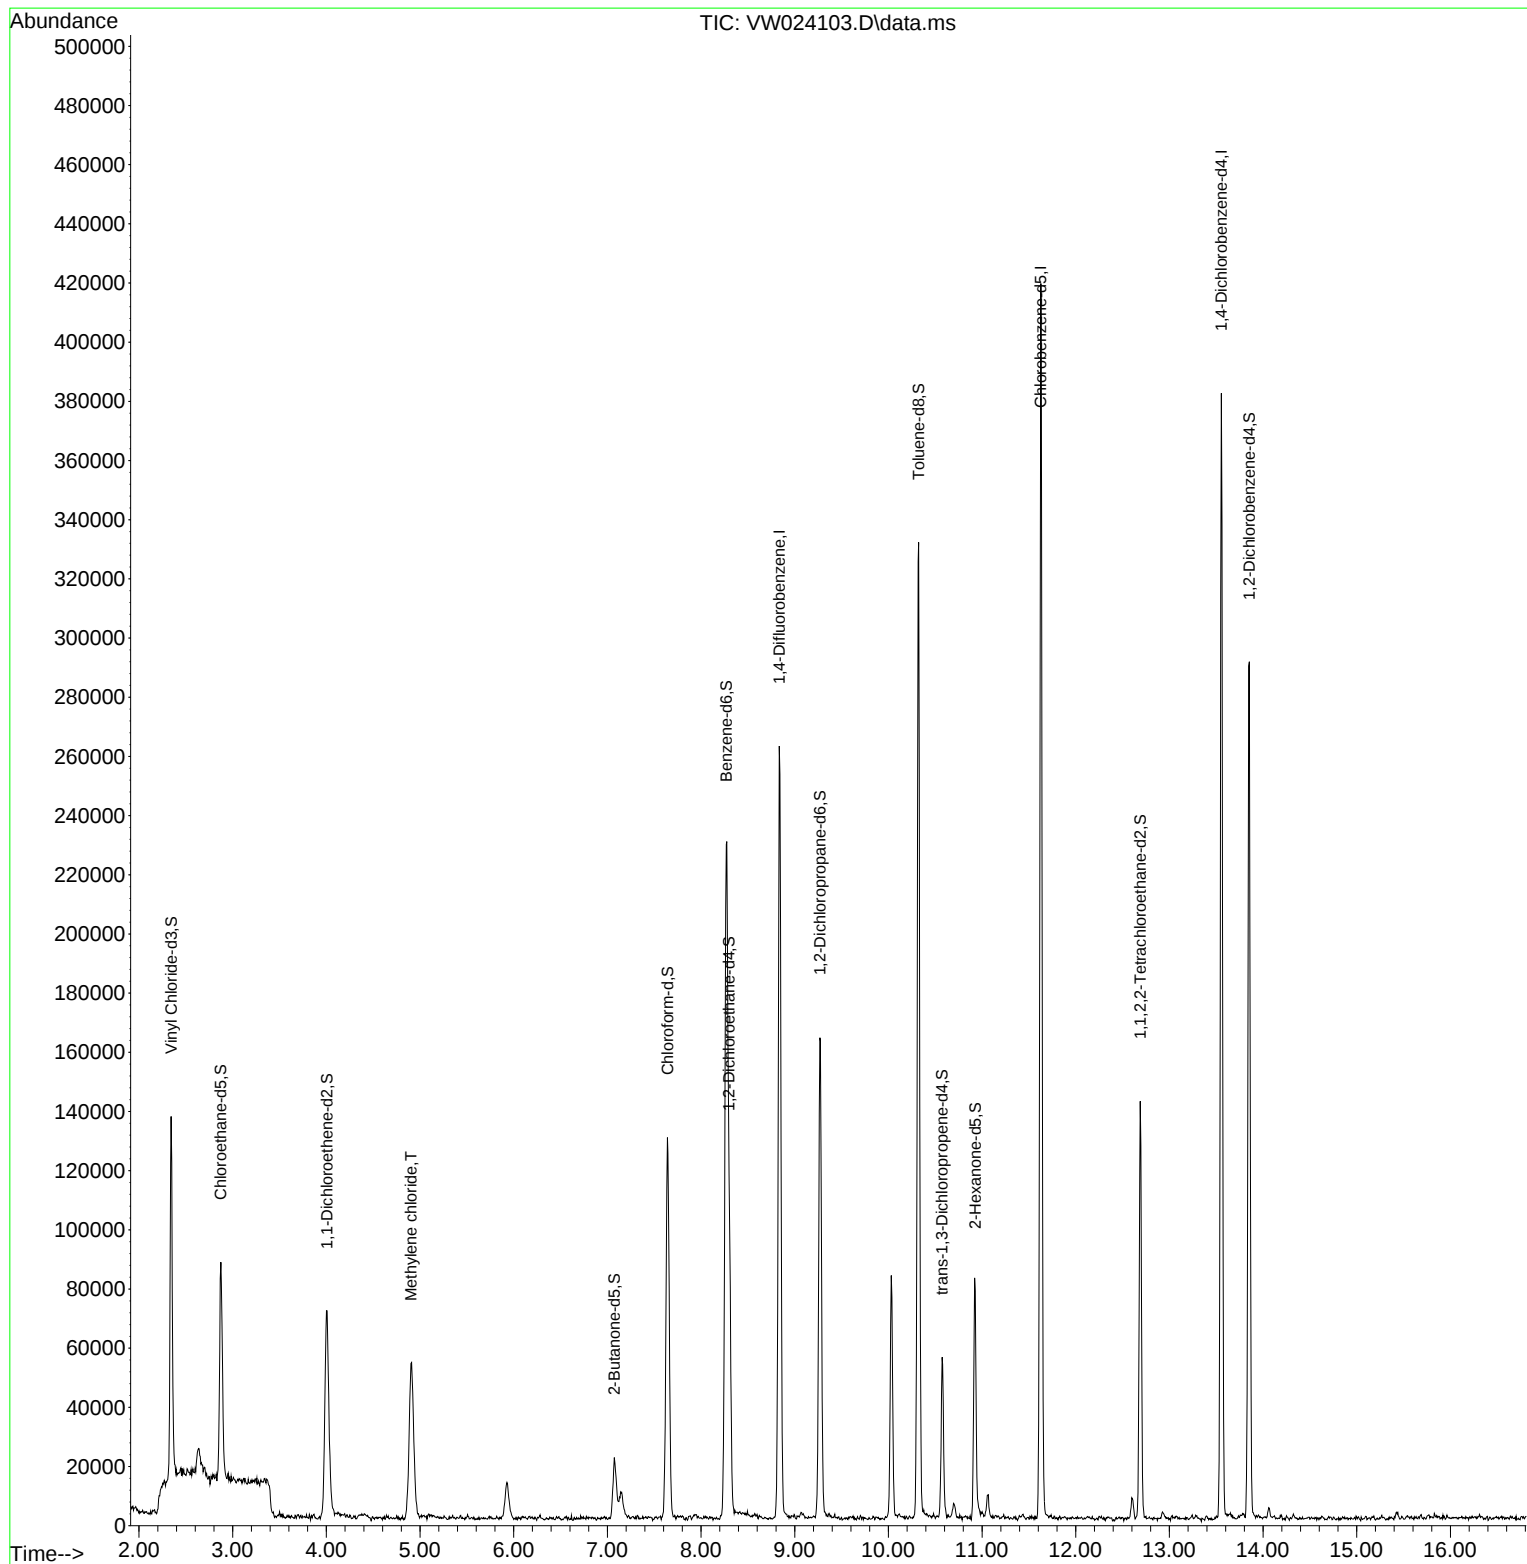

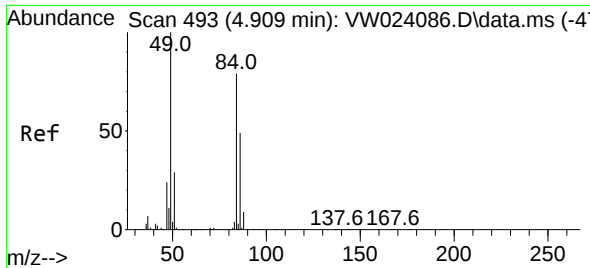

#16

Methylene chloride

Concen: 13.383 ug/L

RT: 4.903 min Scan# 49

Delta R.T. -0.006 min

Lab File: VW024103.D


Acq: 26 Jul 2022 16:14

Instrument :

MSVOA_W

ClientSampleId :

VIBLK517

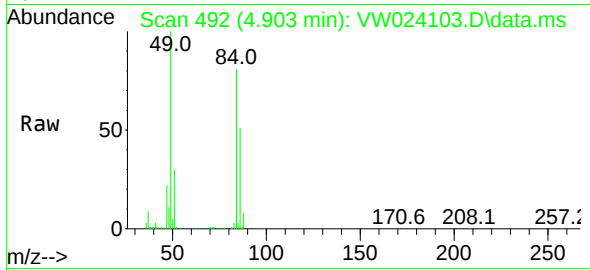

Tgt Ion: 84 Resp: 41583

Ion Ratio Lower Upper

84 100

86 63.2 44.7 83.1

49 124.1 83.7 155.4

