

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024104.D
 Acq On : 26 Jul 2022 16:39
 Operator : SY/VA
 Sample : VIBLK518
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK518

Quant Time: Jul 26 23:43:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	208311	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	215855	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	95160	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.342	65	131882	29.536	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	118.160%
7) Chloroethane-d5	2.873	69	83571	27.700	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.800%
11) 1,1-Dichloroethene-d2	4.007	63	71739	18.246	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.000%
21) 2-Butanone-d5	7.079	46	37083	46.730	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.460%
24) Chloroform-d	7.646	84	134410	23.470	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.880%
26) 1,2-Dichloroethane-d4	8.305	65	78545	23.872	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.480%
32) Benzene-d6	8.274	84	247669	24.700	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.800%
36) 1,2-Dichloropropane-d6	9.274	67	77108	24.380	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.520%
41) Toluene-d8	10.323	98	235202	23.455	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.800%
43) trans-1,3-Dichloroprop...	10.579	79	30187	21.527	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.120%
47) 2-Hexanone-d5	10.920	63	28807	43.568	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.140%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	75062	20.569	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.280%
66) 1,2-Dichlorobenzene-d4	13.852	152	78683	25.531	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.120%
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	44750	14.114	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024104.D
Acq On : 26 Jul 2022 16:39
Operator : SY/VA
Sample : VIBLK518
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK518

Quant Time: Jul 26 23:43:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

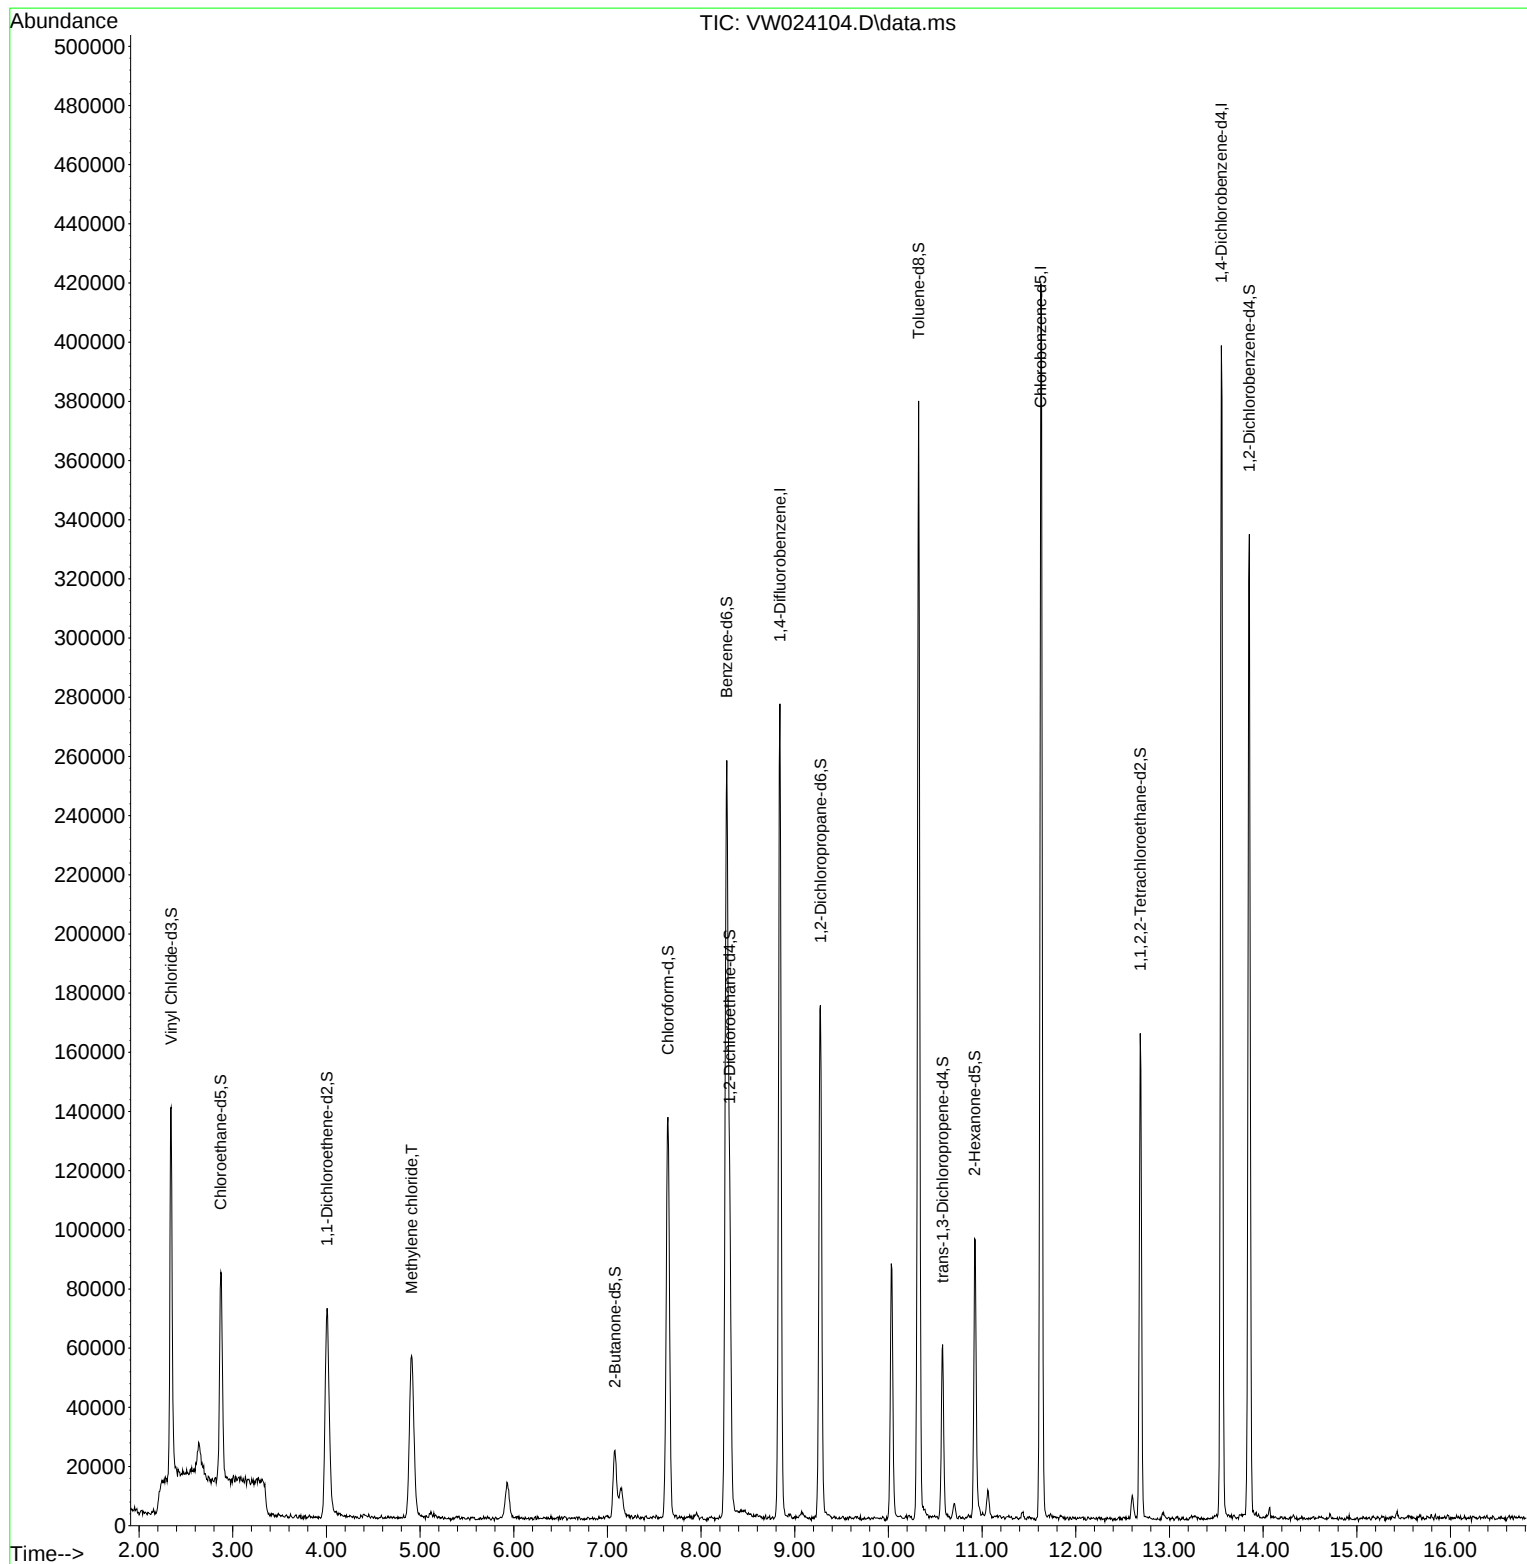

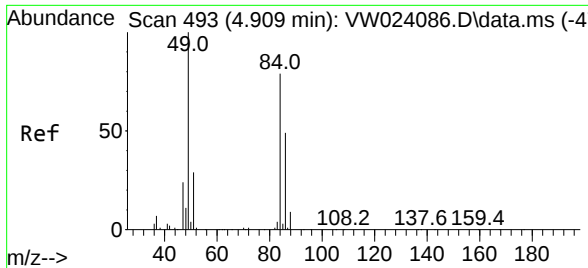

#16
Methylene chloride
Concen: 14.114 ug/L
RT: 4.909 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW024104.D
Acq: 26 Jul 2022 16:39

Instrument :
MSVOA_W
ClientSampleId :
VIBLK518

Tgt Ion: 84 Resp: 44750
Ion Ratio Lower Upper
84 100
86 66.9 44.7 83.1
49 128.2 83.7 155.4

