




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072624\
Data File : VW029747.D
Acq On : 26 Jul 2024 13:27
Operator : SY/MD
Sample : P3278-07
Misc : 9.10g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1ZQ3

Manual IntegrationsAPPROVED

Quant Time: Jul 27 00:54:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 27 00:53:25 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

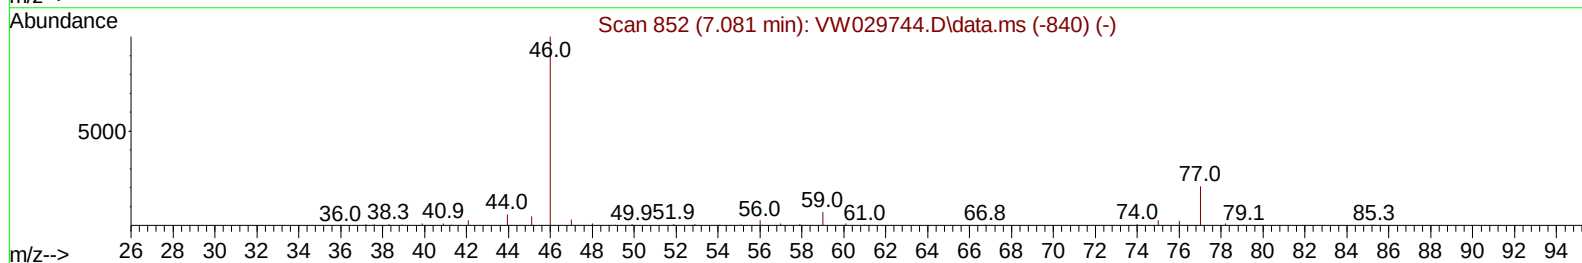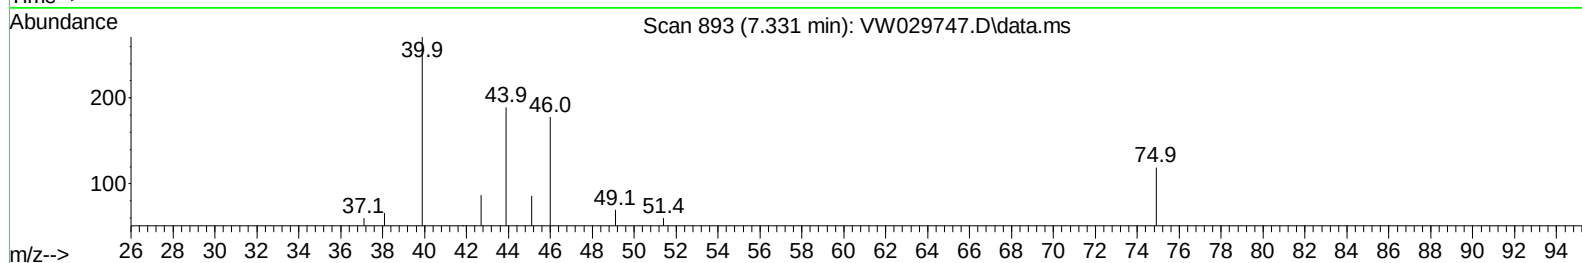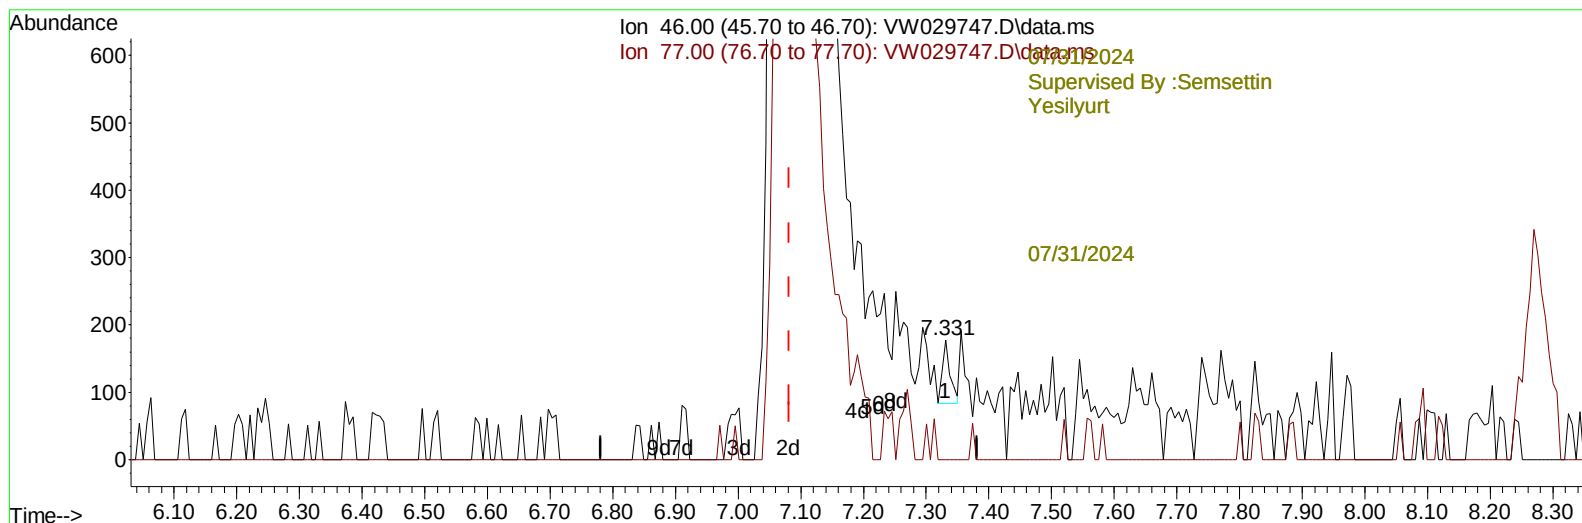

TIC: VW029747.D\data.ms

(21) 2-Butanone-d5 (S)

7.331min (+ 0.250) 0.08 ug/L

response 79

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	23.50	27.85
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072624\
Data File : VW029747.D
Acq On : 26 Jul 2024 13:27
Operator : SY/MD
Sample : P3278-07
Misc : 9.10g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1ZQ3

Manual IntegrationsAPPROVED

Quant Time: Jul 27 00:54:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 27 00:53:25 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

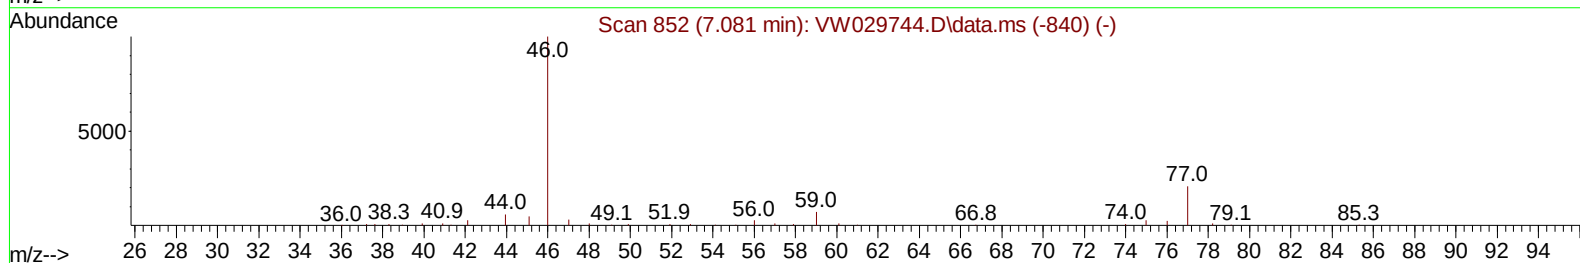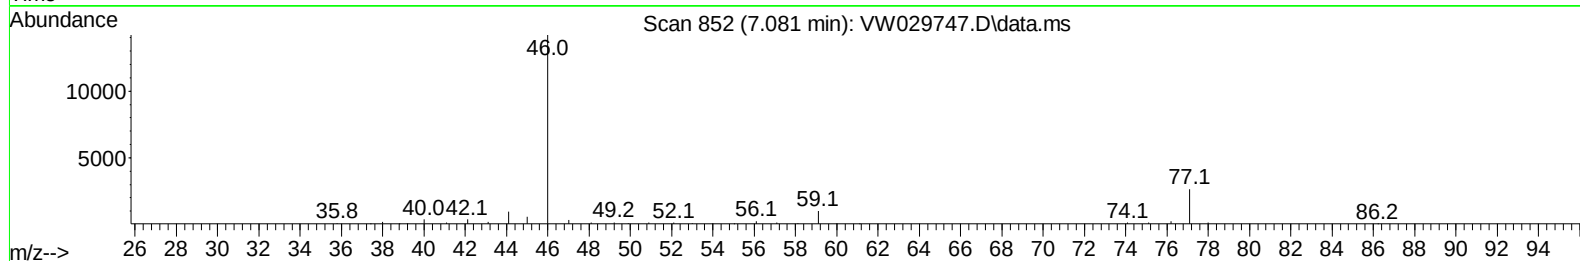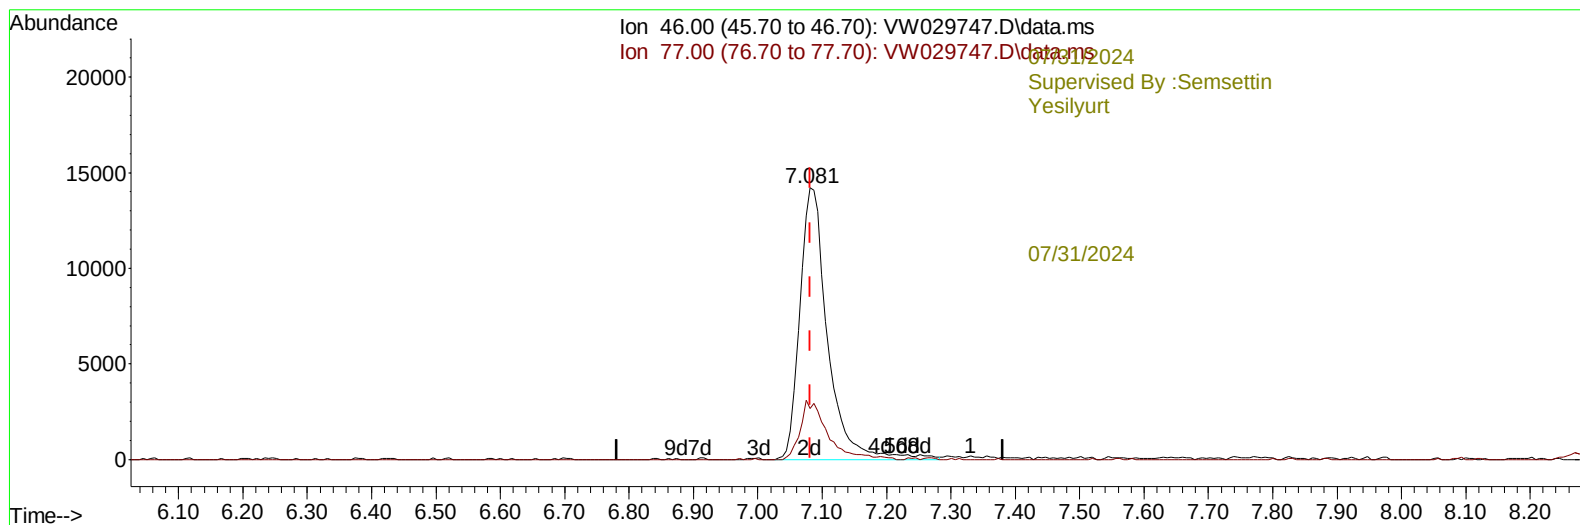

TIC: VW029747.D\data.ms

(21) 2-Butanone-d5 (S)

7.081min (-0.000) 42.98 ug/L m

response 42764

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	23.50	0.05#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072624\
Data File : VW029747.D
Acq On : 26 Jul 2024 13:27
Operator : SY/MD
Sample : P3278-07
Misc : 9.10g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1ZQ3

Manual IntegrationsAPPROVED

Quant Time: Jul 27 00:54:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 27 00:53:25 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

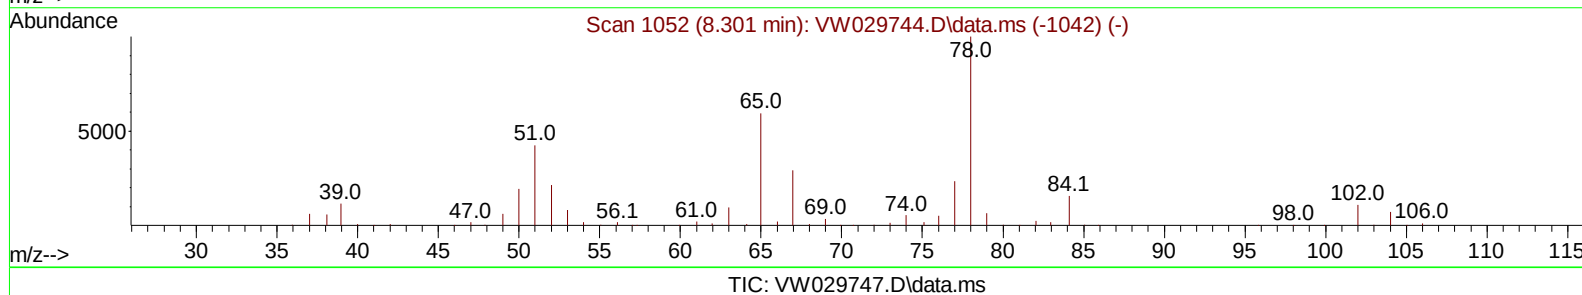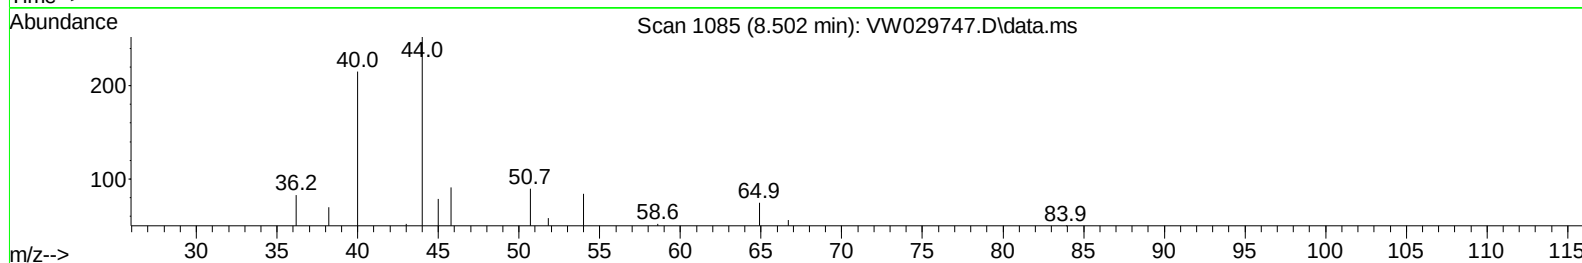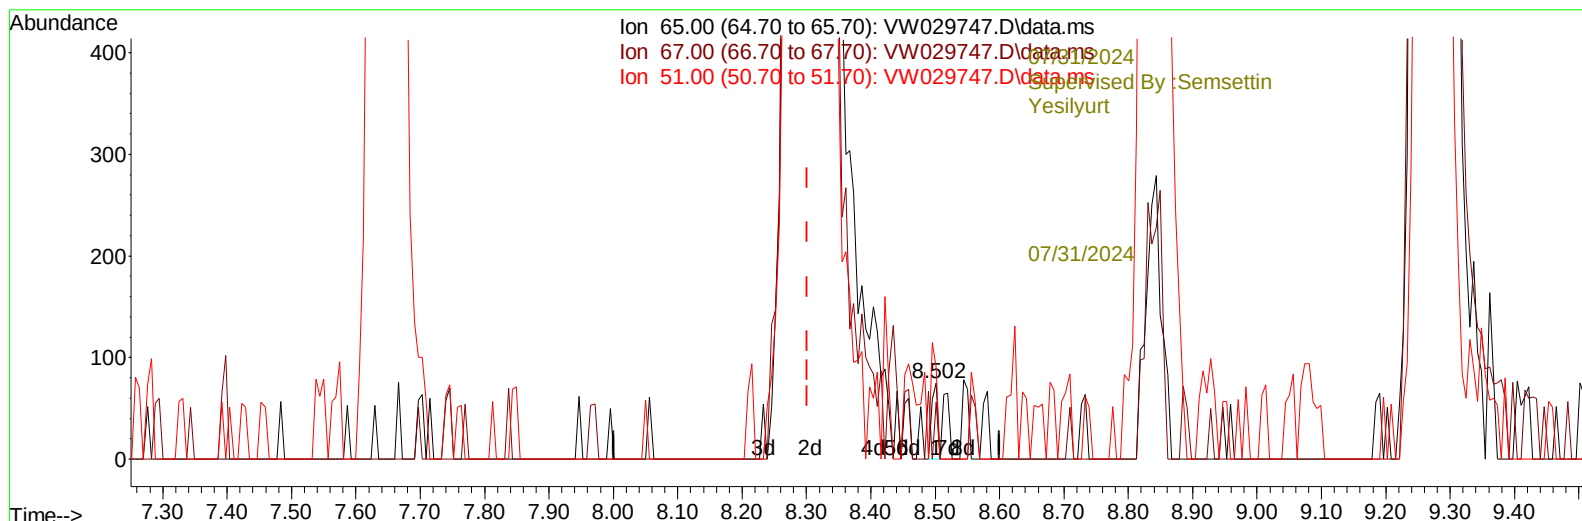

TIC: VW029747.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.502min (+ 0.201) 0.01 ug/L

response 49

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	51.02
51.00	120.50	153.06
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072624\
Data File : VW029747.D
Acq On : 26 Jul 2024 13:27
Operator : SY/MD
Sample : P3278-07
Misc : 9.10g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1ZQ3

Manual IntegrationsAPPROVED

Quant Time: Jul 27 00:54:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 27 00:53:25 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

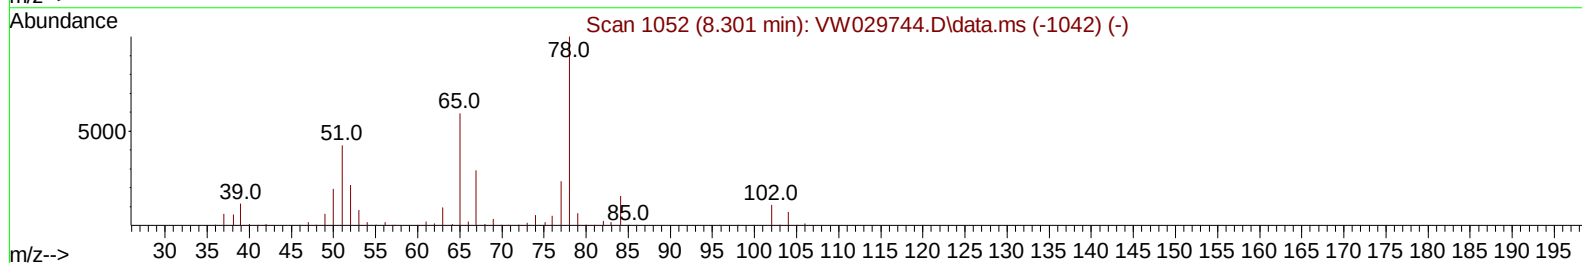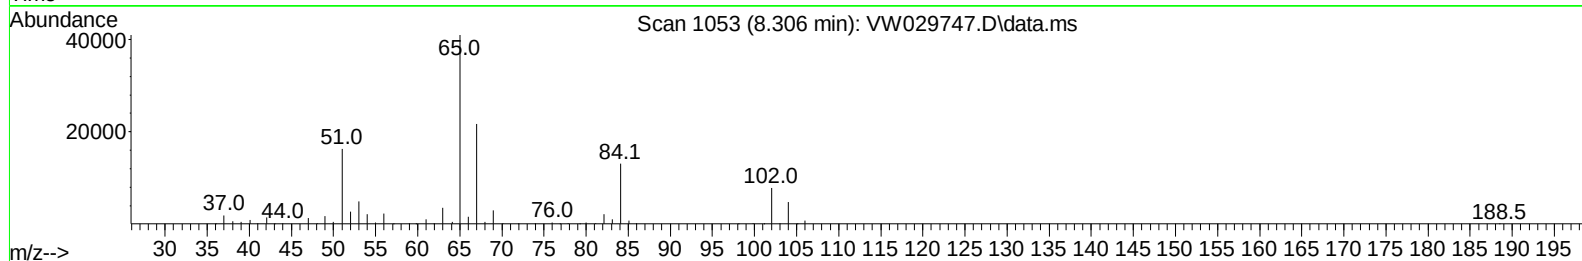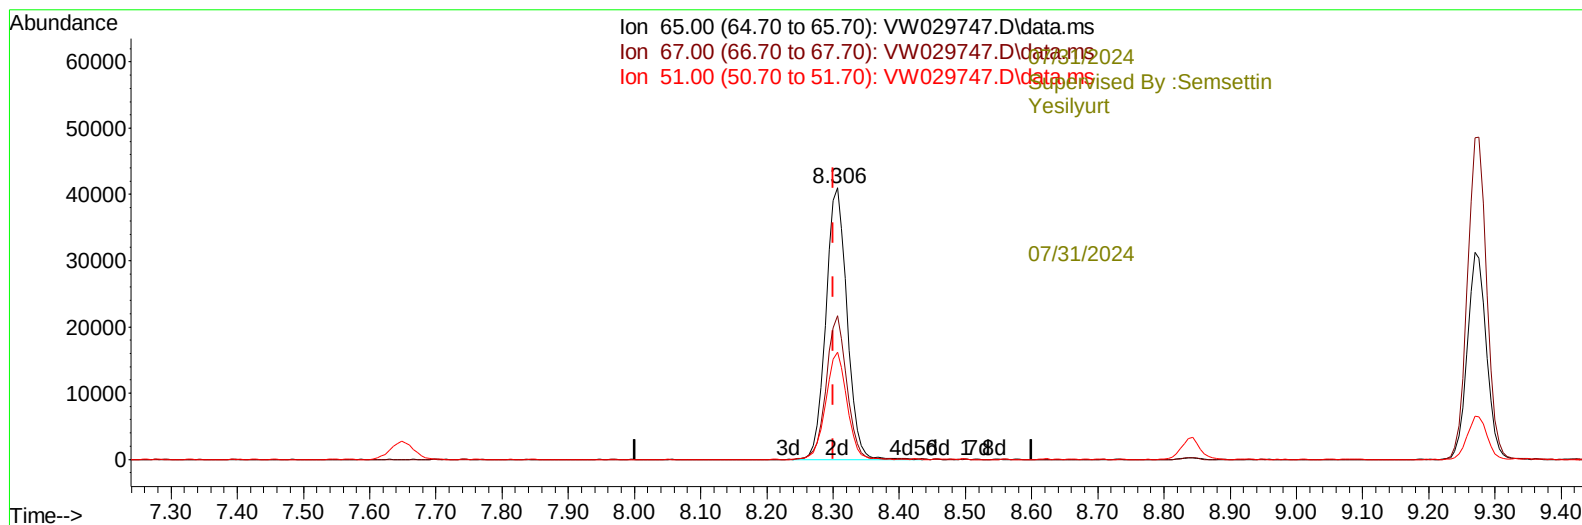

TIC: VW029747.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.306min (+ 0.006) 24.10 ug/L m

response 90853

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.03#
51.00	120.50	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072624\
 Data File : VW029747.D
 Acq On : 26 Jul 2024 13:27
 Operator : SY/MD
 Sample : P3278-07
 Misc : 9.10g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E1ZQ3

Manual IntegrationsAPPROVED

Quant Time: Jul 27 00:54:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 27 00:53:25 2024
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----07/31/2024							
Supervised By :Semsettin							
Yesilyurt							
Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		255722	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		240759	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.549	152		107535	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		72931	20.089	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.360%	
7) Chloroethane-d5	2.899	69		56368	21.748	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.000%	
11) 1,1-Dichloroethene-d2	4.021	65		34519	20.830	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.320%	
21) 2-Butanone-d5	7.081	46		42764m	42.977	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.960%	
24) Chloroform-d	7.648	84		154321	23.312	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.240%	
26) 1,2-Dichloroethane-d4	8.306	65		90853m	24.096	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.400%	
32) Benzene-d6	8.270	84		297774	22.890	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.560%	
36) 1,2-Dichloropropane-d6	9.276	67		98401	23.690	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.760%	
41) Toluene-d8	10.324	98		261974	22.649	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.600%	
43) trans-1,3-Dichloroprop...	10.574	79		37161	22.109	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.440%	
47) 2-Hexanone-d5	10.922	63		26731	39.028	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.060%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		70751	22.940	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.760%	
66) 1,2-Dichlorobenzene-d4	13.848	152		84022	25.164	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.640%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072624\
Data File : VW029747.D
Acq On : 26 Jul 2024 13:27
Operator : SY/MD
Sample : P3278-07
Misc : 9.10g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1ZQ3

Manual IntegrationsAPPROVED

Quant Time: Jul 27 00:54:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 27 00:53:25 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

