

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072722\
 Data File : VW024112.D
 Acq On : 27 Jul 2022 10:47
 Operator : SY/VA
 Sample : N3745-07
 Misc : 5.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jul 27 15:06:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	224006	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	228354	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	102074	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	115733	24.103	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.400%
7) Chloroethane-d5	2.873	69	78721	24.265	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.040%
11) 1,1-Dichloroethene-d2	4.013	63	72557	17.161	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.640%
21) 2-Butanone-d5	7.080	46	37793	44.288	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.580%
24) Chloroform-d	7.647	84	137013	22.248	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	8.305	65	82239	23.244	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.960%
32) Benzene-d6	8.268	84	253814	23.927	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.720%
36) 1,2-Dichloropropane-d6	9.274	67	79490	23.758	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.040%
41) Toluene-d8	10.323	98	240012	22.624	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.480%
43) trans-1,3-Dichloroprop...	10.573	79	31884	21.492	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.960%
47) 2-Hexanone-d5	10.926	63	29515	42.195	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.400%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	76148	19.724	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	78.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	84594	25.590	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.360%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	2939	0.605	ug/L	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072722\
Data File : VW024112.D
Acq On : 27 Jul 2022 10:47
Operator : SY/VA
Sample : N3745-07
Misc : 5.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Jul 27 15:06:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

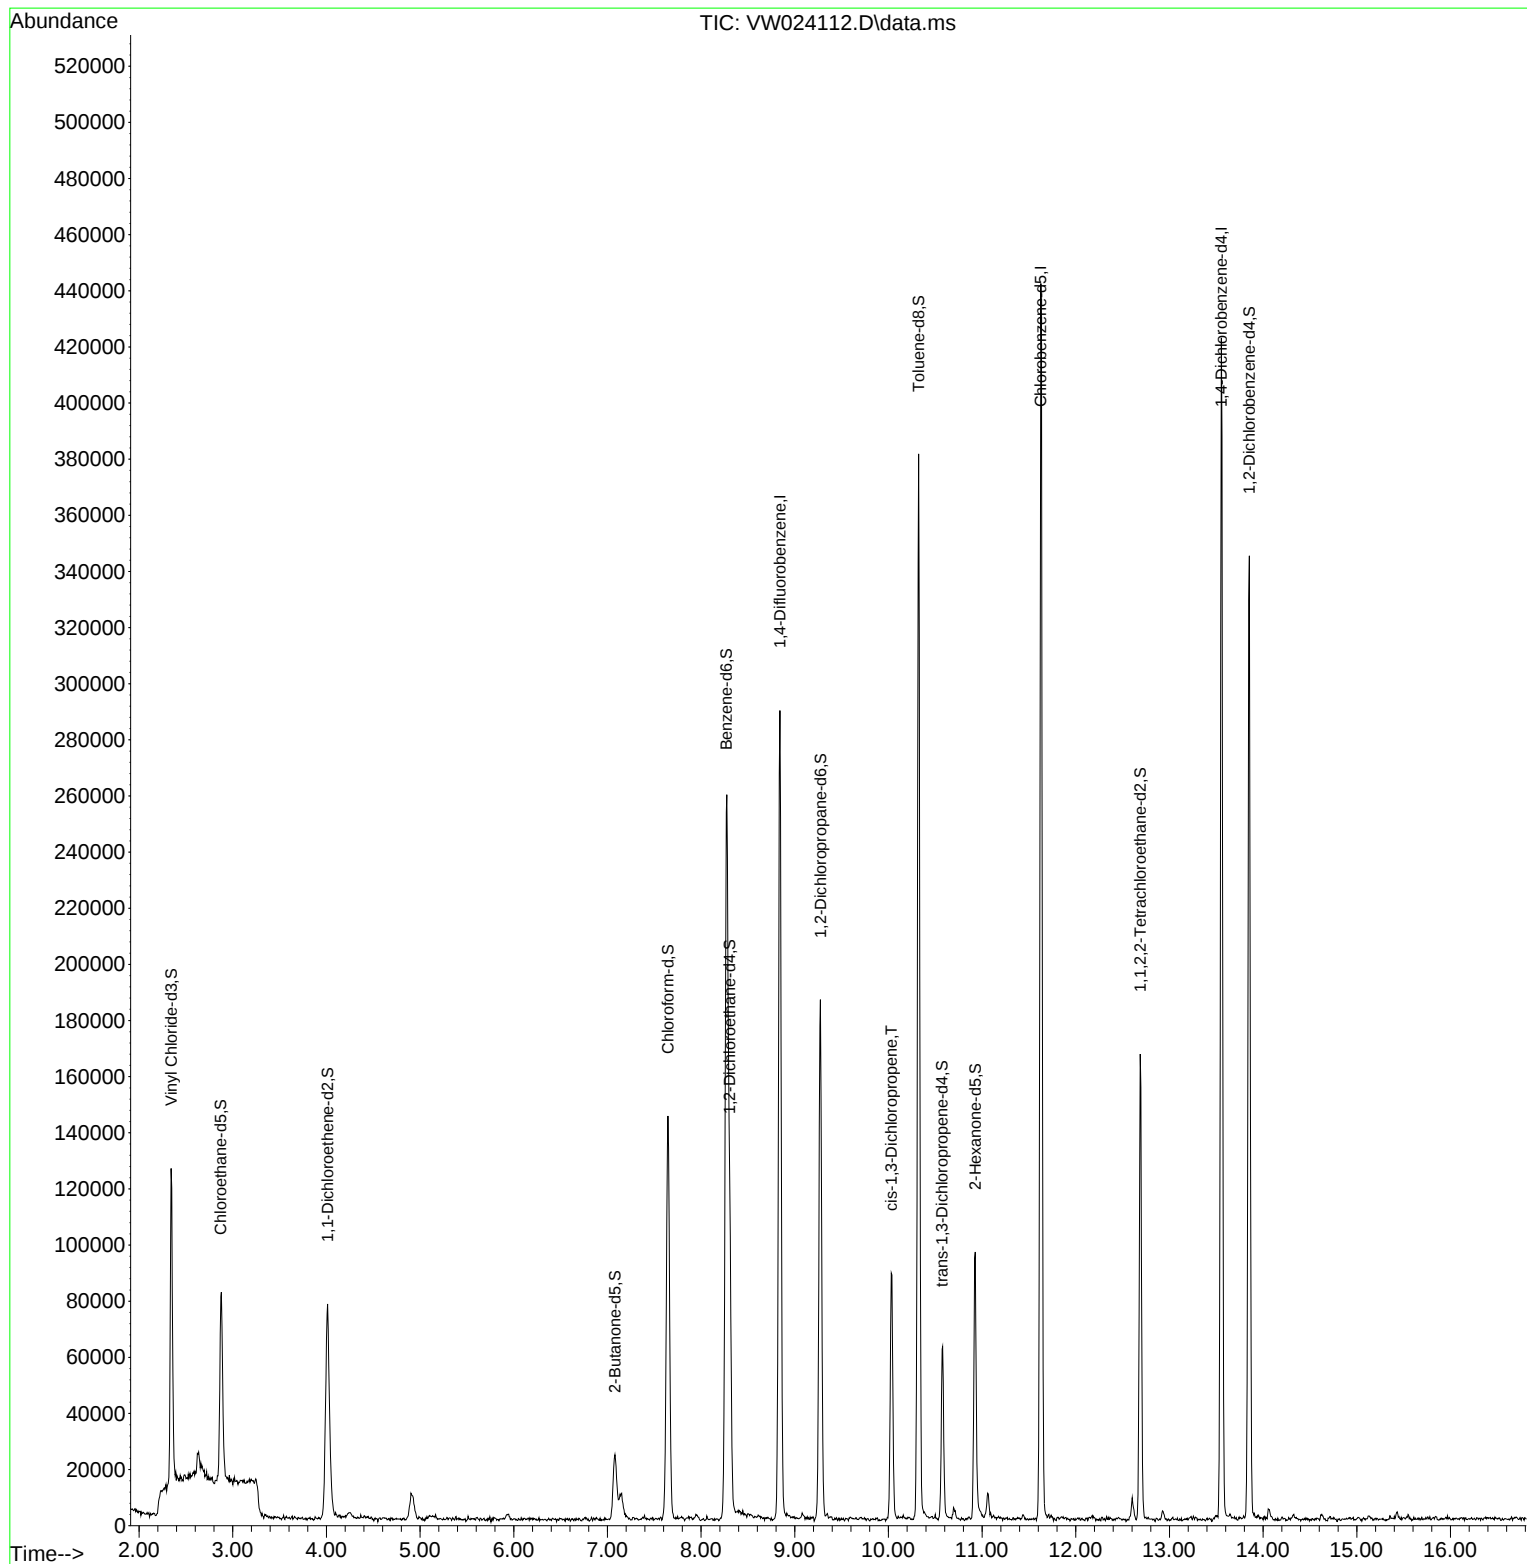

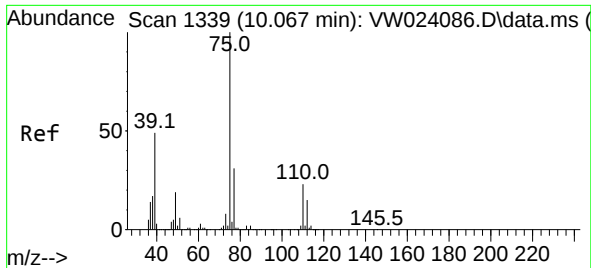

#39

cis-1,3-Dichloropropene

Concen: 0.605 ug/L

RT: 10.030 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW024112.D

Acq: 27 Jul 2022 10:47

Instrument :

MSVOA_W

ClientSampleId :

VHBLK001

Tgt Ion: 75 Resp: 2939

Ion Ratio Lower Upper

75 100

77 42.1 21.8 40.6#

