




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072722\
 Data File : VW024113.D
 Acq On : 27 Jul 2022 11:11
 Operator : SY/VA
 Sample : N3766-05
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/28/2022
 Supervised By :Semsettin Yesilyurt 07/28/2022

Quant Time: Jul 28 02:49:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

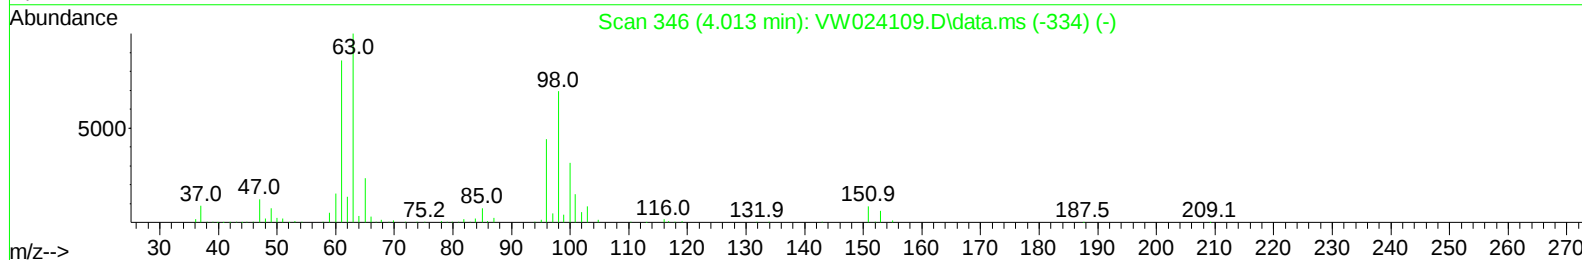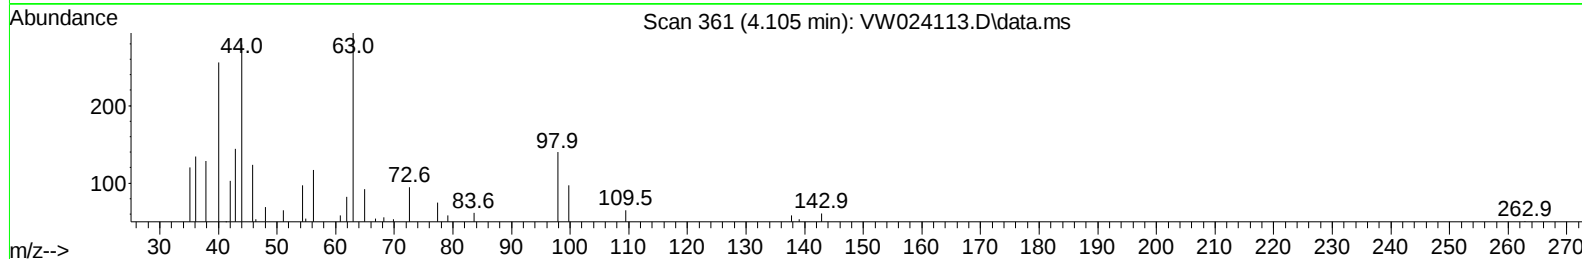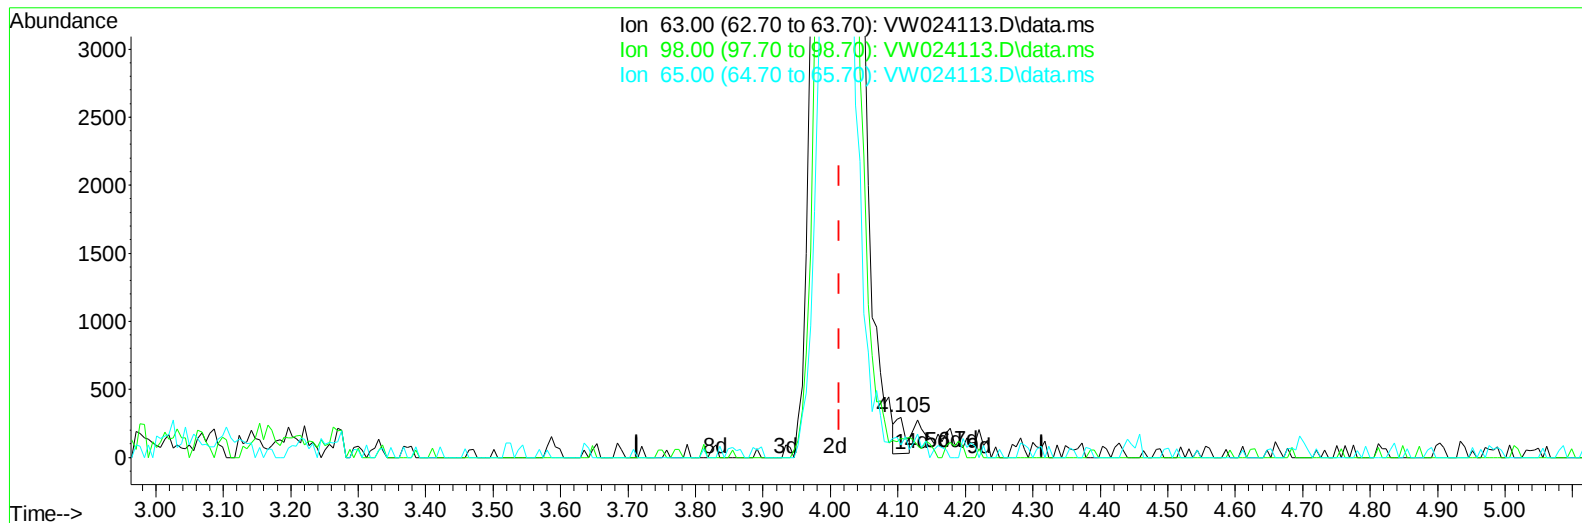

TIC: VW024113.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.105min (+ 0.091) 0.07 ug/L

response 271

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.10	66.05
65.00	23.20	29.15
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072722\
 Data File : VW024113.D
 Acq On : 27 Jul 2022 11:11
 Operator : SY/VA
 Sample : N3766-05
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/28/2022
 Supervised By :Semsettin Yesilyurt 07/28/2022

Quant Time: Jul 28 02:49:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

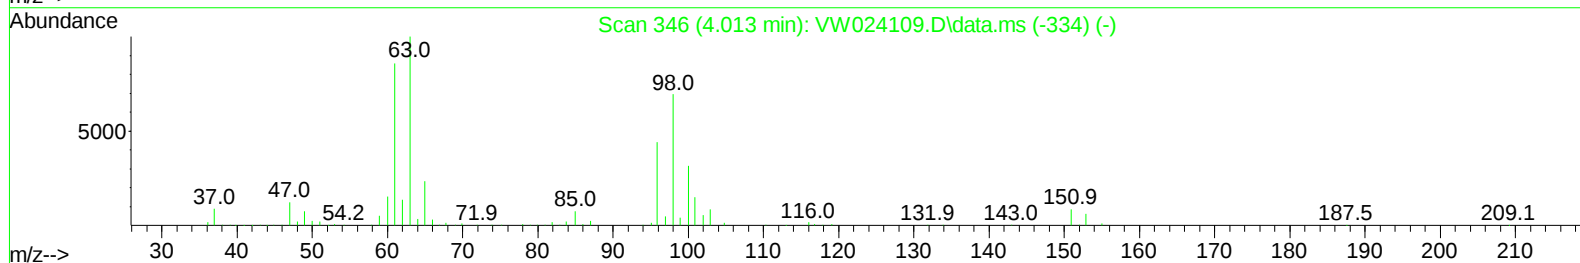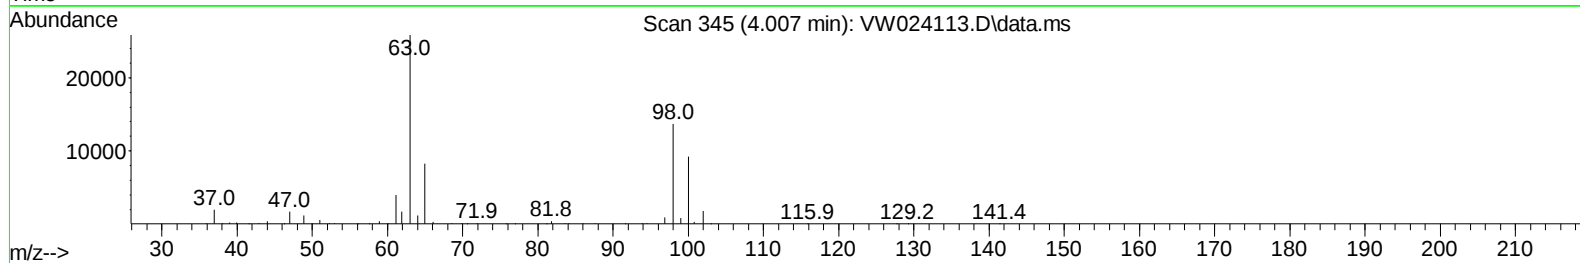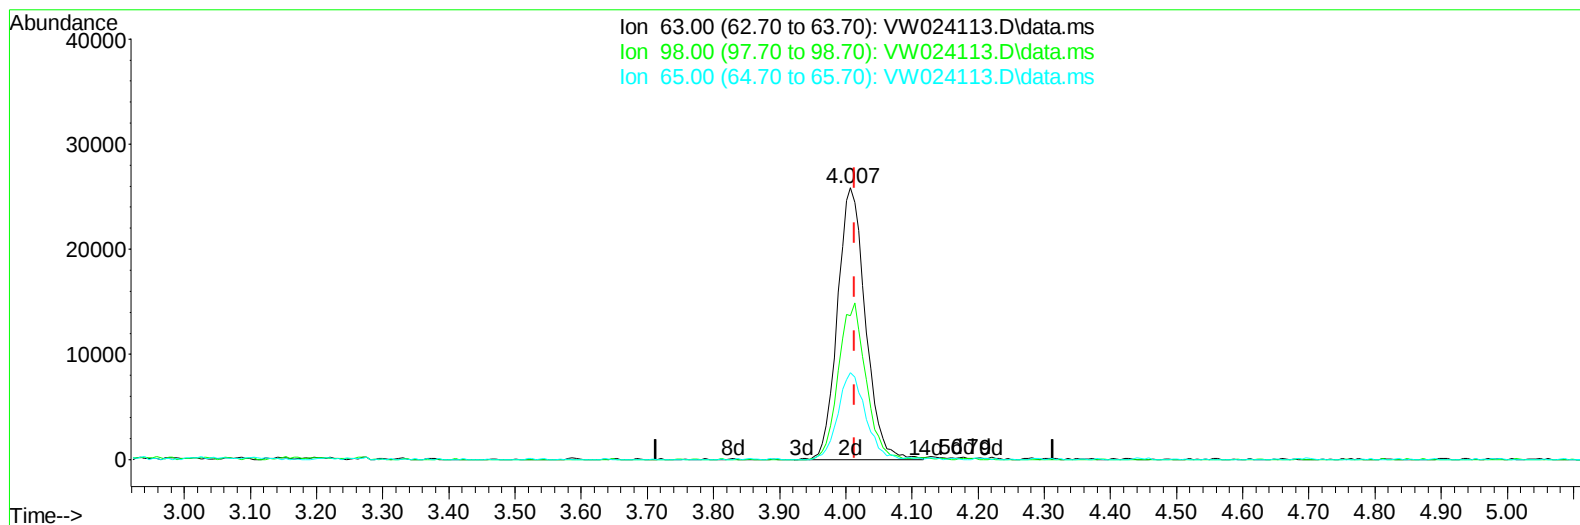

TIC: VW024113.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.007min (-0.006) 18.18 ug/L m

response 75737

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.10	0.24#
65.00	23.20	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072722\
 Data File : VW024113.D
 Acq On : 27 Jul 2022 11:11
 Operator : SY/VA
 Sample : N3766-05
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/28/2022
 Supervised By :Semsettin Yesilyurt 07/28/2022

Quant Time: Jul 28 02:49:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		220724	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		228748	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		97852	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		124508	26.316	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	105.280%	
7) Chloroethane-d5	2.873	69		76873	24.047	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	96.200%	
11) 1,1-Dichloroethene-d2	4.007	63		75737m	18.180	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	72.720%	
21) 2-Butanone-d5	7.080	46		39123	46.528	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	93.060%	
24) Chloroform-d	7.641	84		145133	23.917	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	95.680%	
26) 1,2-Dichloroethane-d4	8.305	65		86889	24.923	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	99.680%	
32) Benzene-d6	8.268	84		271749	25.574	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	102.280%	
36) 1,2-Dichloropropane-d6	9.268	67		83025	24.771	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	99.080%	
41) Toluene-d8	10.323	98		257682	24.248	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	97.000%	
43) trans-1,3-Dichloroprop...	10.573	79		34318	23.093	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	92.360%	
47) 2-Hexanone-d5	10.920	63		31054	44.319	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	88.640%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		82176	21.249	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	85.000%	
66) 1,2-Dichlorobenzene-d4	13.853	152		82782	26.122	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	104.480%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072722\
Data File : VW024113.D
Acq On : 27 Jul 2022 11:11
Operator : SY/VA
Sample : N3766-05
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/28/2022
Supervised By :Semsettin Yesilyurt 07/28/2022

Quant Time: Jul 28 02:49:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

