

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072924\
 Data File : VW029782.D
 Acq On : 29 Jul 2024 11:48
 Operator : SY/MD
 Sample : VW0729SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 30 06:55:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 30 06:26:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	225774	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	218816	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	90977	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	64215	20.034	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.120%
7) Chloroethane-d5	2.899	69	51604	22.551	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	4.021	65	30201	20.641	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	82.560%
21) 2-Butanone-d5	7.075	46	36806	41.896	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.800%
24) Chloroform-d	7.648	84	141878	24.275	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.120%
26) 1,2-Dichloroethane-d4	8.301	65	85419	25.660	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.640%
32) Benzene-d6	8.276	84	269254	22.774	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.080%
36) 1,2-Dichloropropane-d6	9.276	67	90606	24.001	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.000%
41) Toluene-d8	10.325	98	233781	22.238	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.960%
43) trans-1,3-Dichloroprop...	10.575	79	33634	22.017	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.080%
47) 2-Hexanone-d5	10.922	63	24180	38.844	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.680%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	64497	23.009	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.040%
66) 1,2-Dichlorobenzene-d4	13.849	152	74294	26.300	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.200%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2580	0.431	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072924\
Data File : VW029782.D
Acq On : 29 Jul 2024 11:48
Operator : SY/MD
Sample : VW0729SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jul 30 06:55:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 30 06:26:05 2024
Response via : Initial Calibration

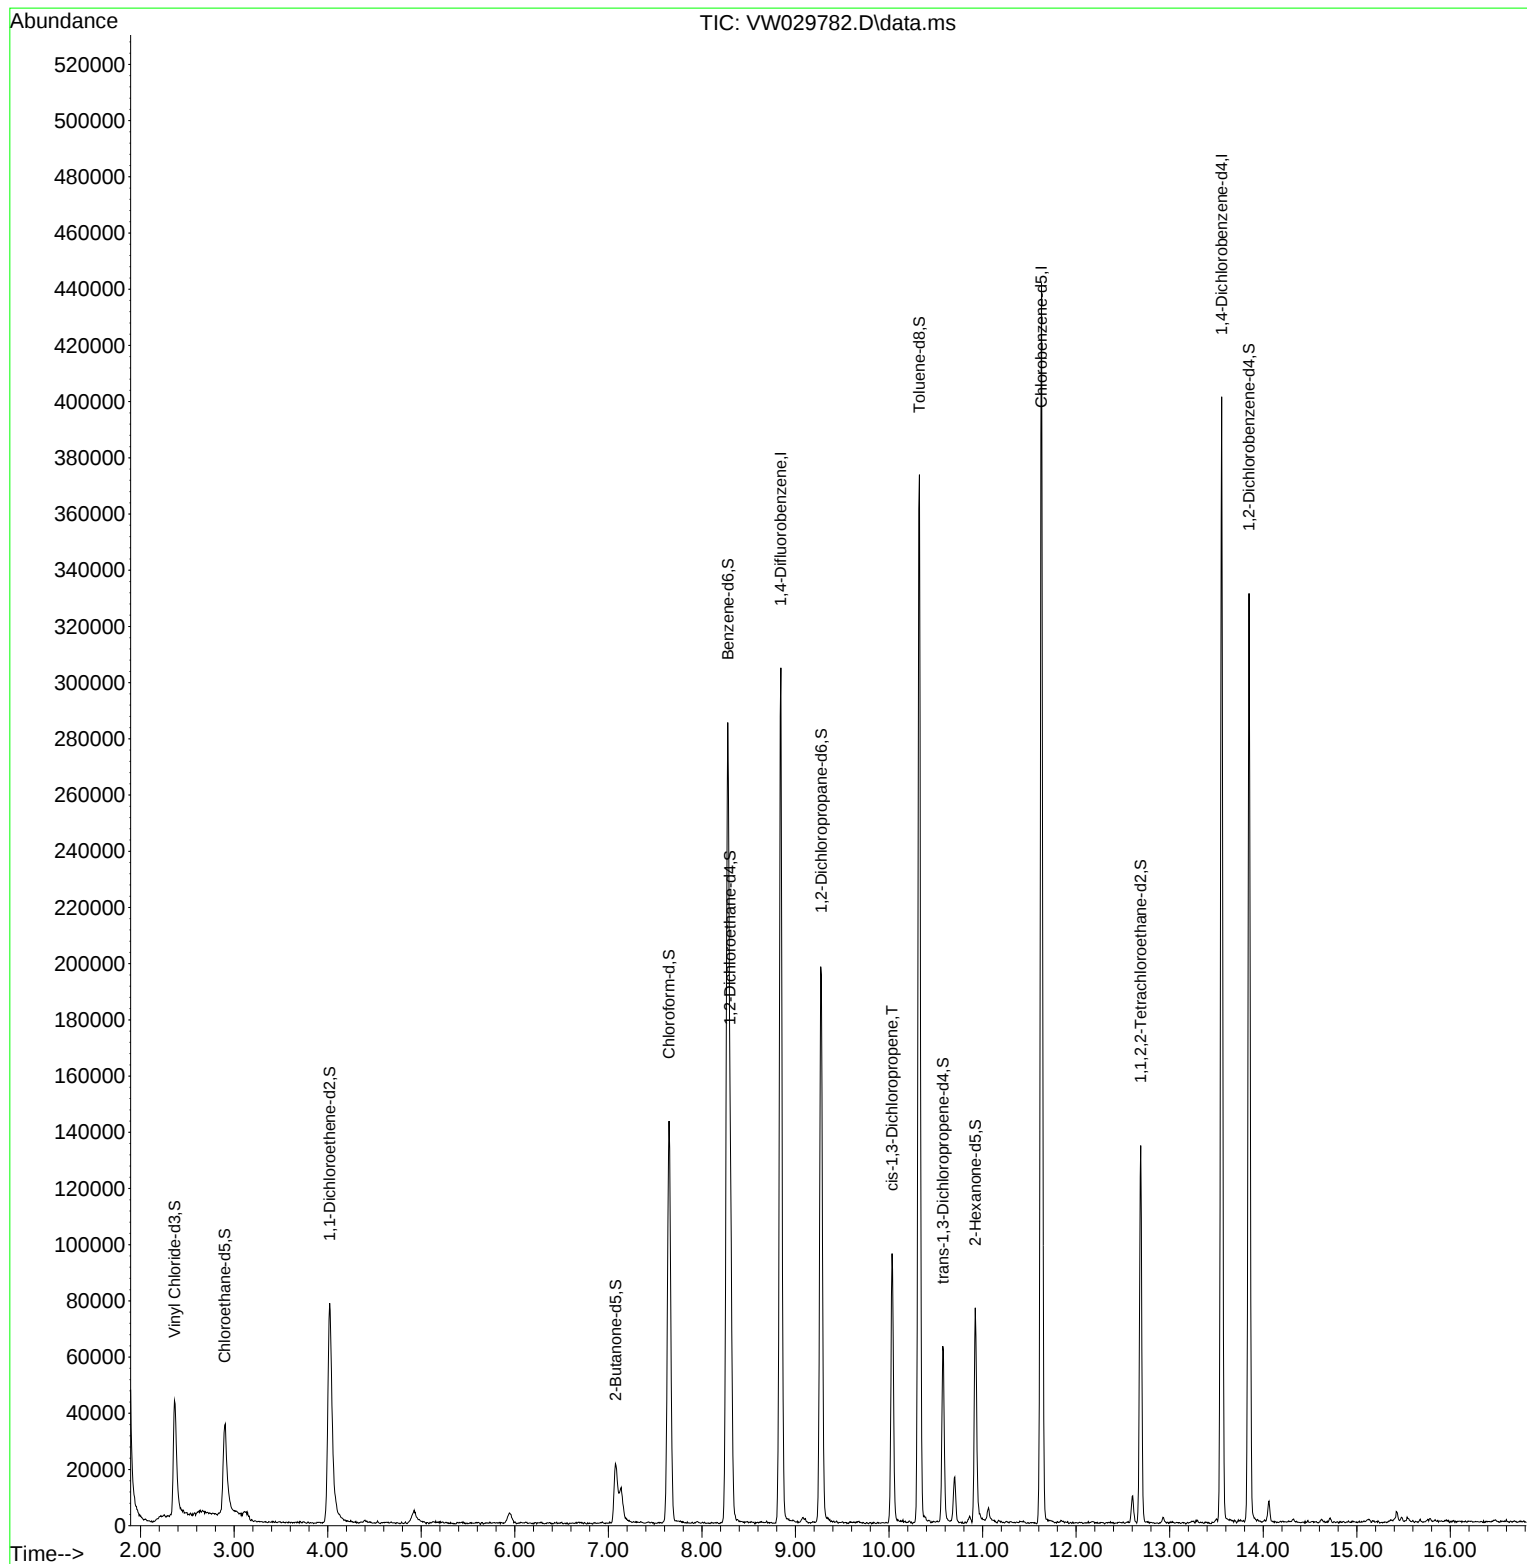

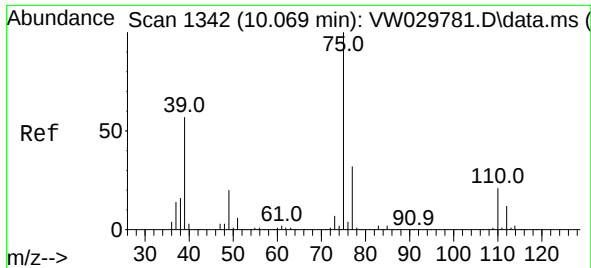

#39
 cis-1,3-Dichloropropene
 Concen: 0.431 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029782.D
 Acq: 29 Jul 2024 11:48

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 2580
 Ion Ratio Lower Upper
 75 100
 77 41.9 20.8 38.6#

