

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072924\
 Data File : VW029784.D
 Acq On : 29 Jul 2024 12:45
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 30 06:55:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 30 06:26:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	251489	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	238262	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	104517	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	60882	17.052	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.200%
7) Chloroethane-d5	2.899	69	48383	18.981	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.920%
11) 1,1-Dichloroethene-d2	4.021	65	29687	18.215	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.880%
21) 2-Butanone-d5	7.075	46	39586	40.453	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.900%
24) Chloroform-d	7.648	84	134312	20.631	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.520%
26) 1,2-Dichloroethane-d4	8.307	65	81447	21.965	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.840%
32) Benzene-d6	8.276	84	255051	19.812	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.240%
36) 1,2-Dichloropropane-d6	9.270	67	87407	21.263	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.040%
41) Toluene-d8	10.325	98	227124	19.842	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.360%
43) trans-1,3-Dichloroprop...	10.575	79	32825	19.734	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.920%
47) 2-Hexanone-d5	10.922	63	25205	37.186	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.380%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	66300	21.722	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	72933	22.473	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.880%
Target Compounds						
					Qvalue	
16) Methylene chloride	4.923	84	21216	4.035	ug/L	94
39) cis-1,3-Dichloropropene	10.032	75	2465	0.378	ug/L #	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072924\
Data File : VW029784.D
Acq On : 29 Jul 2024 12:45
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jul 30 06:55:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 30 06:26:05 2024
Response via : Initial Calibration

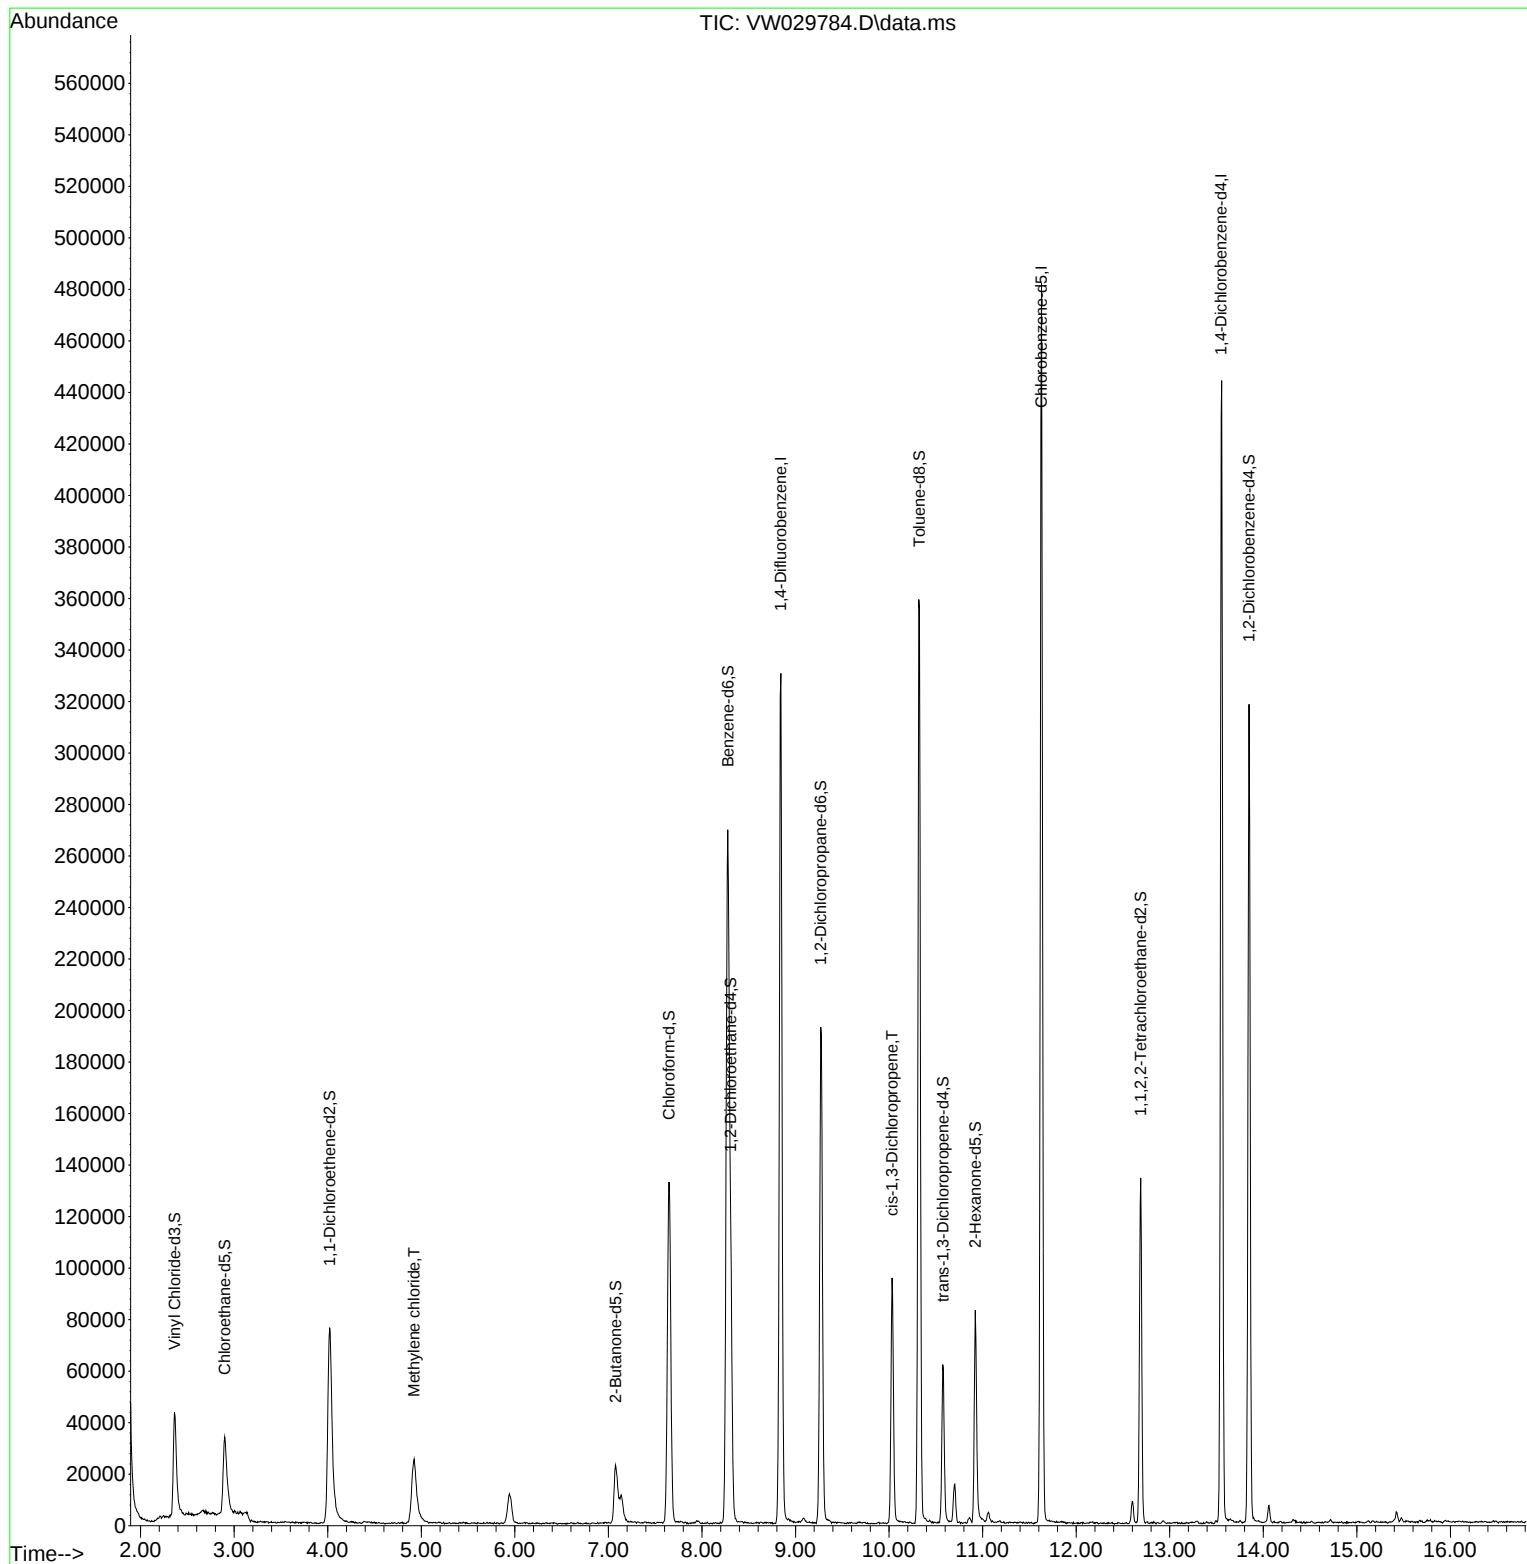



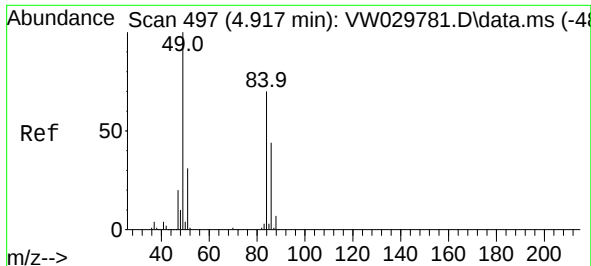


#16
Methylene chloride
Concen: 4.035 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW029784.D
Acq: 29 Jul 2024 12:45

Instrument :
MSVOA_W
ClientSampleId :

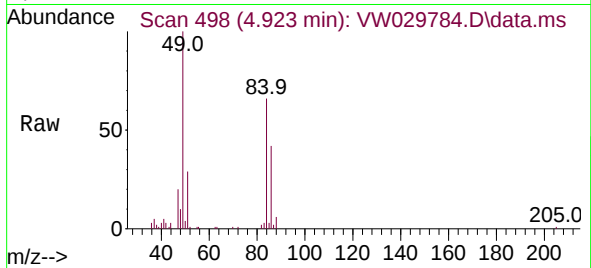

Tgt Ion: 84 Resp: 21216
Ion Ratio Lower Upper
84 100
86 63.8 44.7 82.9
49 152.1 99.0 184.0

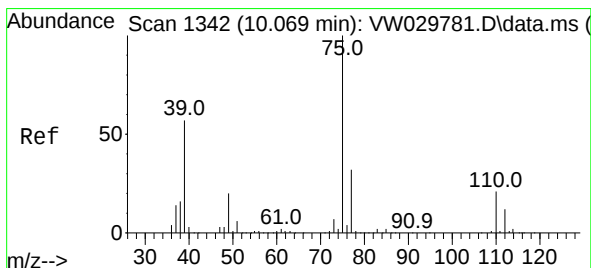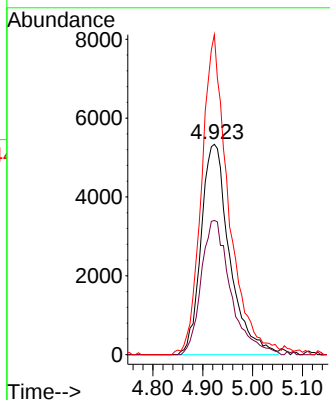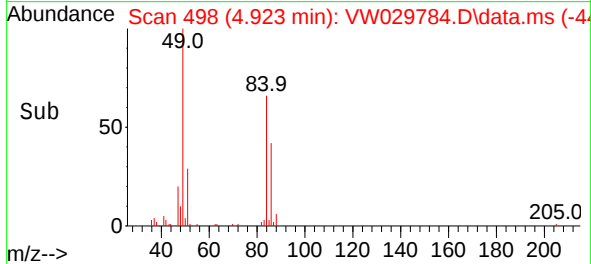

#39
cis-1,3-Dichloropropene
Concen: 0.378 ug/L
RT: 10.032 min Scan# 1336
Delta R.T. -0.037 min
Lab File: VW029784.D
Acq: 29 Jul 2024 12:45

Tgt Ion: 75 Resp: 2465
Ion Ratio Lower Upper
75 100
77 43.6 20.8 38.6#

