


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW073118\
 Data File : VW004357.D
 Acq On : 31 Jul 2018 14:13
 Operator : SY/AP
 Sample : BFB89
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB89

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073118S.M
 Title : VOC Analysis
 Last Update : Tue Jul 31 20:28:54 2018

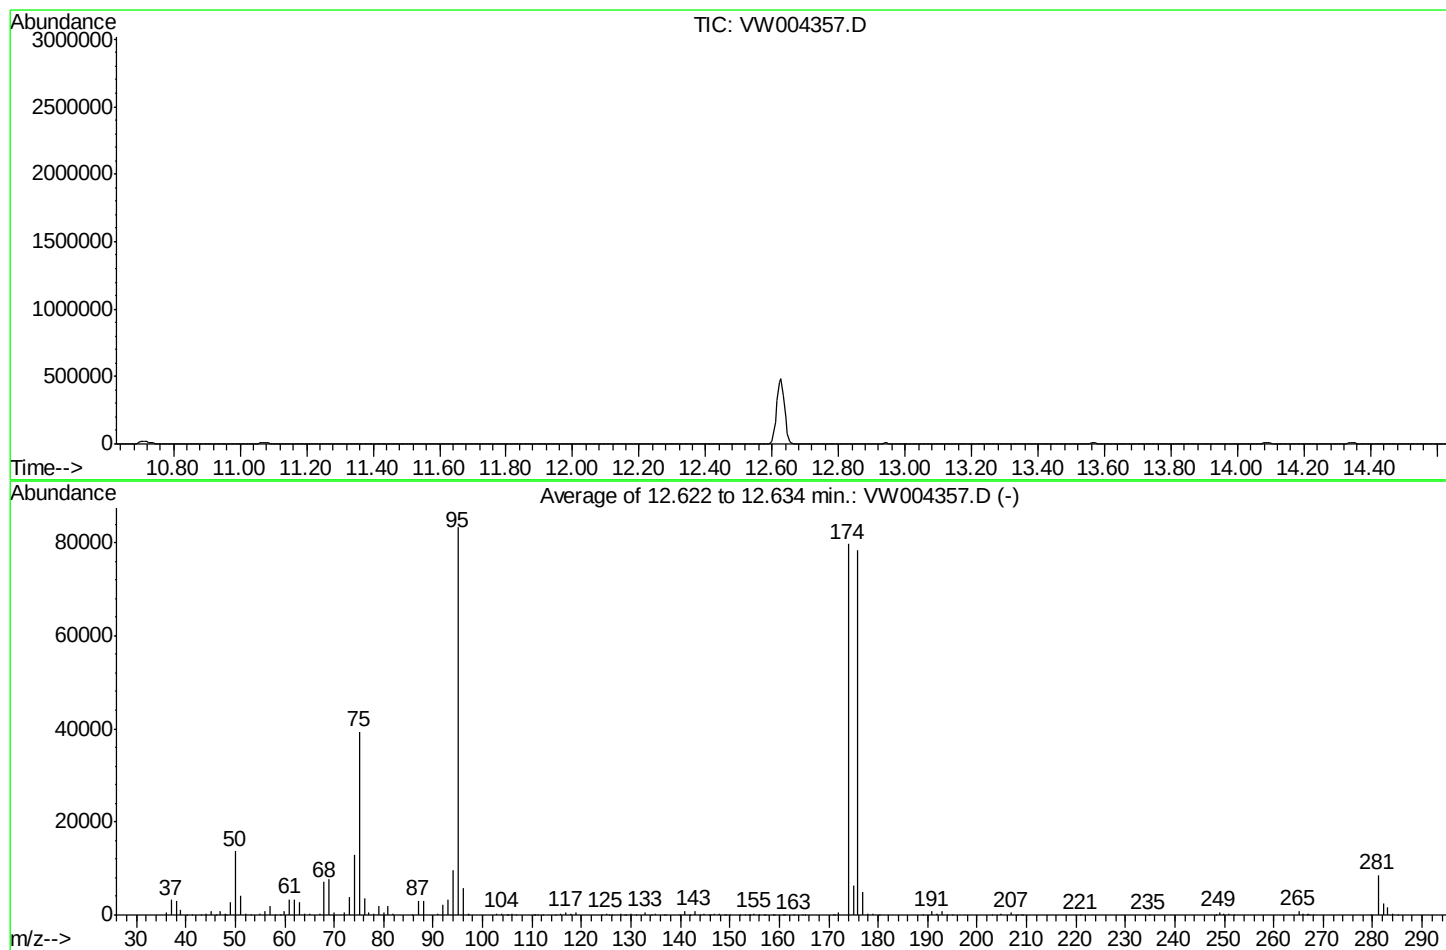

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	13632	PASS
75	95	30	80	47.4	39434	PASS
95	95	100	100	100.0	83280	PASS
96	95	5	9	6.8	5695	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	95.7	79690	PASS
175	174	5	9	8.0	6362	PASS
176	174	95	101	98.5	78485	PASS
177	176	5	9	6.4	5061	PASS

Scan 1802 (12.573 min): VW004357.D
BFB89

m/z	Abundance
39.90	113.0
44.10	73.0
69.90	64.0
207.10	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

m/z	Abundance
36.00	725.0
37.00	3609.0
38.00	3436.0
39.00	1466.0
40.10	108.0
42.90	52.0
43.90	505.0
45.00	794.0
46.20	99.0
47.10	1101.0
47.80	480.0
49.00	3152.0
50.00	14893.0
51.00	4574.0
52.00	227.0
53.10	83.0
54.90	273.0
55.90	1213.0
57.00	2227.0
57.90	64.0
59.90	1037.0
61.00	3916.0
62.00	3803.0
63.10	3075.0
63.90	380.0
65.00	459.0
67.00	413.0
68.00	8213.0
69.00	8604.0
70.00	784.0
72.00	568.0
73.00	4952.0
74.00	14225.0
75.00	43840.0
76.00	3669.0
77.10	537.0
77.90	303.0
78.90	2108.0
80.00	611.0
80.90	2006.0
81.90	419.0
85.80	116.0
86.90	2927.0
87.90	2934.0
91.00	437.0
92.00	2486.0
93.00	4022.0
94.00	10175.0
95.00	85976.0
96.00	6185.0
97.00	284.0
102.80	213.0
104.00	484.0
104.80	141.0
105.80	265.0
106.80	71.0
110.20	77.0
110.80	130.0
112.20	69.0
114.80	122.0
115.80	330.0
117.00	675.0
117.90	347.0
118.90	555.0
124.10	79.0
125.10	555.0
125.60	160.0
126.10	130.0
128.00	416.0
128.70	139.0
129.90	375.0
130.90	143.0
133.00	726.0
135.00	194.0
136.80	124.0
140.90	882.0
141.80	144.0
142.90	978.0
144.90	247.0
145.90	200.0
147.00	281.0
147.80	286.0
148.80	93.0
152.00	67.0
153.00	58.0
153.90	58.0
155.00	334.0
156.90	204.0
158.70	95.0
161.10	238.0
163.00	195.0
164.70	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

171.00	175.0
171.90	603.0
173.90	75720.0
175.00	6502.0
175.90	77192.0
176.90	4714.0
178.00	164.0
178.90	184.0
180.30	55.0
189.10	101.0
190.90	986.0
191.90	371.0
193.00	984.0
194.10	181.0
195.00	102.0
203.10	76.0
204.90	279.0
207.00	738.0
208.10	146.0
208.90	83.0
220.90	57.0
234.80	168.0
248.90	736.0
249.80	250.0
251.00	382.0
251.90	63.0
265.10	1293.0
266.00	466.0
267.00	328.0
268.00	79.0
279.60	120.0
281.10	11261.0
282.00	3040.0
283.00	1810.0
284.00	352.0
285.00	121.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

m/z	Abundance
35.90	604.0
37.00	3515.0
38.00	3299.0
39.00	1218.0
40.10	96.0
41.10	85.0
44.00	444.0
45.00	866.0
46.90	722.0
47.90	595.0
49.10	3121.0
50.00	15076.0
51.00	5005.0
52.10	273.0
53.10	65.0
54.90	267.0
56.00	957.0
57.00	1959.0
58.00	164.0
59.00	54.0
60.00	846.0
61.00	3804.0
62.00	3717.0
63.00	3031.0
63.90	366.0
65.00	262.0
67.00	357.0
68.00	7519.0
69.00	8243.0
70.00	526.0
72.00	596.0
73.00	3686.0
74.00	14075.0
75.00	42816.0
76.00	4201.0
77.00	629.0
77.90	392.0
78.90	2191.0
80.00	663.0
80.90	2001.0
82.00	335.0
85.80	137.0
87.00	3512.0
88.00	3467.0
91.00	328.0
92.00	2447.0
92.90	3465.0
94.00	11322.0
95.00	93824.0
96.00	6540.0
97.00	274.0
102.90	195.0
103.90	361.0
105.10	168.0
105.80	259.0
106.80	62.0
110.60	93.0
111.10	119.0
114.90	165.0
115.90	303.0
116.80	621.0
118.00	443.0
118.90	452.0
124.00	96.0
124.90	289.0
125.60	80.0
126.10	91.0
127.80	404.0
128.90	231.0
129.90	357.0
130.90	151.0
132.90	751.0
134.10	169.0
135.00	191.0
137.00	103.0
140.90	1029.0
141.80	79.0
142.90	988.0
143.90	56.0
144.80	296.0
146.00	200.0
146.80	164.0
147.90	156.0
149.10	74.0
149.90	210.0
152.00	59.0
153.00	77.0
153.90	74.0
154.80	221.0
155.80	55.0
157.10	213.0
159.10	92.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

160.80	166.0
162.90	167.0
165.10	127.0
171.90	497.0
174.00	90312.0
175.00	7018.0
175.90	88912.0
176.90	5793.0
178.00	188.0
179.00	157.0
189.10	77.0
190.90	780.0
191.80	188.0
192.90	816.0
194.00	165.0
195.00	132.0
203.00	50.0
204.80	211.0
207.00	614.0
208.10	98.0
209.20	69.0
221.00	56.0
234.70	112.0
248.20	78.0
249.00	649.0
249.90	205.0
251.00	357.0
252.00	110.0
265.10	835.0
266.00	271.0
267.00	225.0
279.50	74.0
281.10	8685.0
282.10	2490.0
283.00	1655.0
284.10	221.0
284.90	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

m/z	Abundance
36.00	523.0
37.00	2510.0
38.00	2099.0
39.00	886.0
39.80	152.0
44.00	363.0
45.10	521.0
46.30	63.0
47.00	688.0
48.20	265.0
49.00	2264.0
50.00	10928.0
51.00	3117.0
51.90	108.0
55.00	106.0
55.90	641.0
57.00	1571.0
58.10	88.0
60.00	679.0
61.00	2593.0
62.00	2637.0
63.00	2085.0
64.00	236.0
64.90	146.0
68.00	5666.0
69.00	6169.0
70.10	493.0
72.10	456.0
73.00	2828.0
74.00	10385.0
75.00	31648.0
76.10	2796.0
76.90	398.0
77.00	392.0
77.90	301.0
78.90	1337.0
79.90	402.0
80.90	1431.0
81.90	324.0
85.90	94.0
87.00	2649.0
88.00	2307.0
91.00	268.0
92.00	1909.0
93.00	2574.0
94.00	7583.0
95.00	70040.0
96.10	4362.0
97.20	101.0
102.80	82.0
103.90	255.0
104.90	108.0
105.90	222.0
110.70	73.0
114.80	116.0
115.90	238.0
116.90	472.0
117.80	258.0
119.00	332.0
124.00	85.0
124.90	70.0
125.70	88.0
127.90	228.0
129.00	61.0
129.80	244.0
131.00	148.0
132.90	461.0
134.90	173.0
136.80	110.0
137.10	114.0
139.80	75.0
140.90	579.0
142.90	618.0
144.90	128.0
145.70	137.0
146.90	134.0
147.90	228.0
149.10	68.0
149.90	148.0
152.00	53.0
154.10	65.0
155.00	329.0
155.80	63.0
156.90	178.0
159.00	179.0
161.00	125.0
162.90	69.0
164.80	102.0
171.20	79.0
171.90	317.0
174.00	73040.0
175.00	5567.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

175.90	69352.0
176.90	4677.0
177.90	149.0
178.90	176.0
191.00	500.0
192.90	377.0
194.00	64.0
194.90	75.0
205.00	143.0
207.10	361.0
208.20	82.0
209.20	66.0
248.90	489.0
250.00	124.0
250.80	130.0
251.10	127.0
265.00	463.0
265.90	185.0
266.70	181.0
267.20	133.0
281.10	5999.0
282.20	1557.0
283.00	1236.0
284.00	244.0
285.00	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89