

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW073125\
 Data File : VW031969.D
 Acq On : 31 Jul 2025 15:42
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Quant Time: Aug 01 01:15:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W072225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 23 08:18:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.959	168	170284	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	365723	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.629	117	345087	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	158467	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	131899	51.204	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	102.400%
35) Dibromofluoromethane	7.898	113	122959	49.478	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	98.960%
50) Toluene-d8	10.325	98	430853	45.809	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	91.620%
62) 4-Bromofluorobenzene	12.617	95	145758	40.359	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	80.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW073125\
Data File : VW031969.D
Acq On : 31 Jul 2025 15:42
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Quant Time: Aug 01 01:15:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W072225S.M
Quant Title : SW846 8260
QLast Update : Wed Jul 23 08:18:46 2025
Response via : Initial Calibration




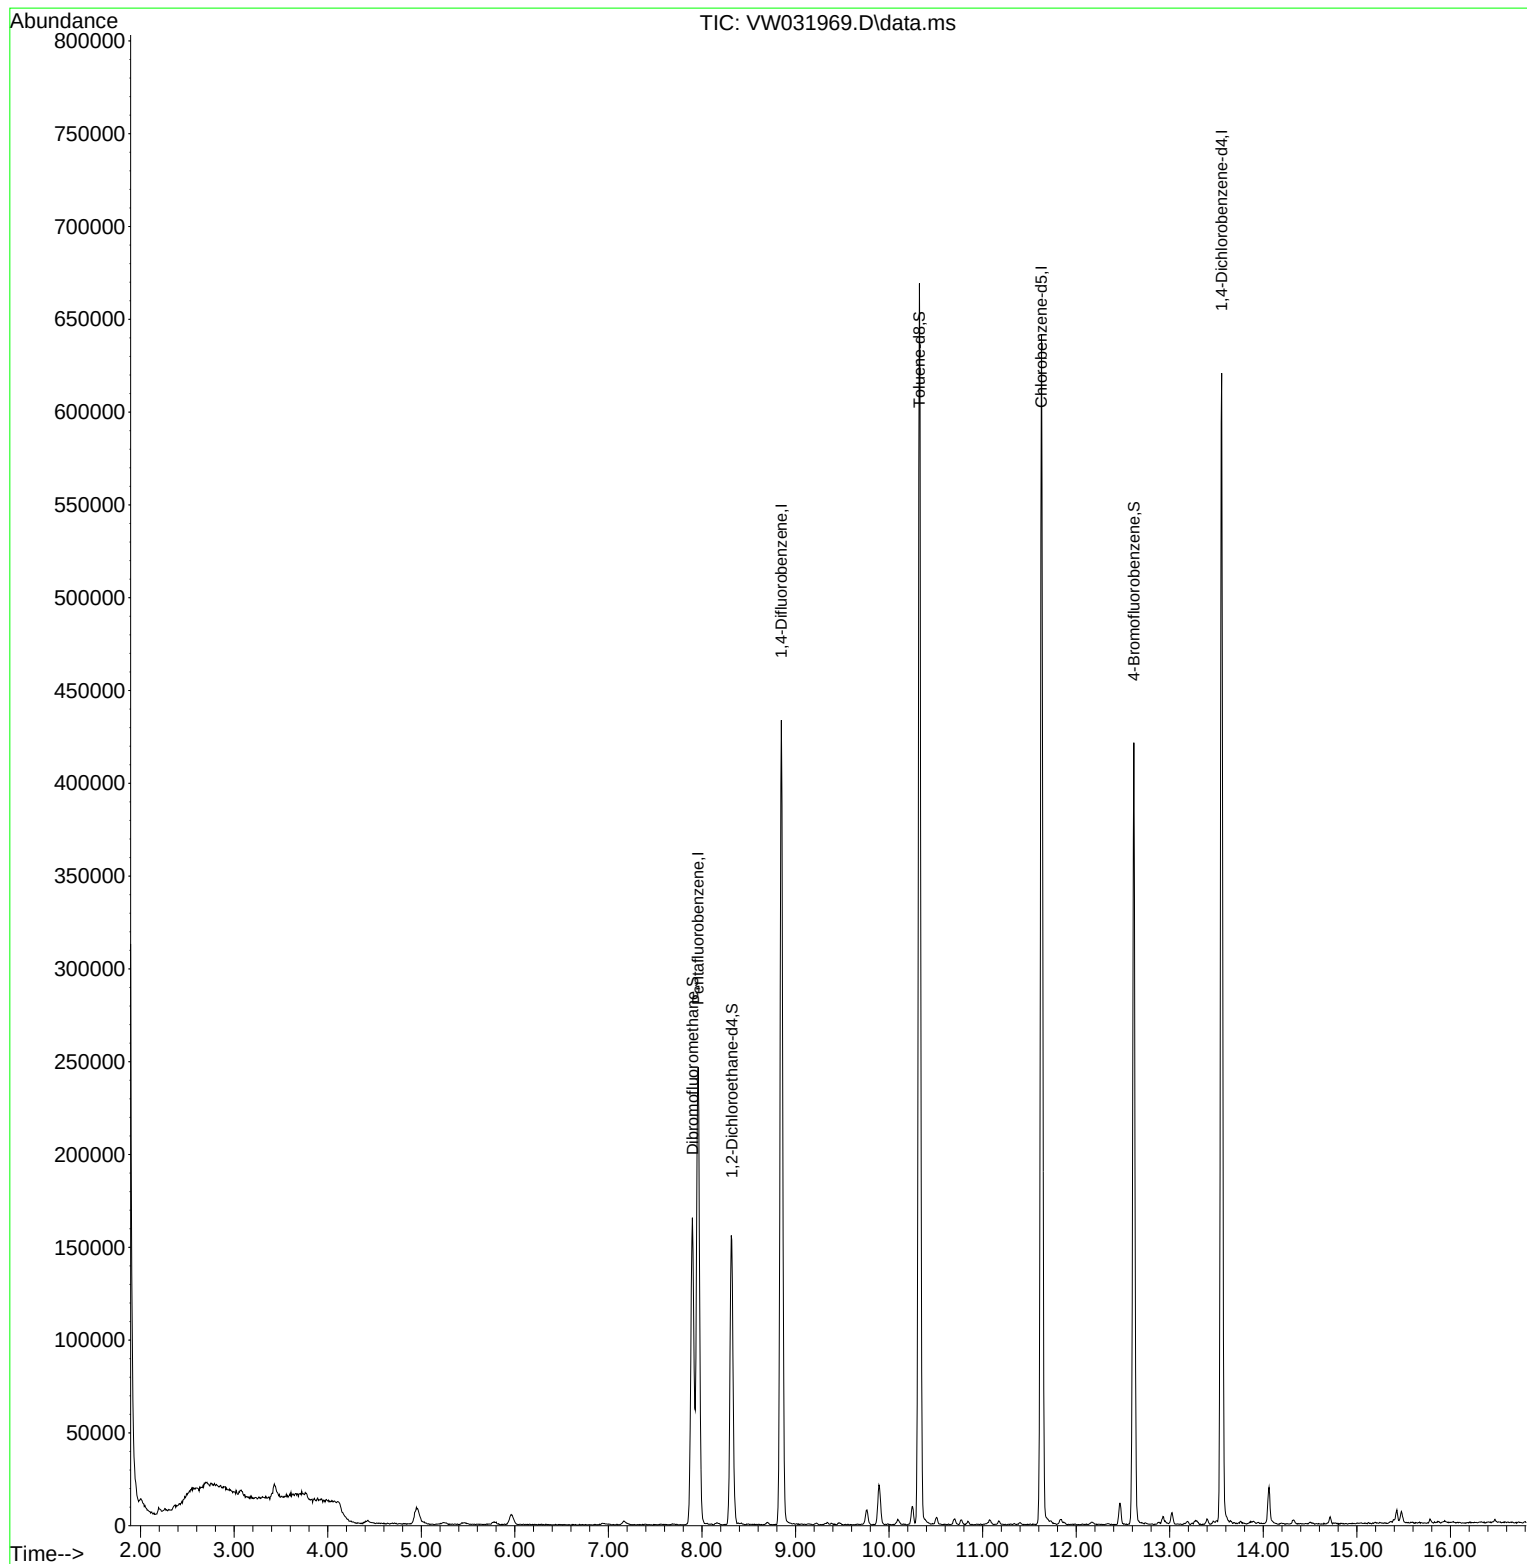


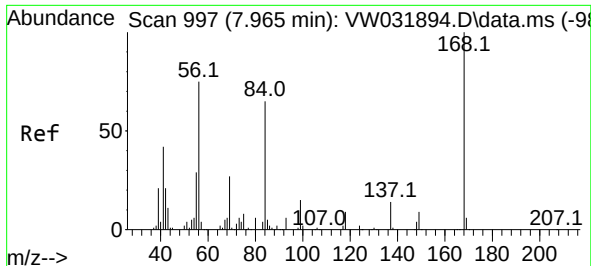

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.959 min Scan# 996
Delta R.T. -0.006 min
Lab File: VW031969.D
Acq: 31 Jul 2025 15:42




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 170284
Ion Ratio Lower Upper
168 100
99 71.7 48.2 72.2

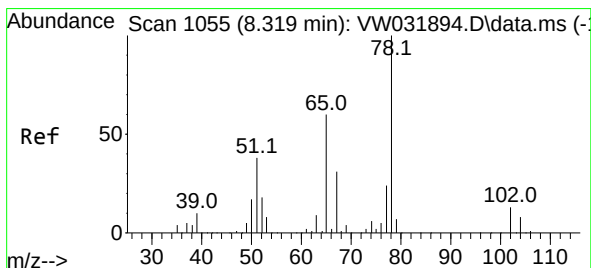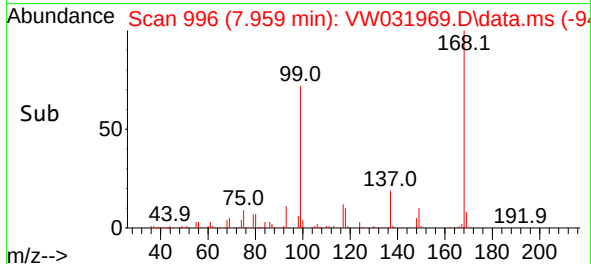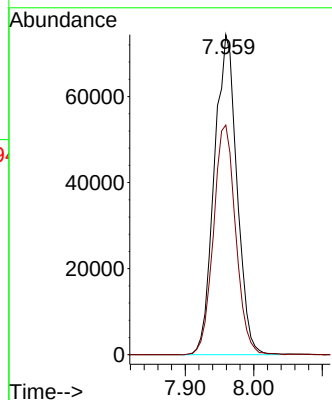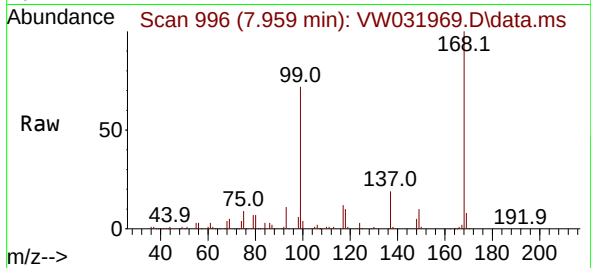

#33
1,2-Dichloroethane-d4
Concen: 51.204 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW031969.D
Acq: 31 Jul 2025 15:42

Tgt Ion: 65 Resp: 131899
Ion Ratio Lower Upper
65 100
67 50.8 0.0 101.4

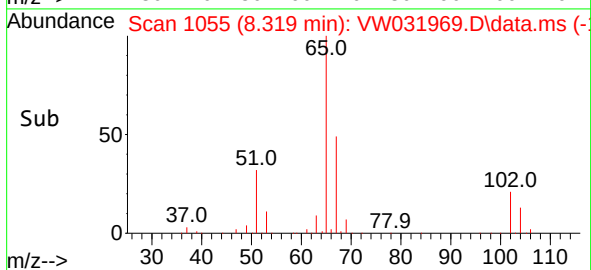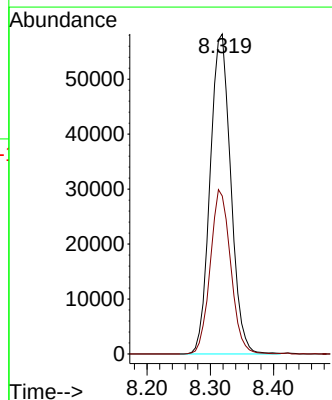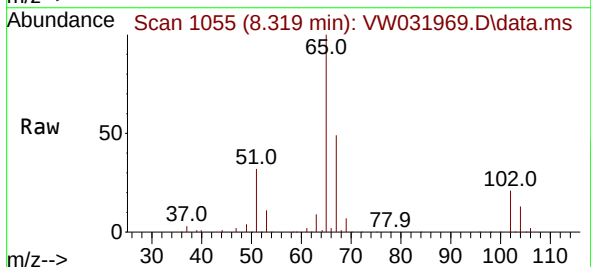

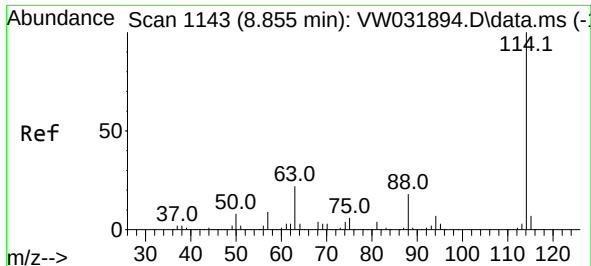

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.849 min Scan# 1143

Delta R.T. -0.006 min

Lab File: VW031969.D

Acq: 31 Jul 2025 15:42

Instrument :

MSVOA_W

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 365723

Ion Ratio Lower Upper

114 100

63 21.3 0.0 44.2

88 17.2 0.0 35.6

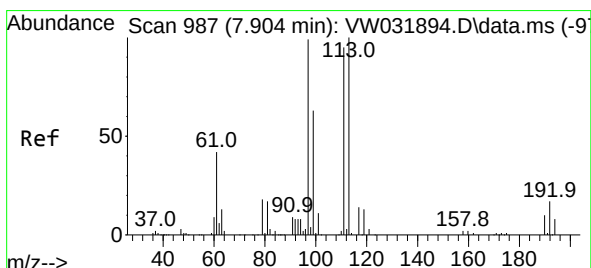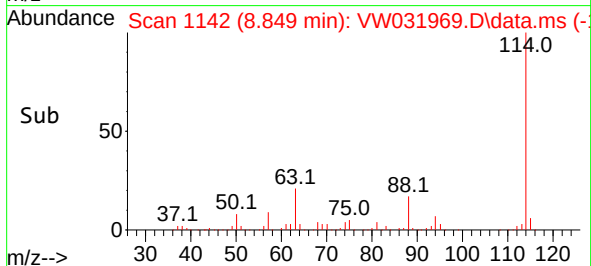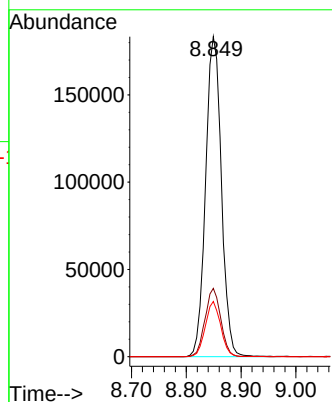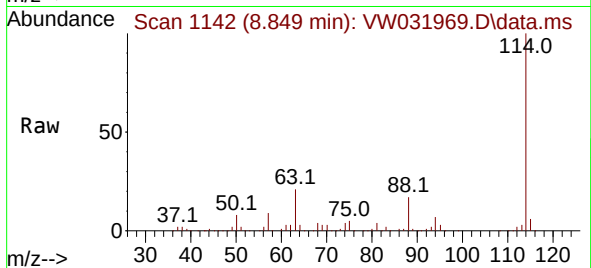

#35

Dibromofluoromethane

Concen: 49.478 ug/l

RT: 7.898 min Scan# 986

Delta R.T. -0.006 min

Lab File: VW031969.D

Acq: 31 Jul 2025 15:42




Tgt Ion:113 Resp: 122959


Ion Ratio Lower Upper

113 100

111 101.5 79.9 119.9

192 15.1 12.6 19.0


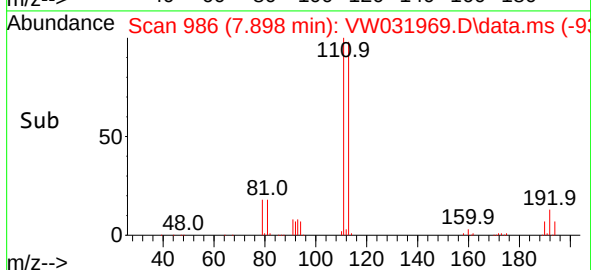
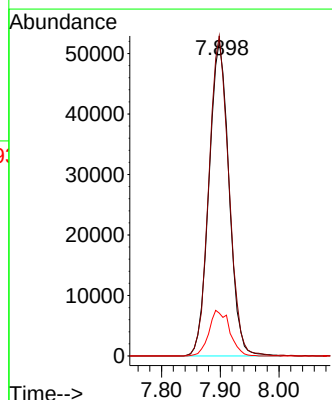
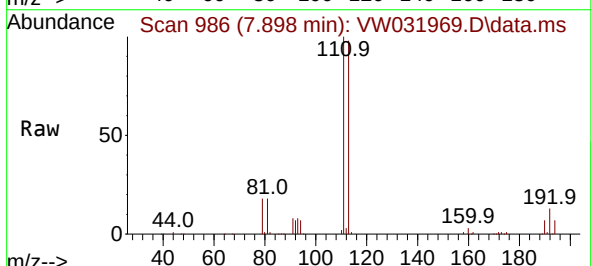


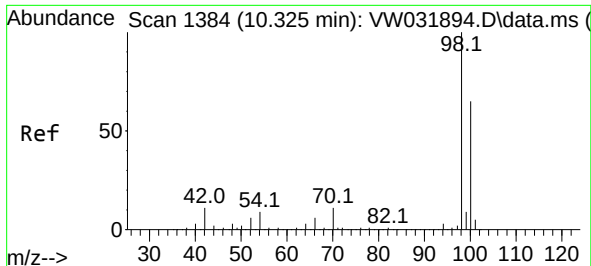

#50
Toluene-d8
Concen: 45.809 ug/l
RT: 10.325 min Scan# 1
Delta R.T. 0.000 min
Lab File: VW031969.D
Acq: 31 Jul 2025 15:42




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 430853
Ion Ratio Lower Upper
98 100
100 67.5 51.7 77.5

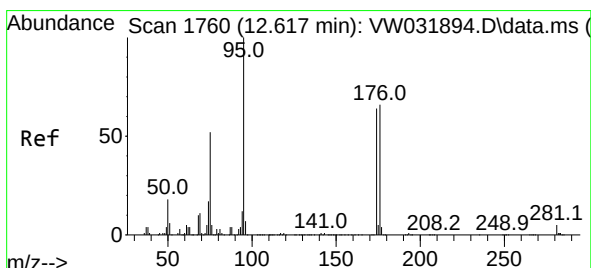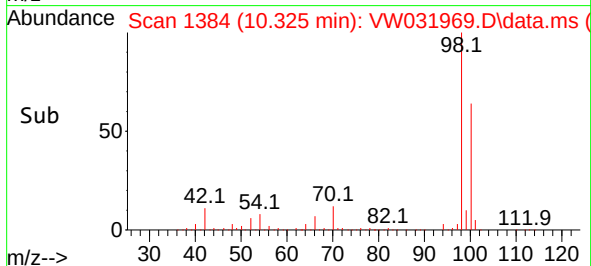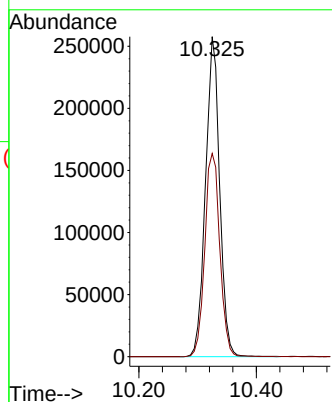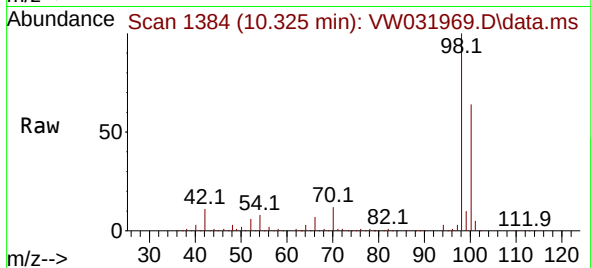

#62
4-Bromofluorobenzene
Concen: 40.359 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.000 min
Lab File: VW031969.D
Acq: 31 Jul 2025 15:42

Tgt Ion: 95 Resp: 145758
Ion Ratio Lower Upper
95 100
174 68.2 0.0 129.8
176 64.1 0.0 130.4


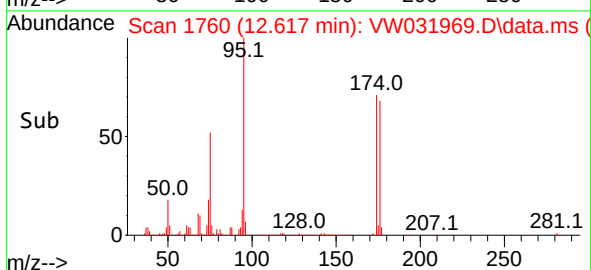
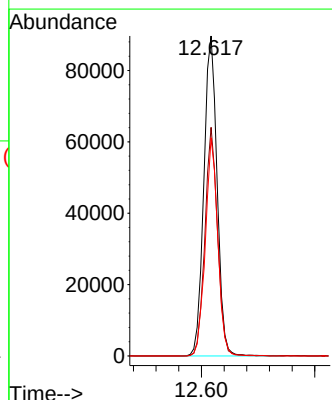
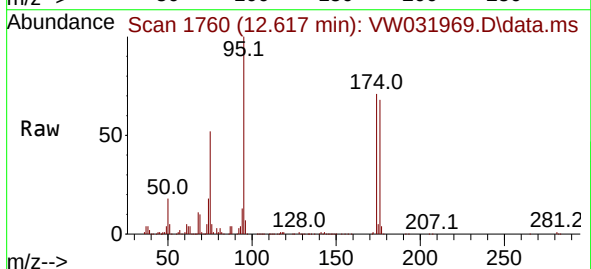


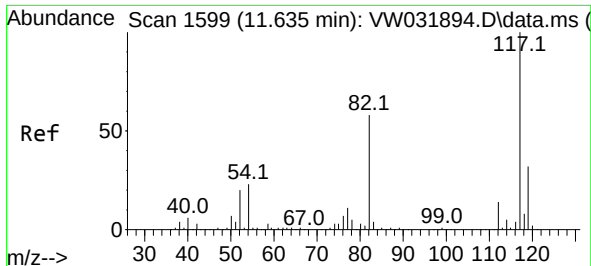

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.629 min Scan# 11
Delta R.T. -0.006 min
Lab File: VW031969.D
Acq: 31 Jul 2025 15:42

Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 345087
Ion Ratio Lower Upper
117 100
82 55.2 46.5 69.7
119 30.0 25.8 38.6

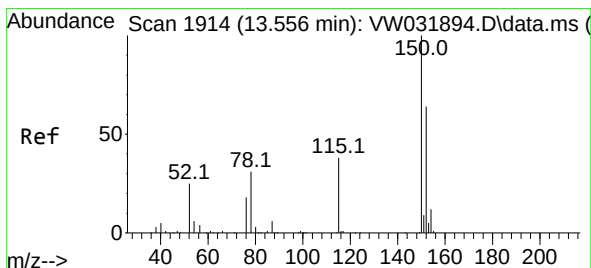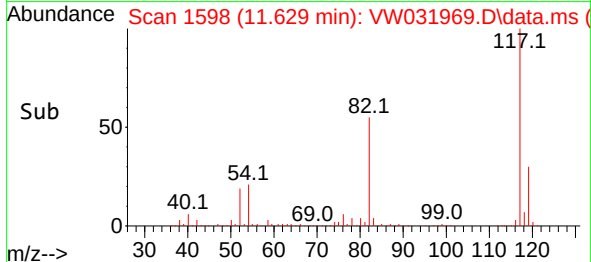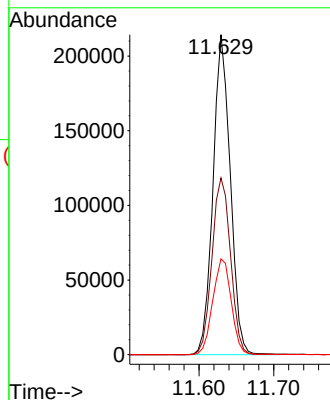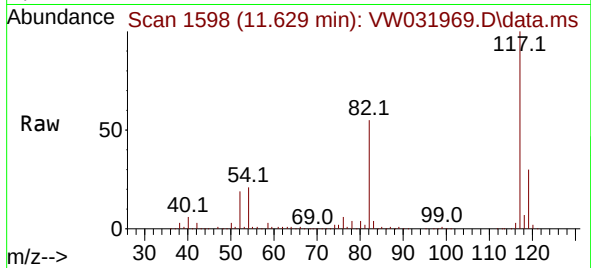

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. 0.000 min
Lab File: VW031969.D
Acq: 31 Jul 2025 15:42

Tgt Ion:152 Resp: 158467
Ion Ratio Lower Upper
152 100
115 68.1 33.4 100.1
150 158.9 0.0 352.2

