

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080218\
 Data File : VW004410.D
 Acq On : 02 Aug 2018 19:54
 Operator : SY/AP
 Sample : J4209-13
 Misc : 7.79G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC9

Quant Time: Aug 03 04:49:56 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 02 17:07:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	962574	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	927346	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	335162	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	346761	28.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.84%
7) Chloroethane-d5	2.89	69	278222	27.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.48%
10) 1,1-Dichloroethene-d2	4.01	63	475385	19.55	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.20%
20) 2-Butanone-d5	7.09	46	175772	33.30	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.60%
24) Chloroform-d	7.65	84	642402	24.65	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	8.43	65	64	0.00	ug/L	0.12
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.00%#
29) Benzene-d6	8.27	84	1248553	25.31	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.24%
33) 1,2-Dichloropropane-d6	9.28	67	415672	25.78	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.12%
37) Toluene-d8	10.33	98	1051637	24.18	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.72%
38) trans-1,3-Dichloropropene-	10.59	79	151405	22.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.36%
39) 2-Hexanone-d5	10.93	63	135229	34.45	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.90%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	364901	20.87	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.48%
61) 1,2-Dichlorobenzene-d4	13.86	152	335564	26.66	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.64%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.57	75	41343	3.240 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW080218\
Data File : VW004410.D
Acq On : 02 Aug 2018 19:54
Operator : SY/AP
Sample : J4209-13
Misc : 7.79G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC9

Quant Time: Aug 03 04:49:56 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 02 17:07:44 2018
Response via : Initial Calibration

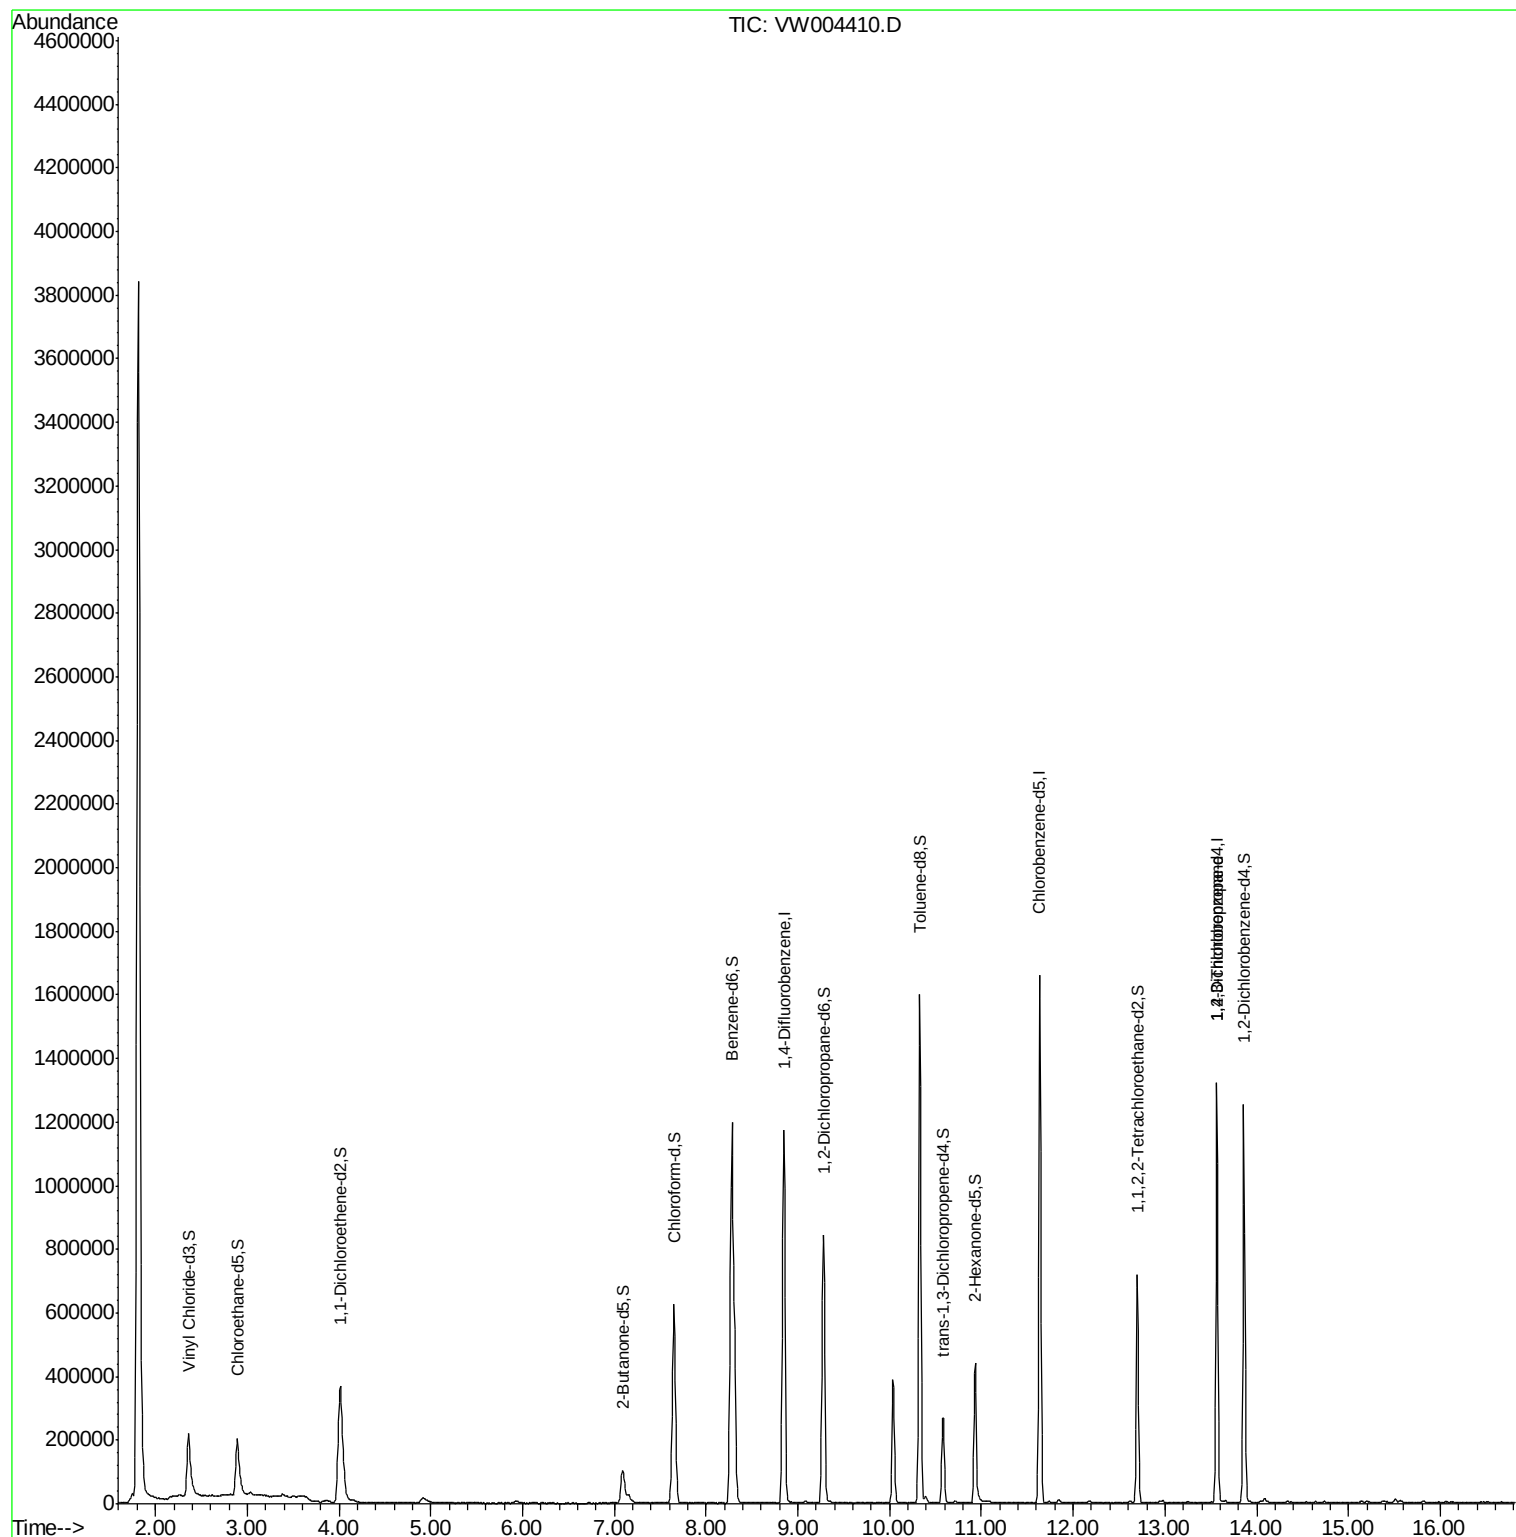

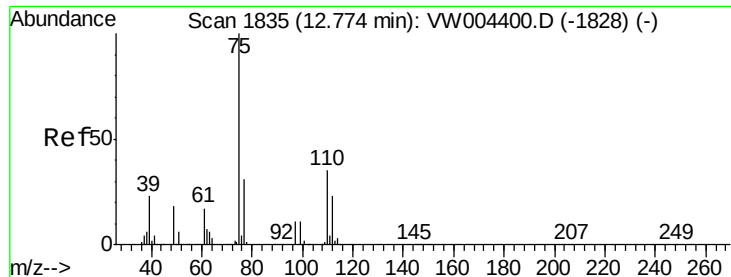

#59

1,2,3-Trichloropropane

Concen: 3.240 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW004410.D

Acq: 02 Aug 2018 19:54

Instrument :

MSVOA_W

ClientSampleId :

C0AC9

Tot Ion: 75 Resp: 41343

Ion Ratio Lower Upper

75 100

77 37.0 25.3 37.9

