

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW080218\
 Data File : VW004437.D
 Acq On : 03 Aug 2018 09:43
 Operator : SY/AP
 Sample : VW0802SBL03
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK95

Quant Time: Aug 04 01:27:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 04 01:26:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	1033582	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1061886	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	475136	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	252707	19.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.64%
7) Chloroethane-d5	2.89	69	208170	19.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.00%
10) 1,1-Dichloroethene-d2	4.01	63	370920	14.21	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.84%
20) 2-Butanone-d5	7.09	46	193817	34.19	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.38%
24) Chloroform-d	7.65	84	547608	19.57	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.28%
26) 1,2-Dichloroethane-d4	8.42	65	203	0.01	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.04%#
29) Benzene-d6	8.28	84	1035788	18.34	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.36%
33) 1,2-Dichloropropane-d6	9.28	67	342439	18.55	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.20%
37) Toluene-d8	10.33	98	894865	17.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.88%
38) trans-1,3-Dichloropropene-	10.58	79	131412	17.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.24%
39) 2-Hexanone-d5	10.93	63	140449	31.25	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.50%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	346487	17.31	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	69.24%
61) 1,2-Dichlorobenzene-d4	13.86	152	362163	20.29	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.16%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	13.57	75	59382	4.064	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW080218\
Data File : VW004437.D
Acq On : 03 Aug 2018 09:43
Operator : SY/AP
Sample : VW0802SBL03
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK95

Quant Time: Aug 04 01:27:02 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 04 01:26:48 2018
Response via : Initial Calibration

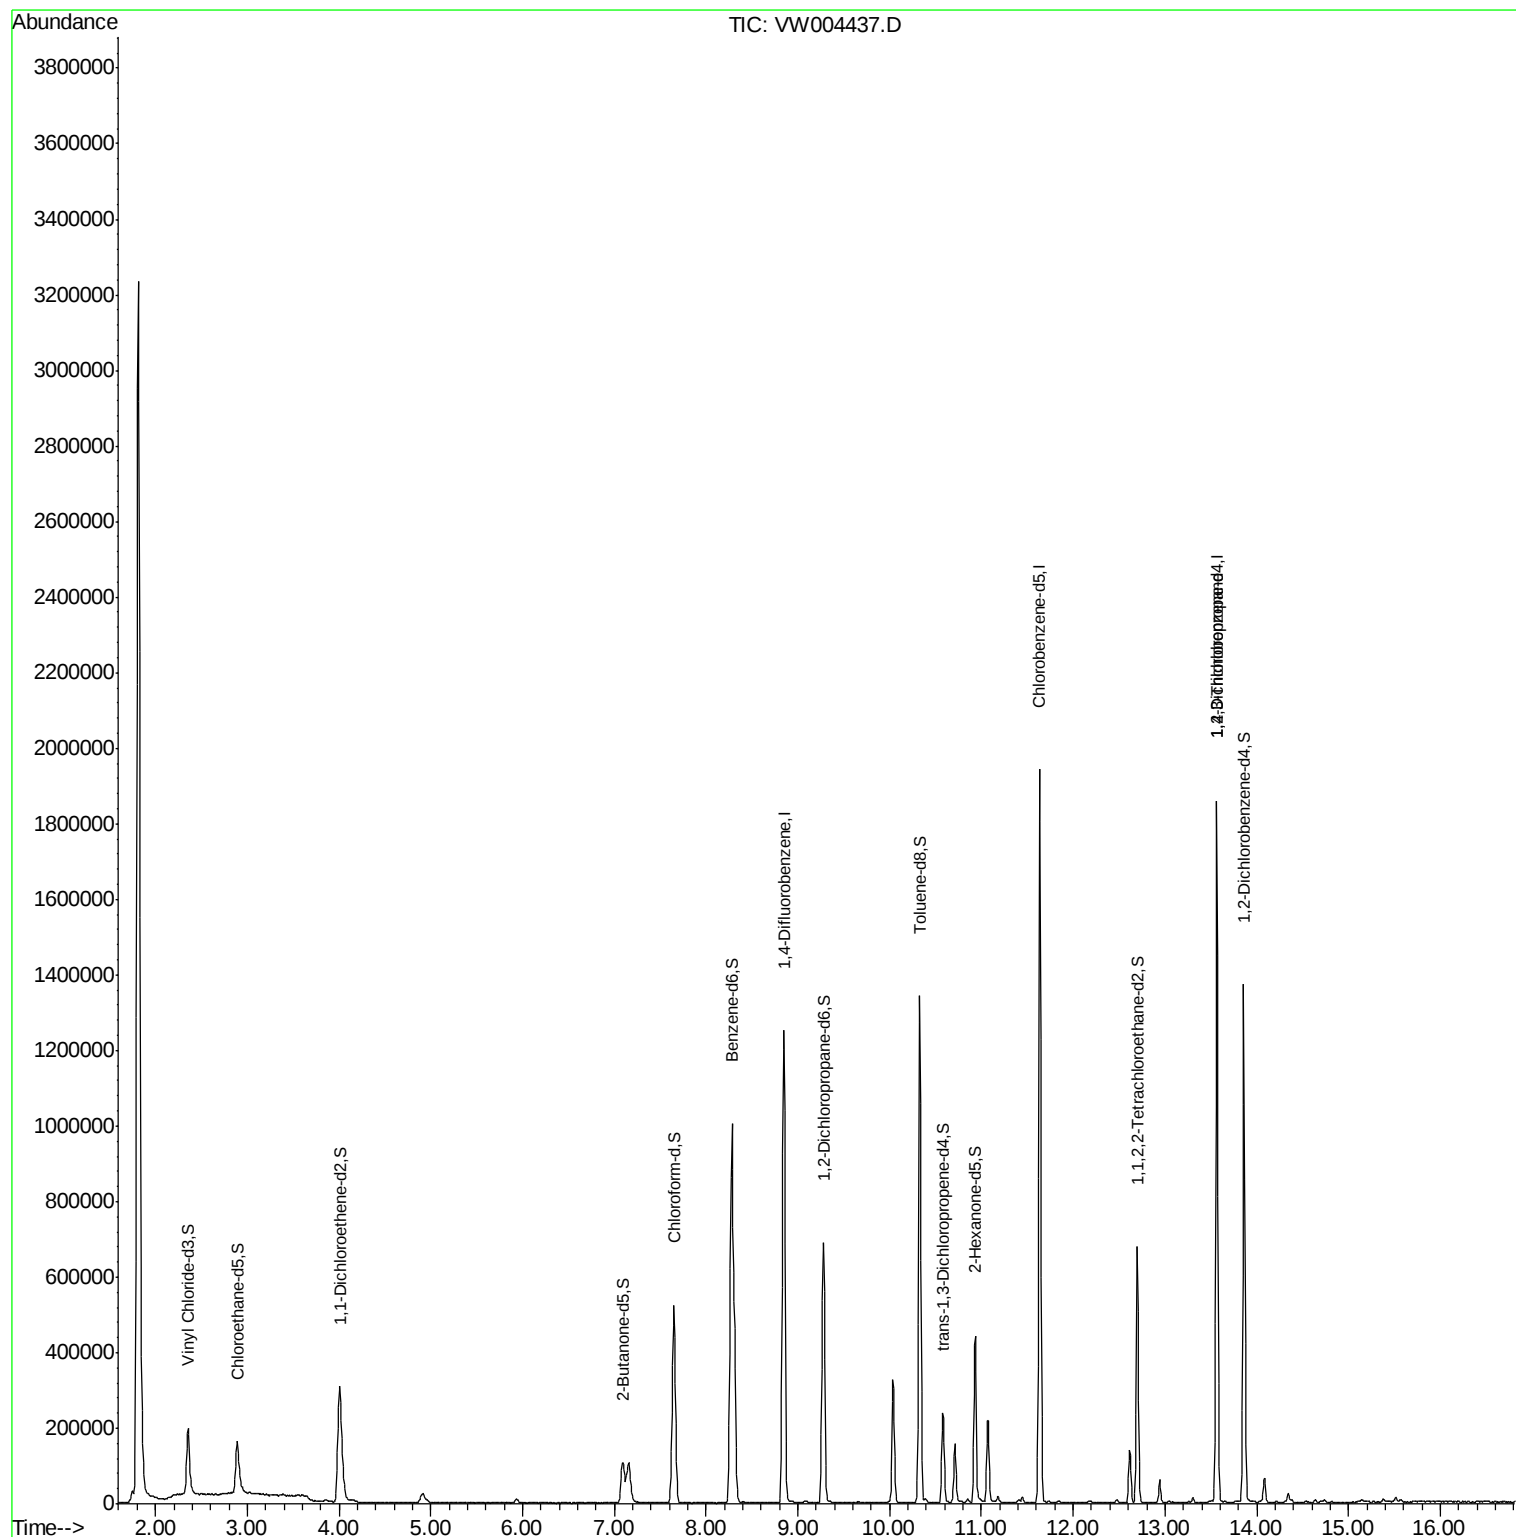

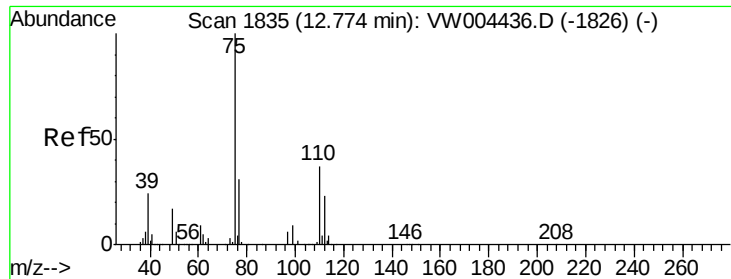

#59

1,2,3-Trichloropropane

Concen: 4.064 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW004437.D

Acq: 03 Aug 2018 09:43

Instrument :

MSVOA_W

ClientSampleId :

VBLK95

Tgt Ion: 75 Resp: 59382

Ion Ratio Lower Upper

75 100

77 36.6 25.3 37.9

