

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW080218\
 Data File : VW004473.D
 Acq On : 04 Aug 2018 02:41
 Operator : SY/AP
 Sample : J4209-17
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Quant Time: Aug 04 04:08:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 04 02:26:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	790838	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	798618	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	336607	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	211494	21.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.00%
7) Chloroethane-d5	2.89	69	175969	21.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.04%
10) 1,1-Dichloroethene-d2	4.01	63	316121	15.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.32%
20) 2-Butanone-d5	7.09	46	227771	52.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.04%
24) Chloroform-d	7.65	84	465951	21.76	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.04%
26) 1,2-Dichloroethane-d4	8.31	65	269121	22.55	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.20%
29) Benzene-d6	8.27	84	872374	20.53	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.12%
33) 1,2-Dichloropropane-d6	9.28	67	294722	21.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.92%
37) Toluene-d8	10.33	98	719743	19.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.88%
38) trans-1,3-Dichloropropene-	10.58	79	103287	18.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.36%
39) 2-Hexanone-d5	10.93	63	152901	45.23	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.46%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	323521	21.49	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.96%
61) 1,2-Dichlorobenzene-d4	13.86	152	296983	23.49	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.96%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Methylene chloride	4.91	84	35284	2.246	ug/L	88
59) 1,2,3-Trichloropropane	13.57	75	42615	3.878	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW080218\
Data File : VW004473.D
Acq On : 04 Aug 2018 02:41
Operator : SY/AP
Sample : J4209-17
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Aug 04 04:08:15 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 04 02:26:08 2018
Response via : Initial Calibration




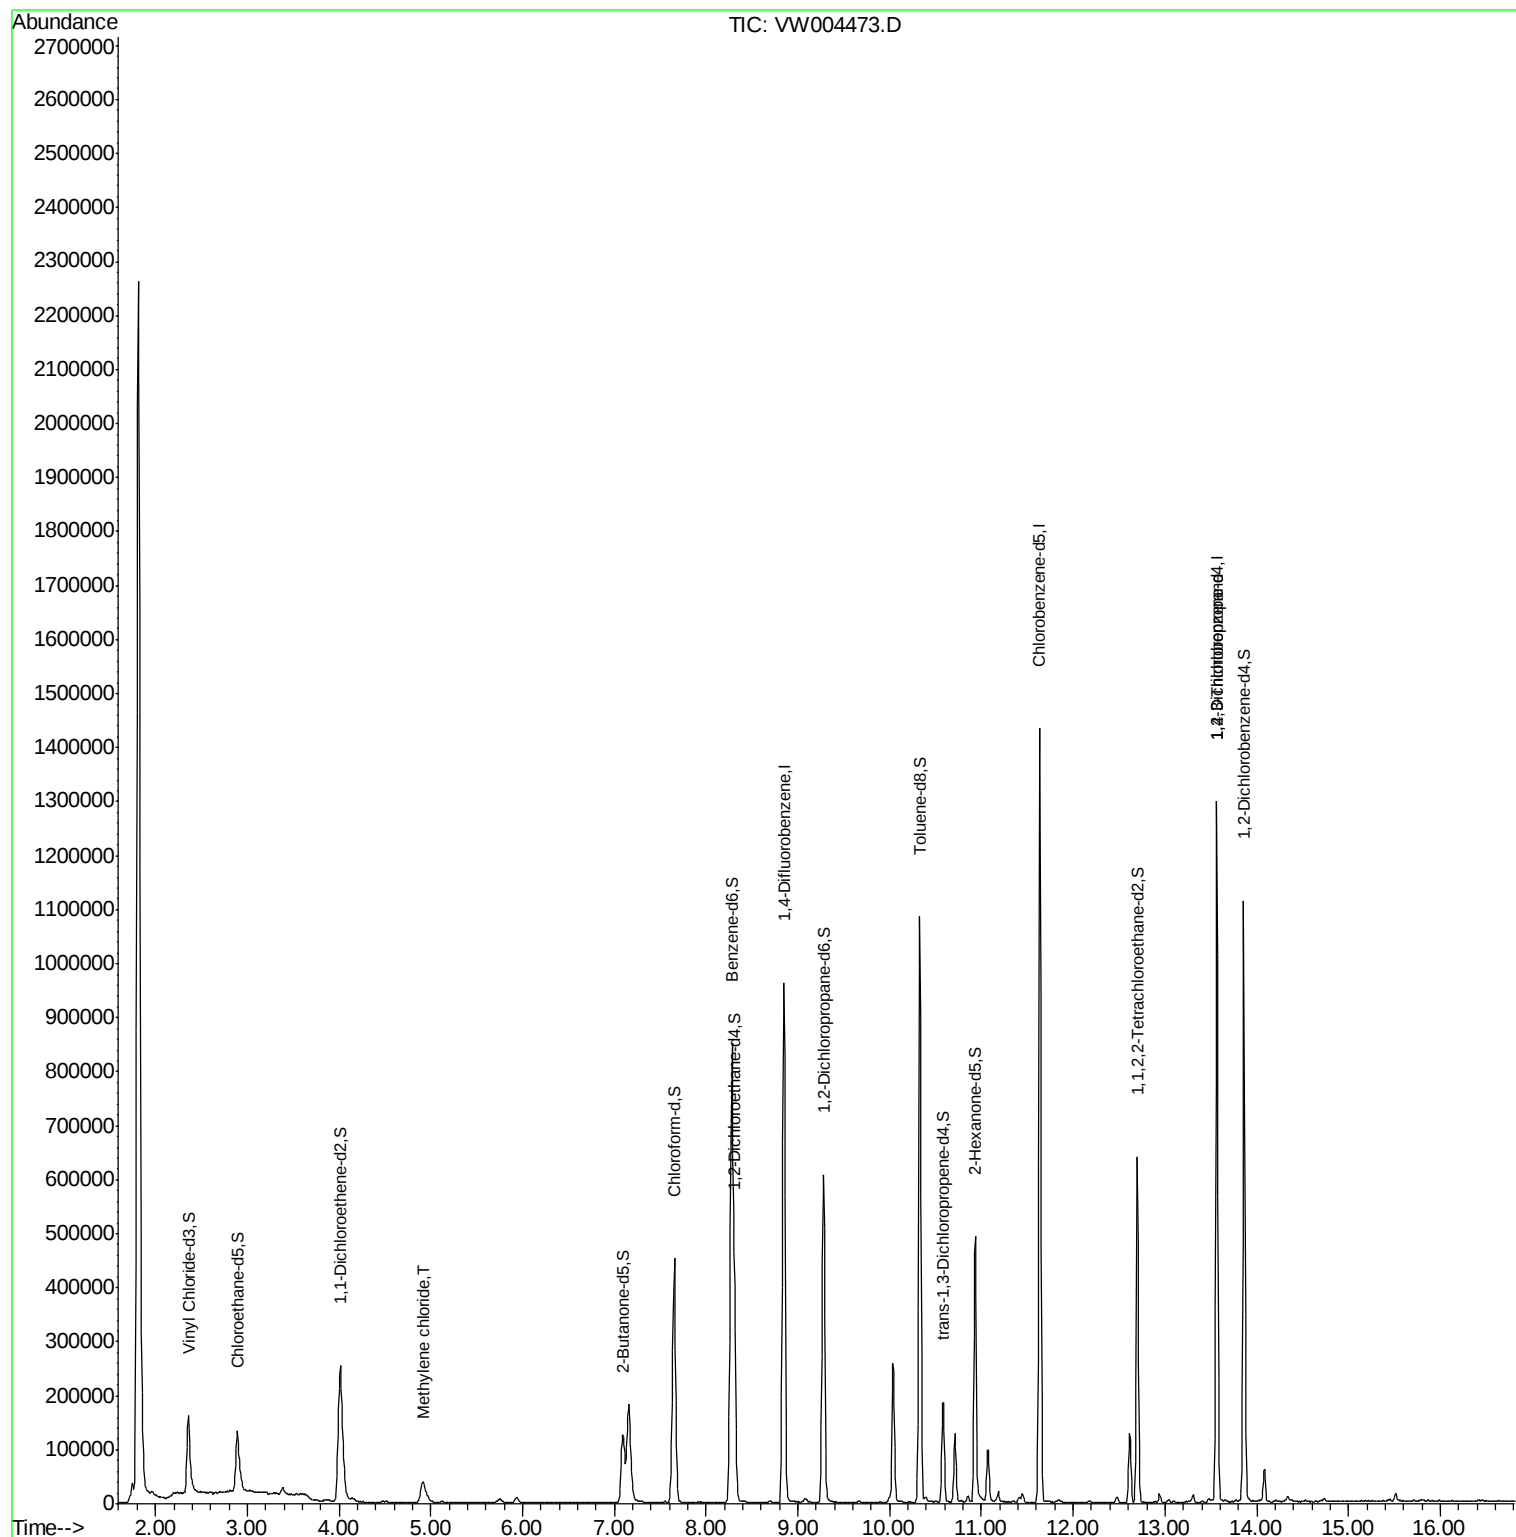


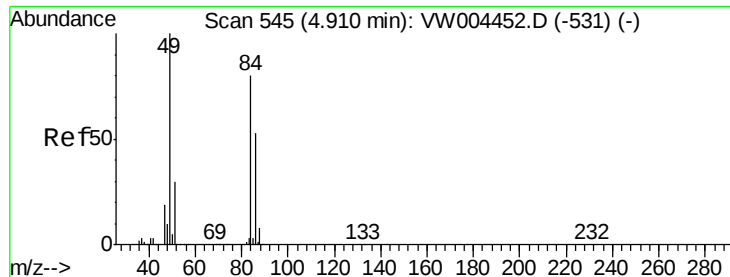

#16
Methylene chloride
Concen: 2.246 ug/L
RT: 4.91 min Scan# 545
Delta R.T. -0.00 min
Lab File: VW004473.D
Acq: 04 Aug 2018 02:41

Instrument :
MSVOA_W
ClientSampled :
VHBLK01

Tgt Ion: 84 Resp: 35284
Ion Ratio Lower Upper
84 100
49 106.8 86.0 159.6
86 57.3 43.5 80.9

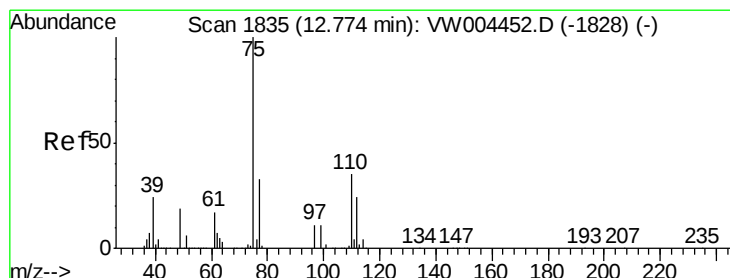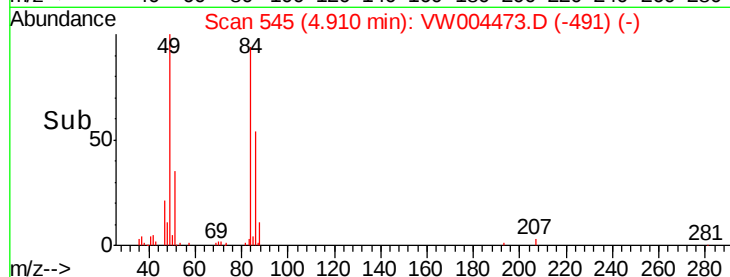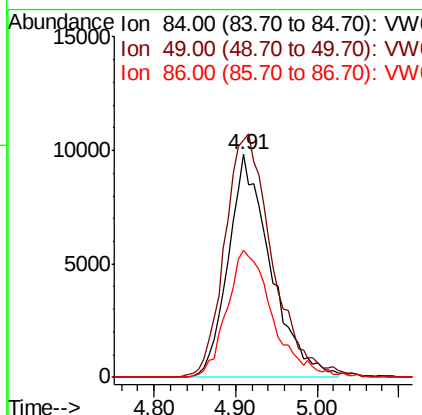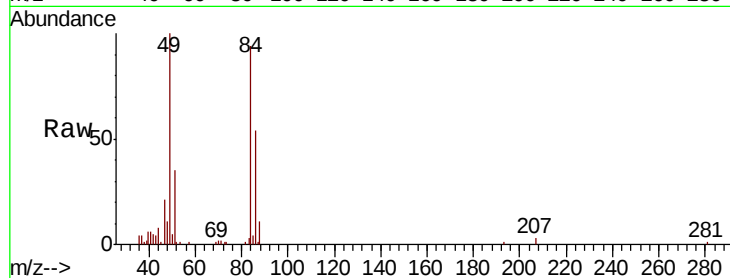

#59
1,2,3-Trichloropropane
Concen: 3.878 ug/L
RT: 13.57 min Scan# 1965
Delta R.T. 0.79 min
Lab File: VW004473.D
Acq: 04 Aug 2018 02:41

Tgt Ion: 75 Resp: 42615
Ion Ratio Lower Upper
75 100
77 37.0 25.3 37.9

