

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080218\
Data File : VW004434.D
Acq On : 03 Aug 2018 07:57
Operator : SY/AP
Sample : J4299-01
Misc : 6.53G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AD8

Quant Time: Aug 03 08:40:28 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 03 08:39:00 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDa000a
8/6/2018 5:19:00 PM

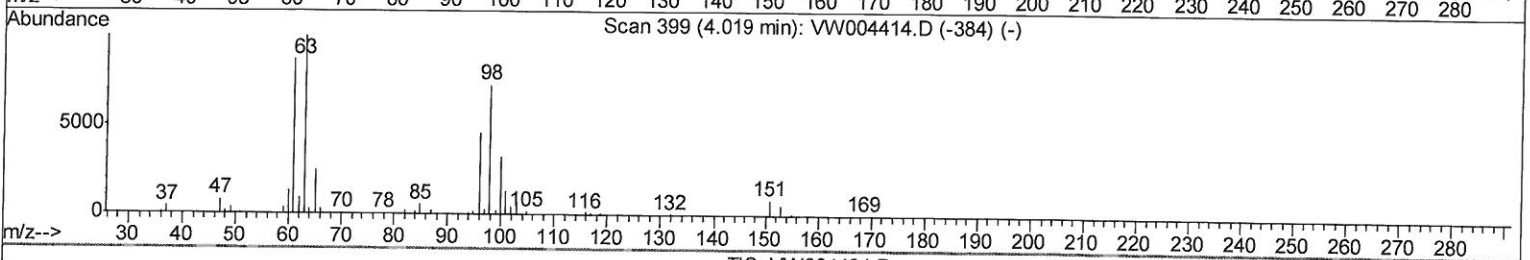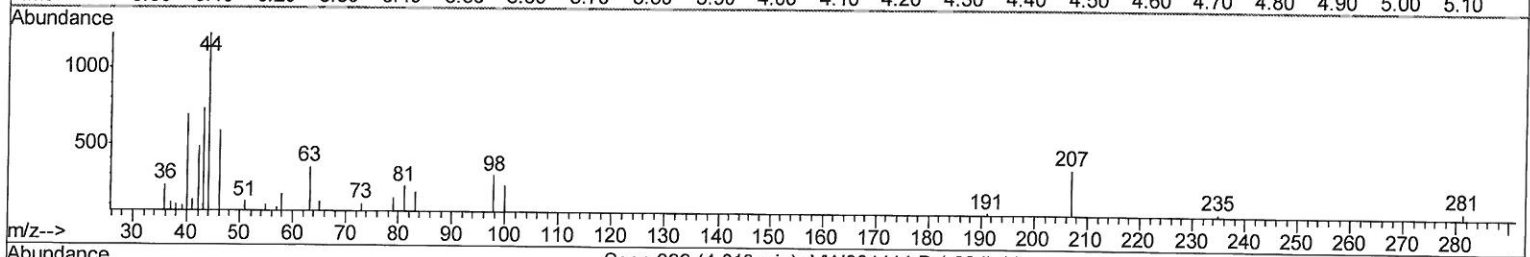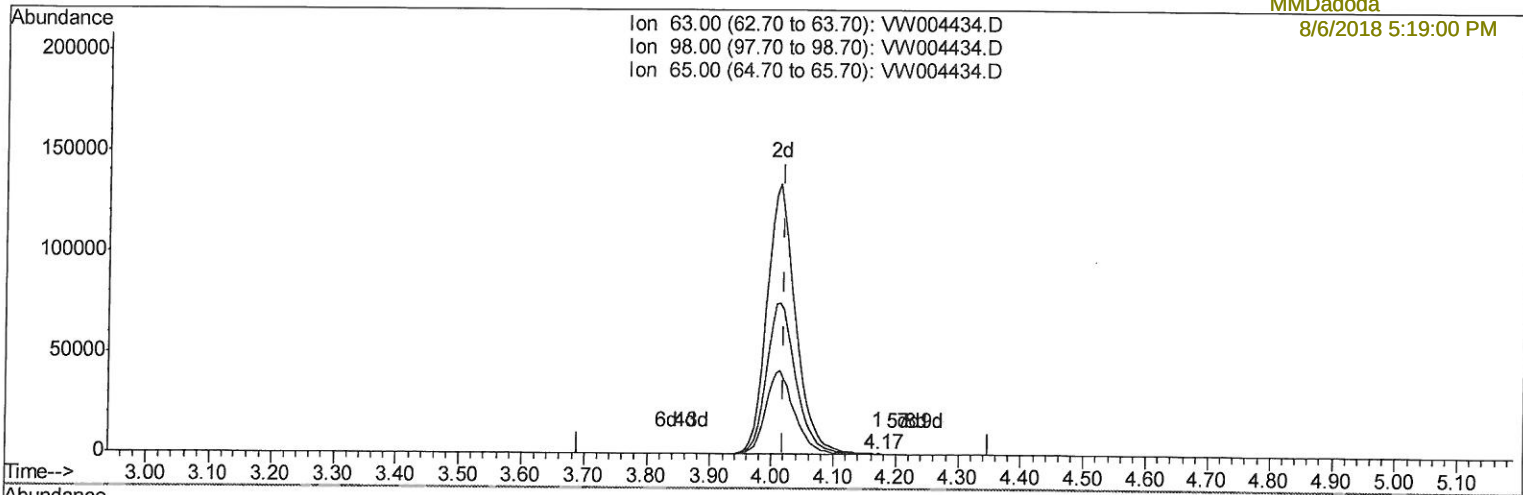

TIC: VW004434.D

(10) 1,1-Dichloroethene-d2 (S)

4.172min (+0.153) 0.02ug/L

response 340

Ion	Exp%	Act%
63.00	100	100
98.00	76.60	57.35
65.00	22.30	22.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080218\
 Data File : VW004434.D
 Acq On : 03 Aug 2018 07:57
 Operator : SY/AP
 Sample : J4299-01
 Misc : 6.53G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AD8

Quant Time: Aug 03 08:40:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 03 08:39:00 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/6/2018 5:19:00 PM

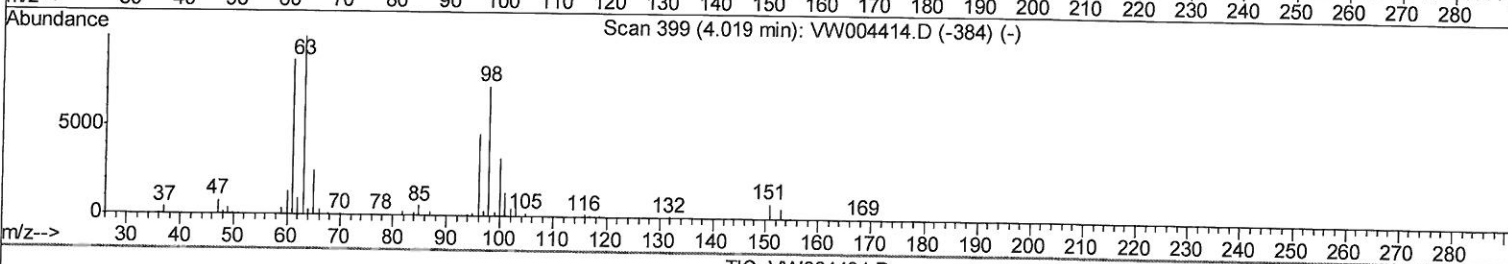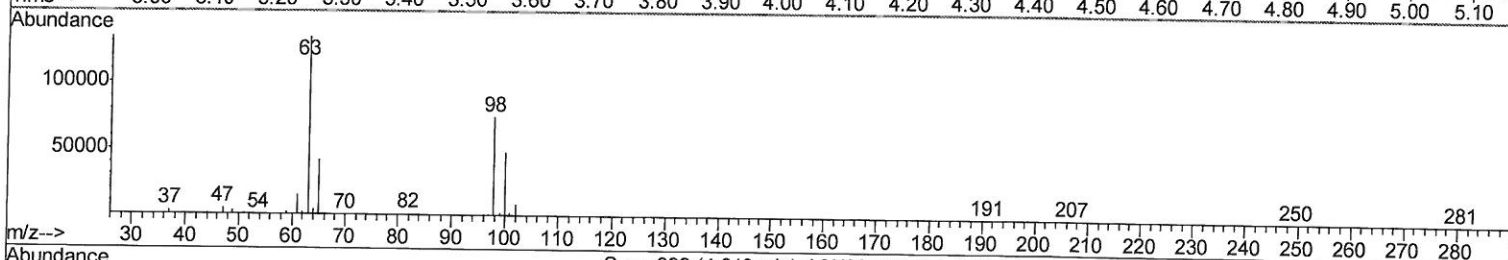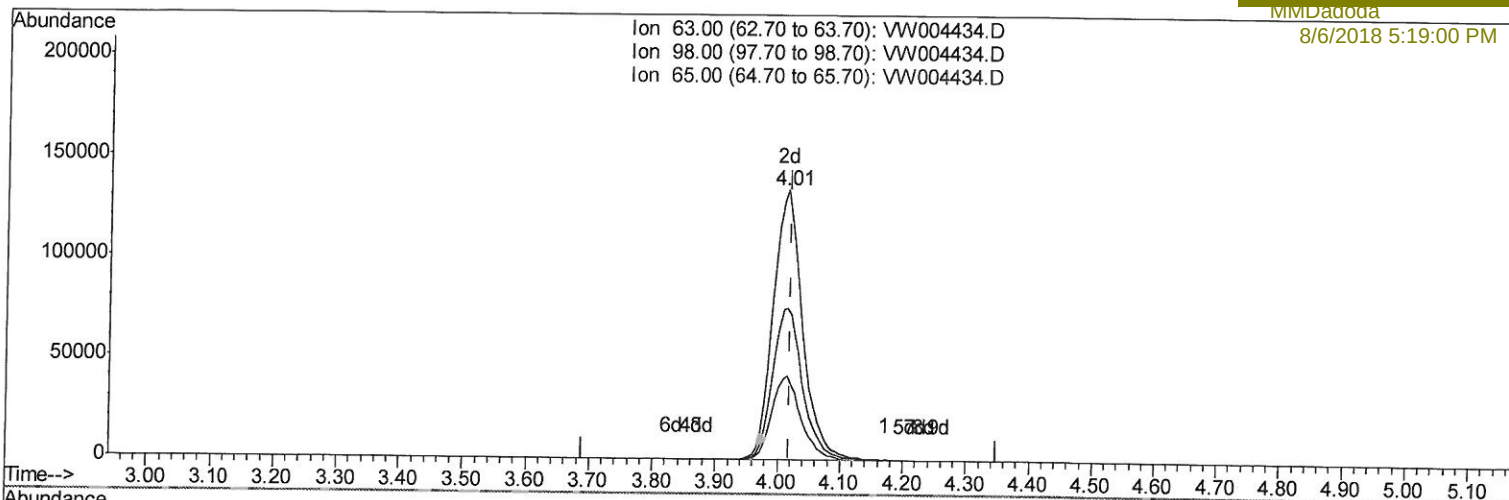

(10) 1,1-Dichloroethene-d2 (S)

4.014min (-0.006) 21.25ug/L m

response 436015

Ion	Exp%	Act%
63.00	100	100
98.00	76.60	0.04#
65.00	22.30	0.02#
0.00	0.00	0.00

08/08/18 Sy

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080218\
 Data File : VW004434.D
 Acq On : 03 Aug 2018 07:57
 Operator : SY/AP
 Sample : J4299-01
 Misc : 6.53G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AD8

Quant Time: Aug 03 08:40:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 03 08:39:00 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

VW004434.D
 8/6/2018 5:19:00 PM

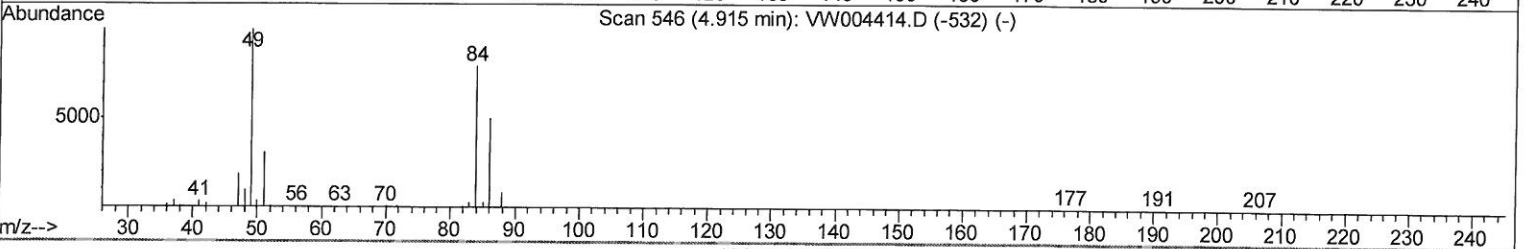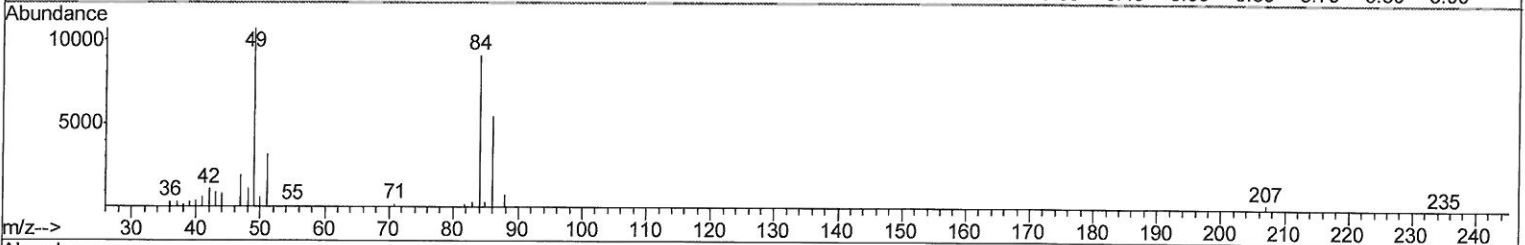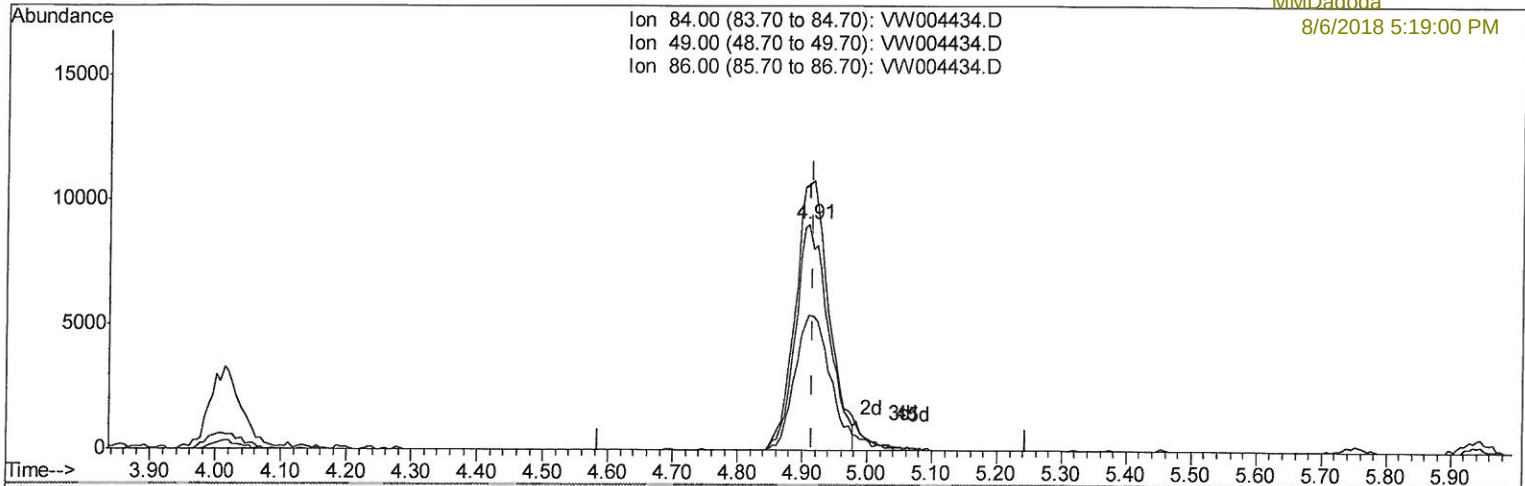

TIC: VW004434.D

(16) Methylene chloride (T)

4.910min (-0.006) 1.99ug/L

response 32076

Ion	Exp%	Act%
84.00	100	100
49.00	122.80	117.43
86.00	62.20	59.66
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080218\
Data File : VW004434.D
Acq On : 03 Aug 2018 07:57
Operator : SY/AP
Sample : J4299-01
Misc : 6.53G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AD8

Quant Time: Aug 03 08:40:28 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 03 08:39:00 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadada
8/6/2018 5:19:00 PM

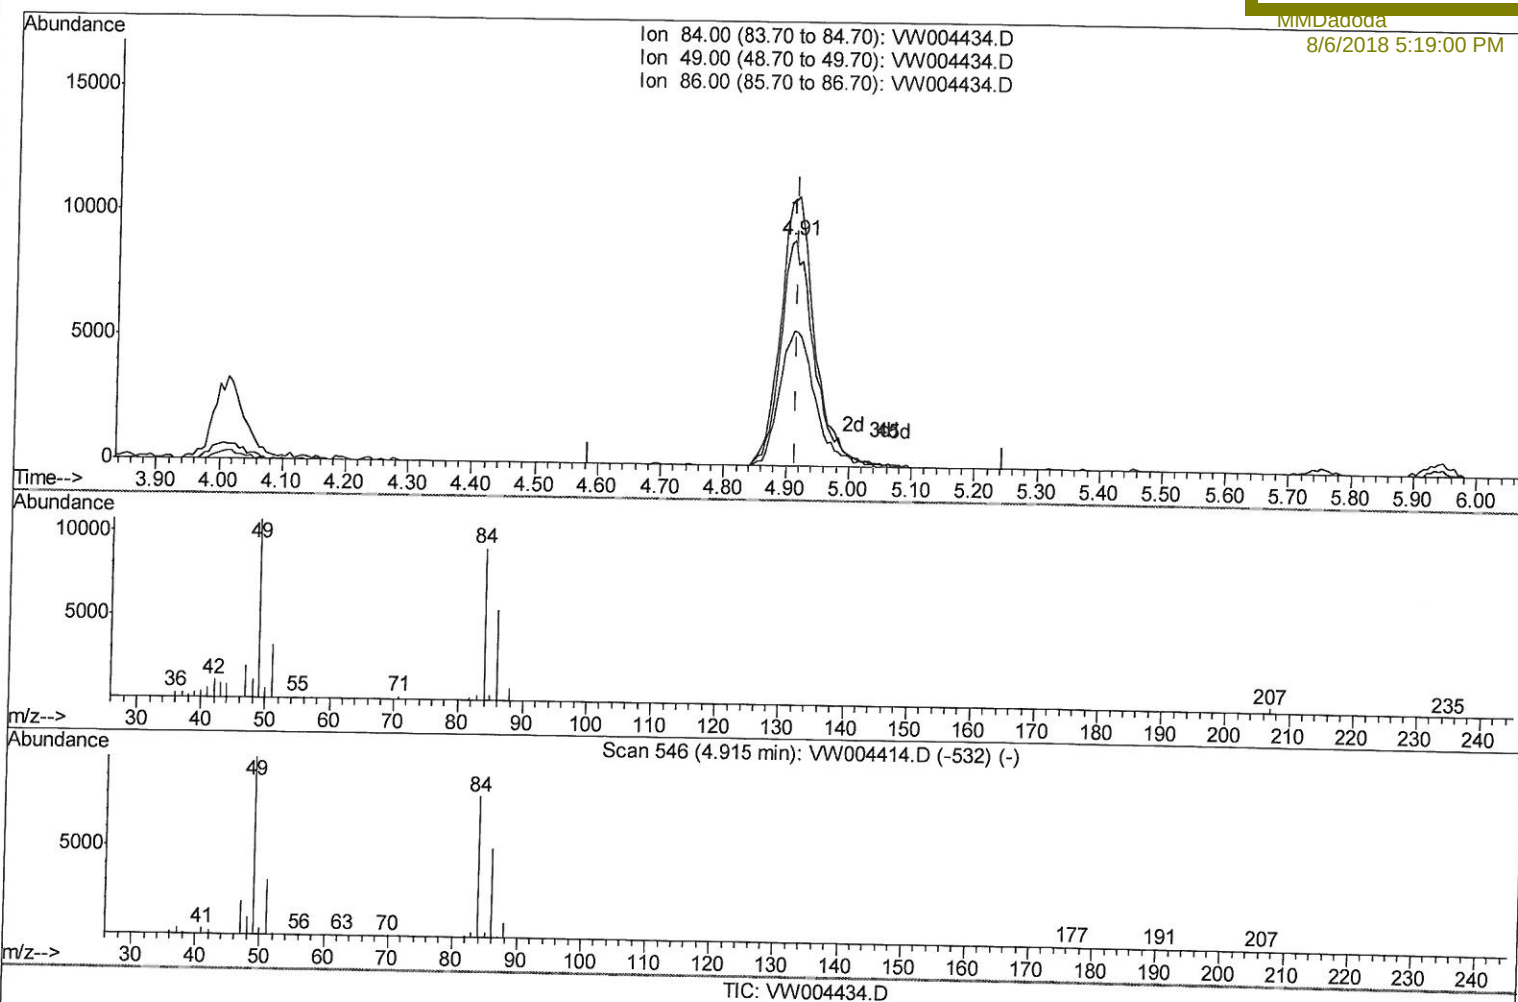

(16) Methylene chloride (T)

4.910min (-0.006) 2.09ug/L m

response 33781

Ion	Exp%	Act%
84.00	100	100
49.00	122.80	117.43
86.00	62.20	59.66
0.00	0.00	0.00

08/08/18 Sy

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080218\
 Data File : VW004434.D
 Acq On : 03 Aug 2018 07:57
 Operator : SY/AP
 Sample : J4299-01
 Misc : 6.53G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 C0AD8

Quant Time: Aug 03 09:02:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 03 08:39:00 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadada
 8/6/2018 5:19:00 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	812505	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	813766	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	306281	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	321583	31.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	127.28%
7) Chloroethane-d5	2.89	69	258334	30.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	121.56%
10) 1,1-Dichloroethene-d2	4.01	63	436015m	21.25	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.00%
20) 2-Butanone-d5	7.10	46	105272	23.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	47.26%
24) Chloroform-d	7.65	84	587369	26.70	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	106.80%
26) 1,2-Dichloroethane-d4	8.31	65	326878	26.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.60%
29) Benzene-d6	8.28	84	1122970	25.94	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.76%
33) 1,2-Dichloropropane-d6	9.28	67	374561	26.47	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.88%
37) Toluene-d8	10.33	98	940808	24.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.60%
38) trans-1,3-Dichloropropene-	10.58	79	116537	20.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.12%
39) 2-Hexanone-d5	10.93	63	78101	22.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	45.36%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	300534	19.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	78.36%
61) 1,2-Dichlorobenzene-d4	13.86	152	312447	27.16	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.64%

Target Compounds

16) Methylene chloride	4.91	84	33781m)	2.093	ug/L	Ovalue
35) Trichloroethene	9.09	95	220136	17.443	ug/L	99
47) Tetrachloroethene	10.87	164	31781	3.183	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080218\
 Data File : VW004434.D
 Acq On : 03 Aug 2018 07:57
 Operator : SY/AP
 Sample : J4299-01
 Misc : 6.53G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 C0AD8

Quant Time: Aug 03 09:02:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 03 08:39:00 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

