

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024162.D
 Acq On : 04 Aug 2022 15:24
 Operator : SY/VA
 Sample : VW0804SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Quant Time: Aug 05 01:01:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.835	114	306221	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	298298	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	139829	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	156315	24.421	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.680%
7) Chloroethane-d5	2.873	69	93165	23.365	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.480%
11) 1,1-Dichloroethene-d2	4.001	63	121200	16.615	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.440%
21) 2-Butanone-d5	7.074	46	52199	43.834	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.660%
24) Chloroform-d	7.641	84	196380	21.195	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.760%
26) 1,2-Dichloroethane-d4	8.116	65	43	0.008	ug/L	-0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.268	84	384090	21.833	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.320%
36) 1,2-Dichloropropane-d6	9.268	67	113826	21.914	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.640%
41) Toluene-d8	10.323	98	353106	21.474	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.880%
43) trans-1,3-Dichloroprop...	10.573	79	46969	20.645	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.560%
47) 2-Hexanone-d5	10.920	63	40611	42.329	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.660%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103271	20.492	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	120389	23.528	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.120%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	2.001	85	3100	1.151	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
Data File : VW024162.D
Acq On : 04 Aug 2022 15:24
Operator : SY/VA
Sample : VW0804SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK569

Quant Time: Aug 05 01:01:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 01:00:42 2022
Response via : Initial Calibration

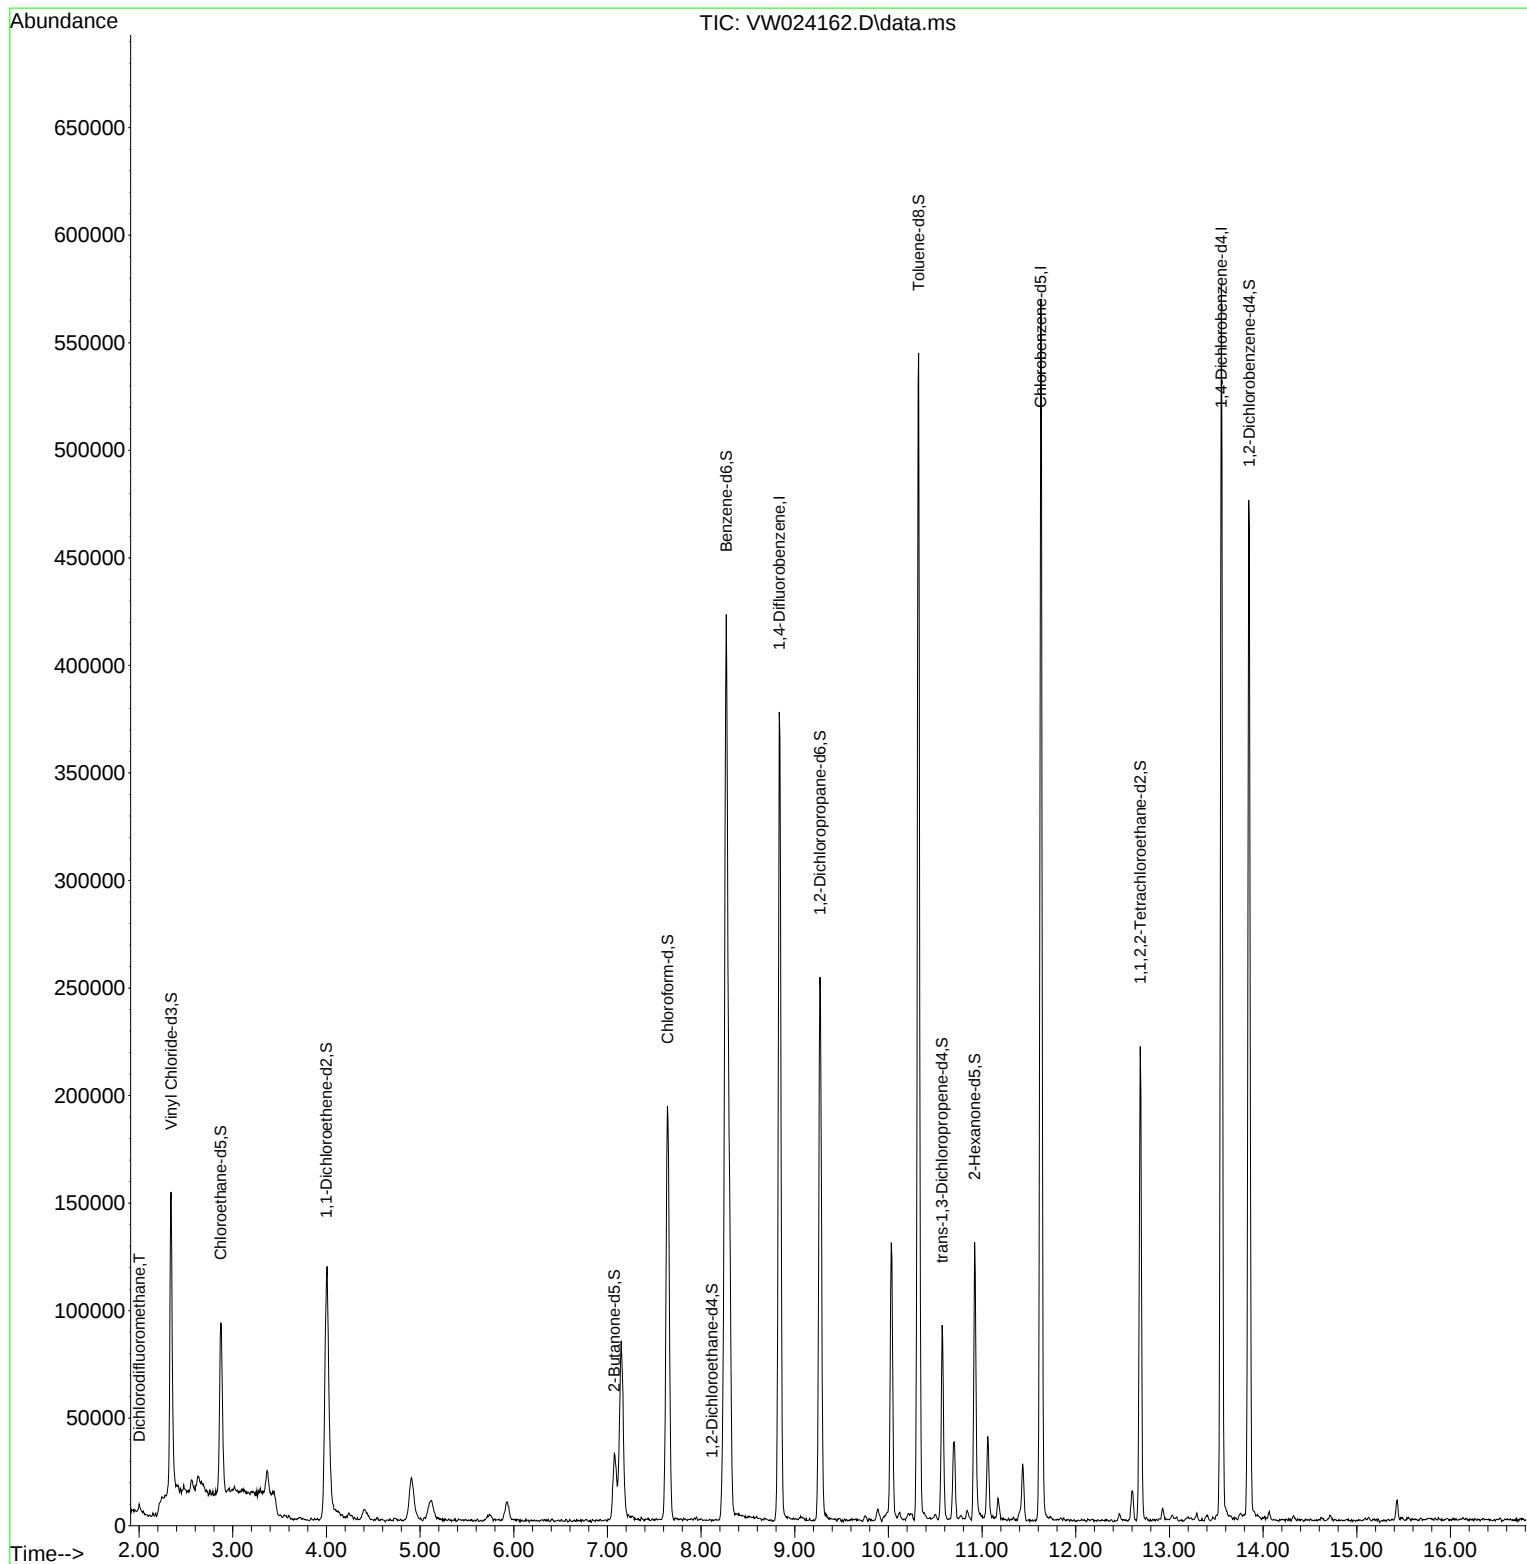

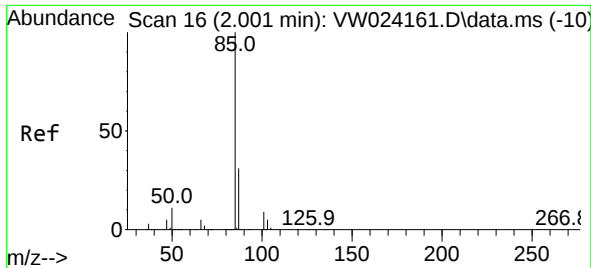

#2
 Dichlorodifluoromethane
 Concen: 1.151 ug/L
 RT: 2.001 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VW024162.D
 Acq: 04 Aug 2022 15:24

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Tgt Ion: 85 Resp: 3100
 Ion Ratio Lower Upper
 85 100
 87 29.4 24.5 36.7

