

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024177.D
 Acq On : 04 Aug 2022 21:59
 Operator : SY/VA
 Sample : N4004-10
 Misc : 5.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY138

Quant Time: Aug 05 01:05:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	399231	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	339404	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	138661	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	204841	24.547	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.200%
7) Chloroethane-d5	2.873	69	98091	18.869	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.480%
11) 1,1-Dichloroethene-d2	4.001	63	155595	16.361	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.440%
21) 2-Butanone-d5	7.080	46	73622	47.421	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.840%
24) Chloroform-d	7.647	84	265973	22.018	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.080%
26) 1,2-Dichloroethane-d4	8.305	65	149688	22.320	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.280%
32) Benzene-d6	8.268	84	527905	26.373	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.480%
36) 1,2-Dichloropropane-d6	9.268	67	155146	26.251	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.000%
41) Toluene-d8	10.323	98	457959	24.477	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.920%
43) trans-1,3-Dichloroprop...	10.579	79	55449	21.420	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.680%
47) 2-Hexanone-d5	10.920	63	56046	51.342	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.680%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	122496	21.363	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	119432	23.537	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.160%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	45885	6.518	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
Data File : VW024177.D
Acq On : 04 Aug 2022 21:59
Operator : SY/VA
Sample : N4004-10
Misc : 5.31g/10mL/MSVOA_W/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY138

Quant Time: Aug 05 01:05:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 01:00:42 2022
Response via : Initial Calibration

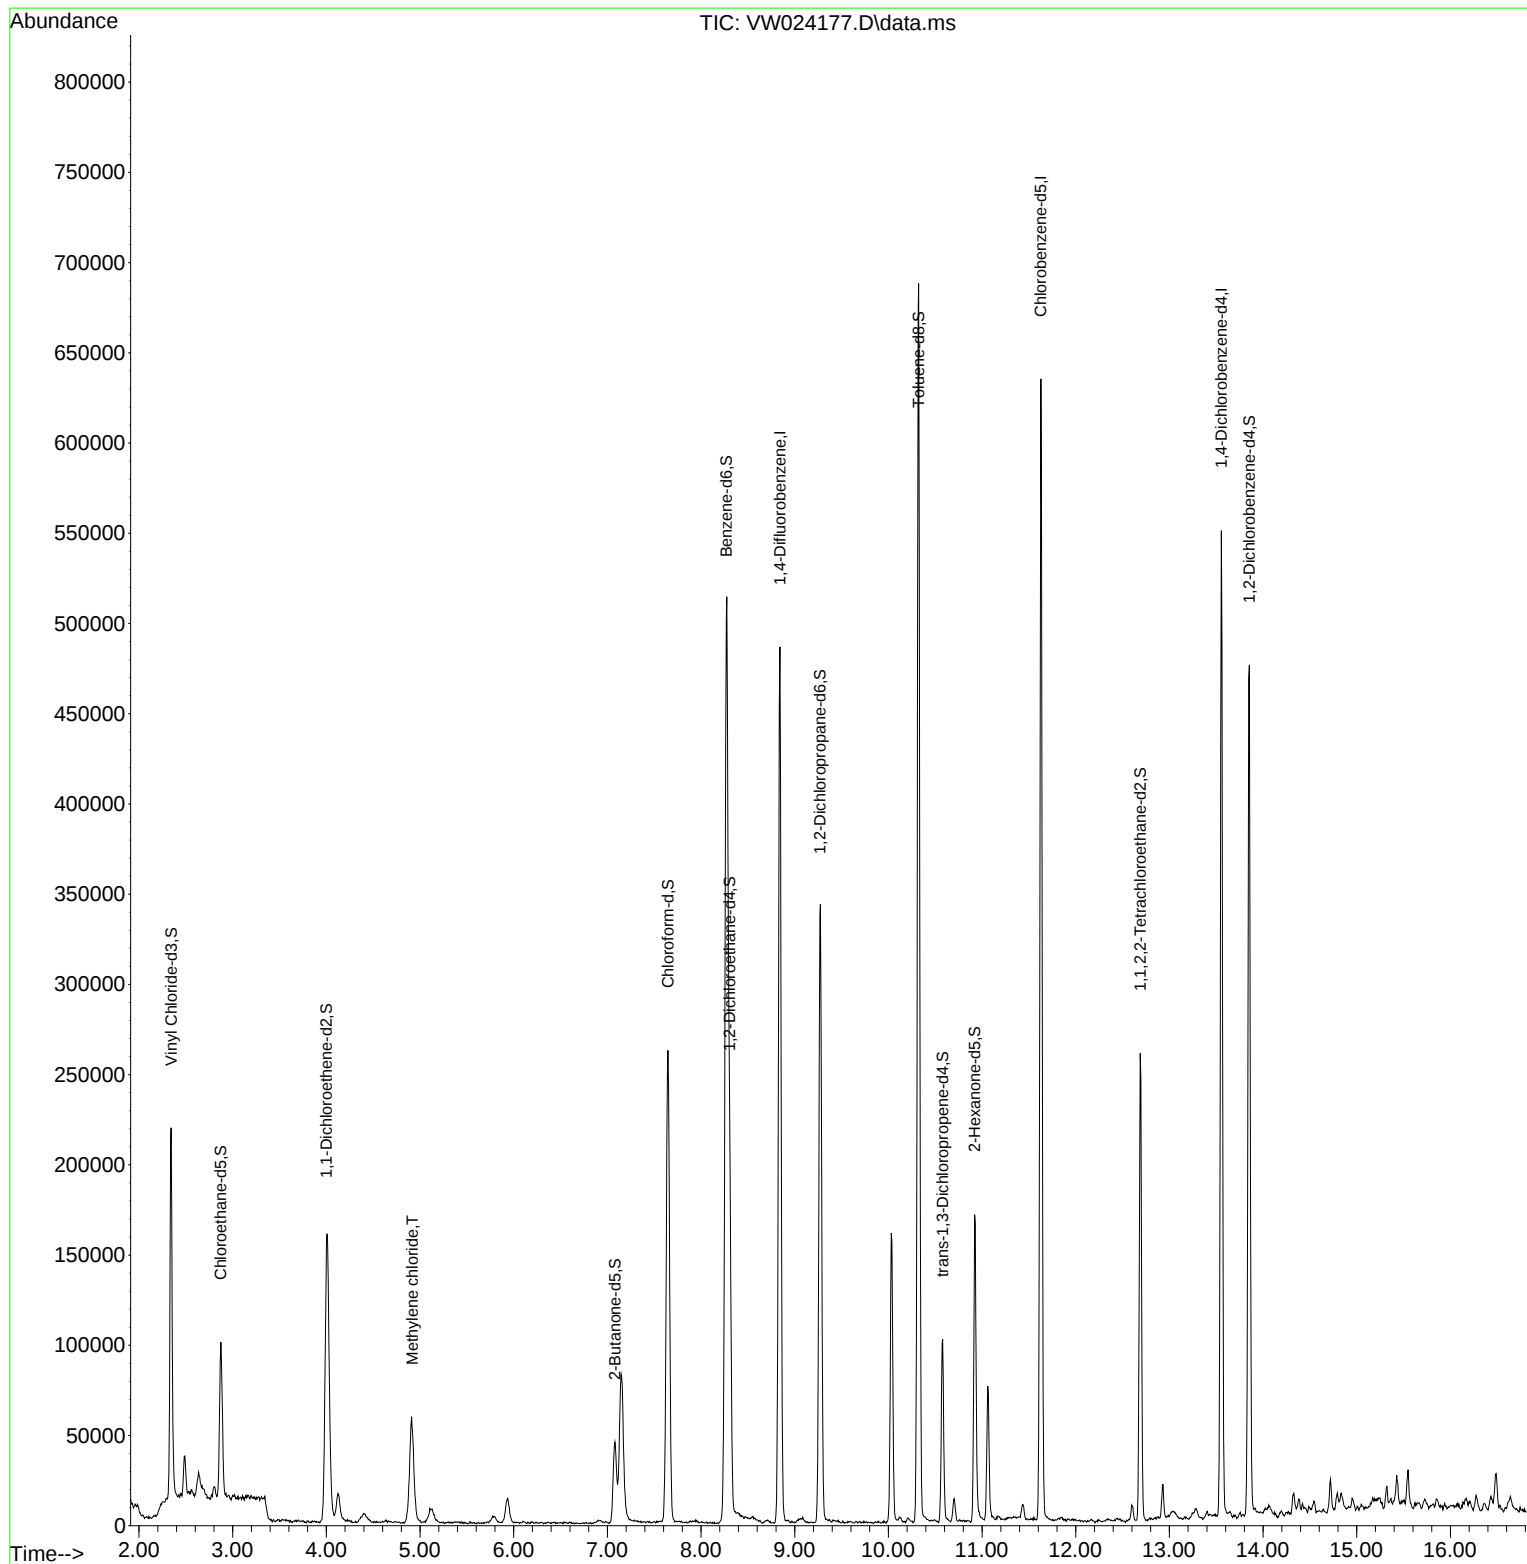

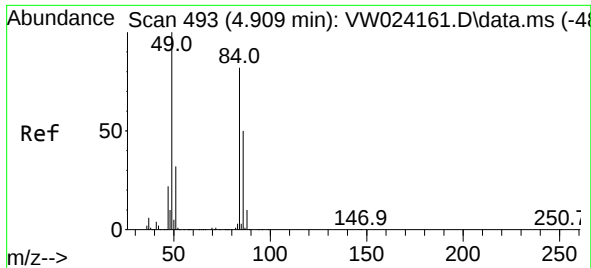

#16
Methylene chloride
Concen: 6.518 ug/L
RT: 4.915 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW024177.D
Acq: 04 Aug 2022 21:59

Instrument :
MSVOA_W
ClientSampleId :
EY138

Tgt Ion: 84 Resp: 45885
Ion Ratio Lower Upper
84 100
86 58.8 42.8 79.6
49 105.1 85.3 158.3

