




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024162.D
 Acq On : 04 Aug 2022 15:24
 Operator : SY/VA
 Sample : VW0804SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Manual IntegrationsAPPROVED

Quant Time: Aug 05 02:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

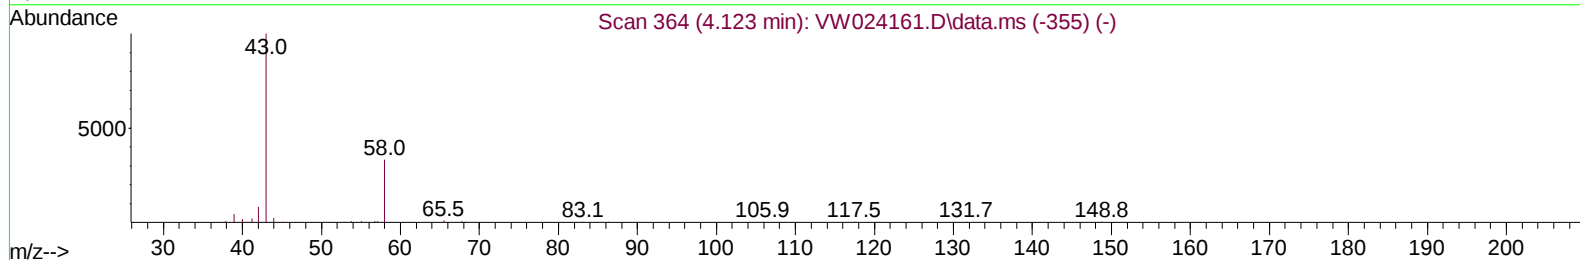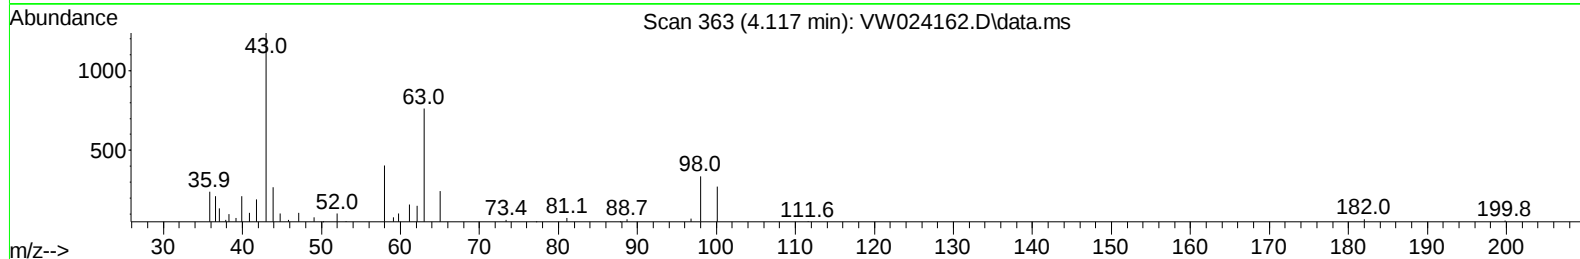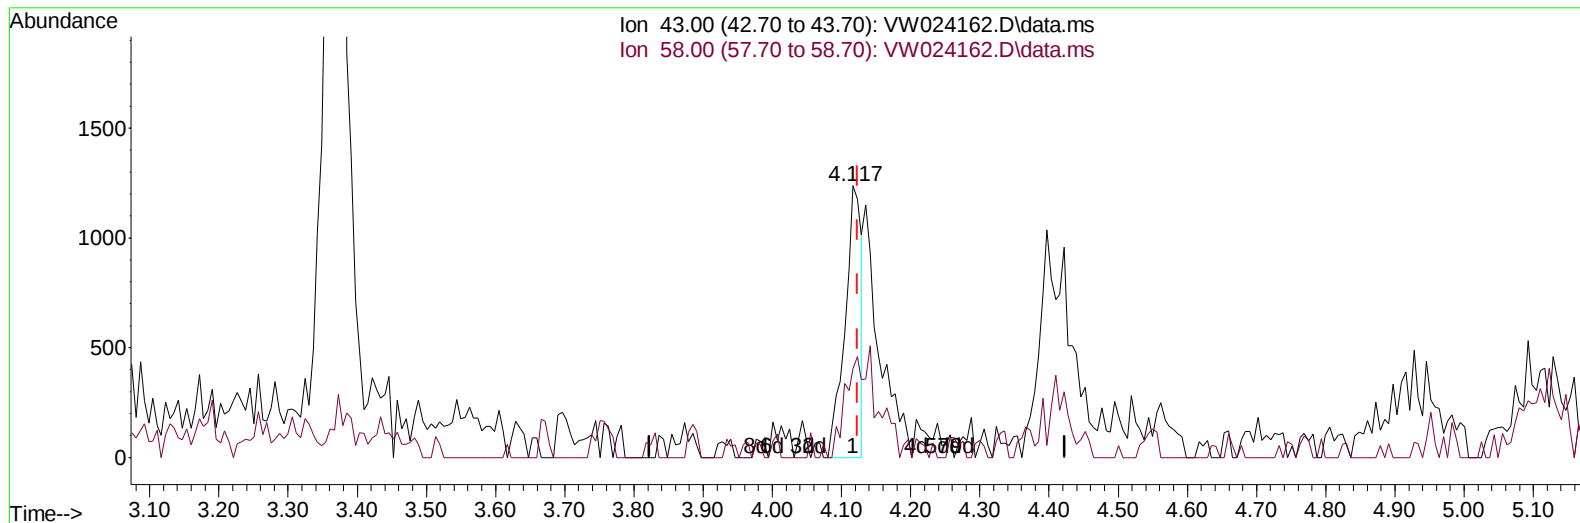

TIC: VW024162.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 2.34 ug/L

response 2052

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	37.23#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024162.D
 Acq On : 04 Aug 2022 15:24
 Operator : SY/VA
 Sample : VW0804SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Manual IntegrationsAPPROVED

Quant Time: Aug 05 02:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

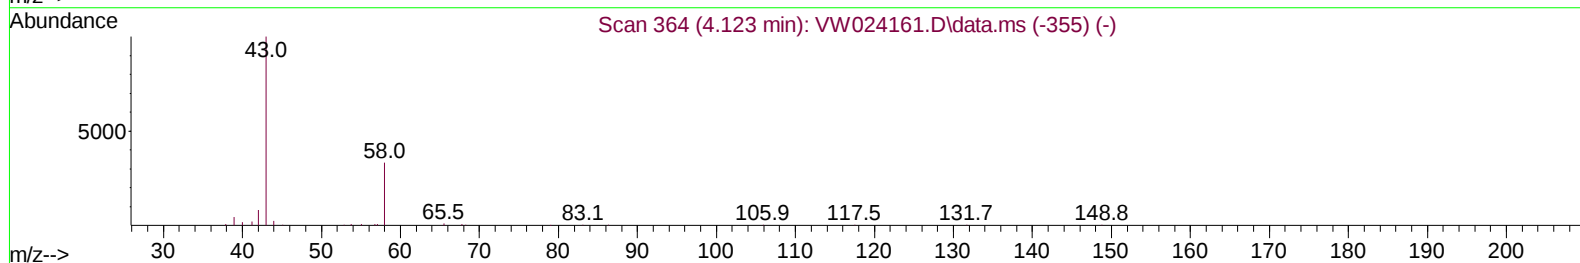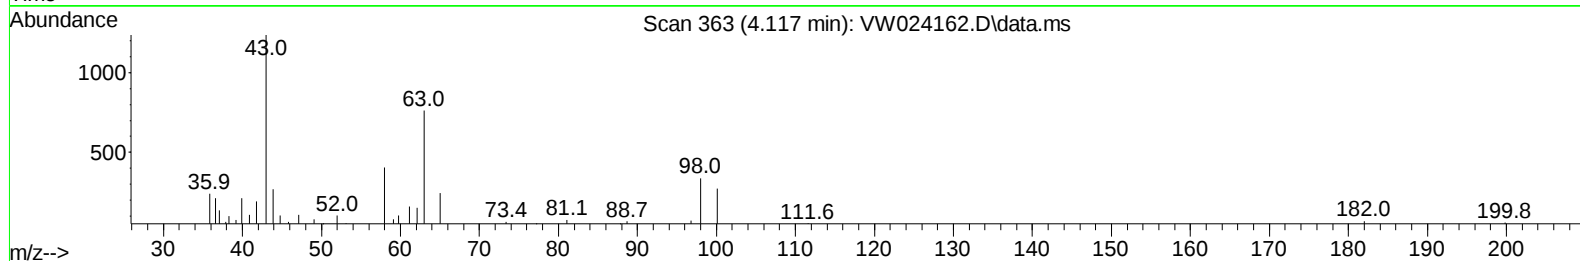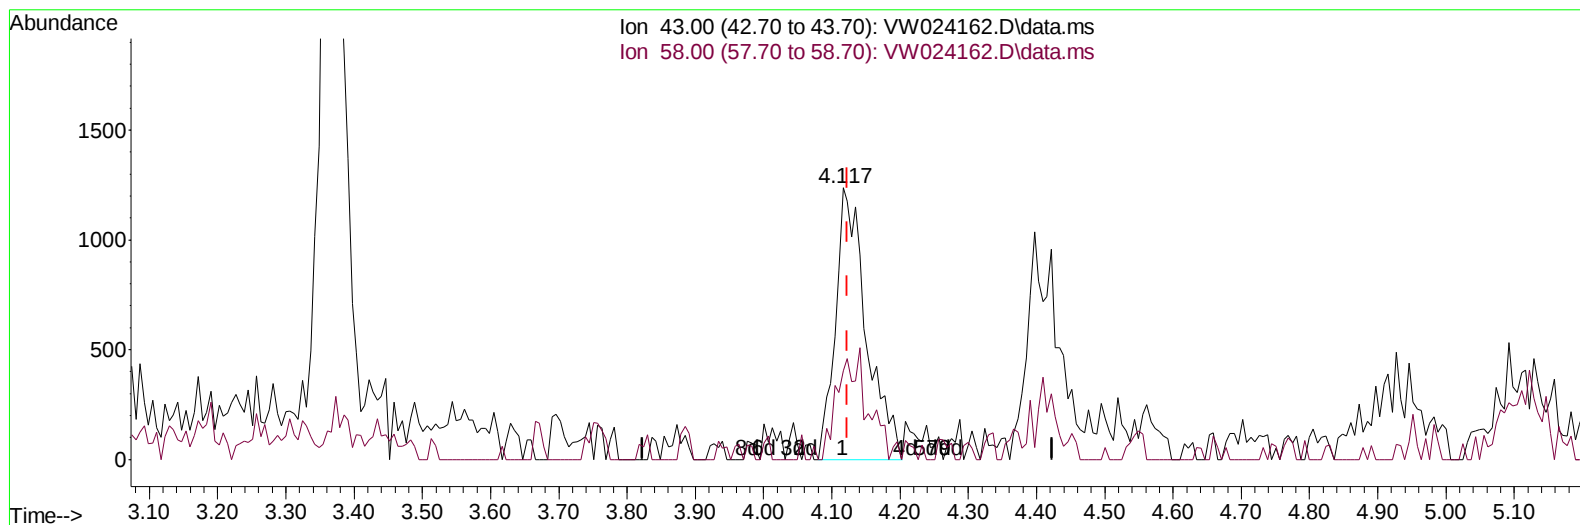

TIC: VW024162.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 4.40 ug/L m

response 3861

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	19.79
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024162.D
 Acq On : 04 Aug 2022 15:24
 Operator : SY/VA
 Sample : VW0804SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

Quant Time: Aug 05 02:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

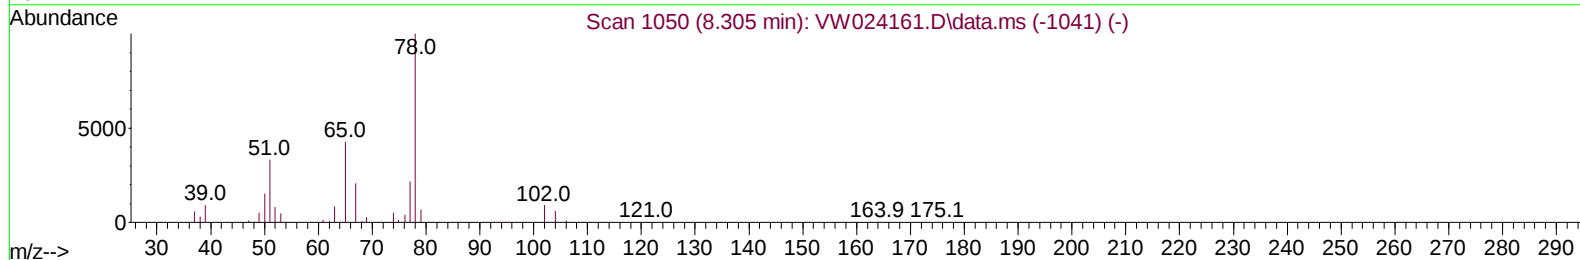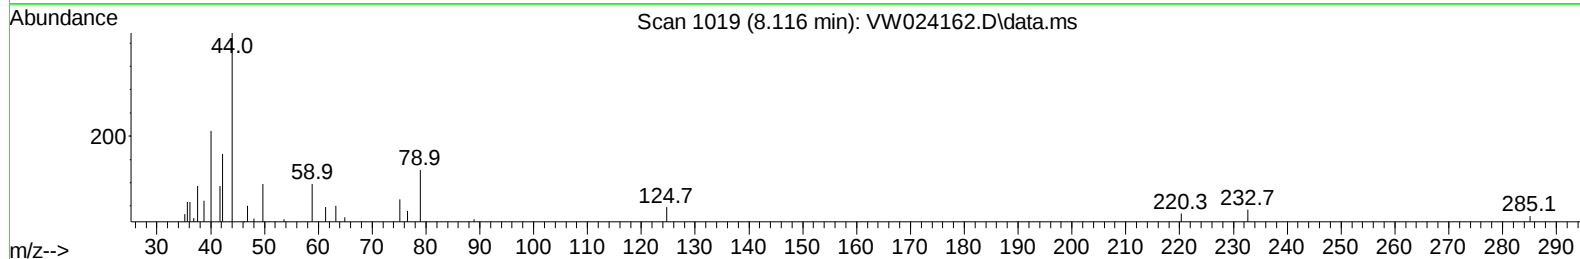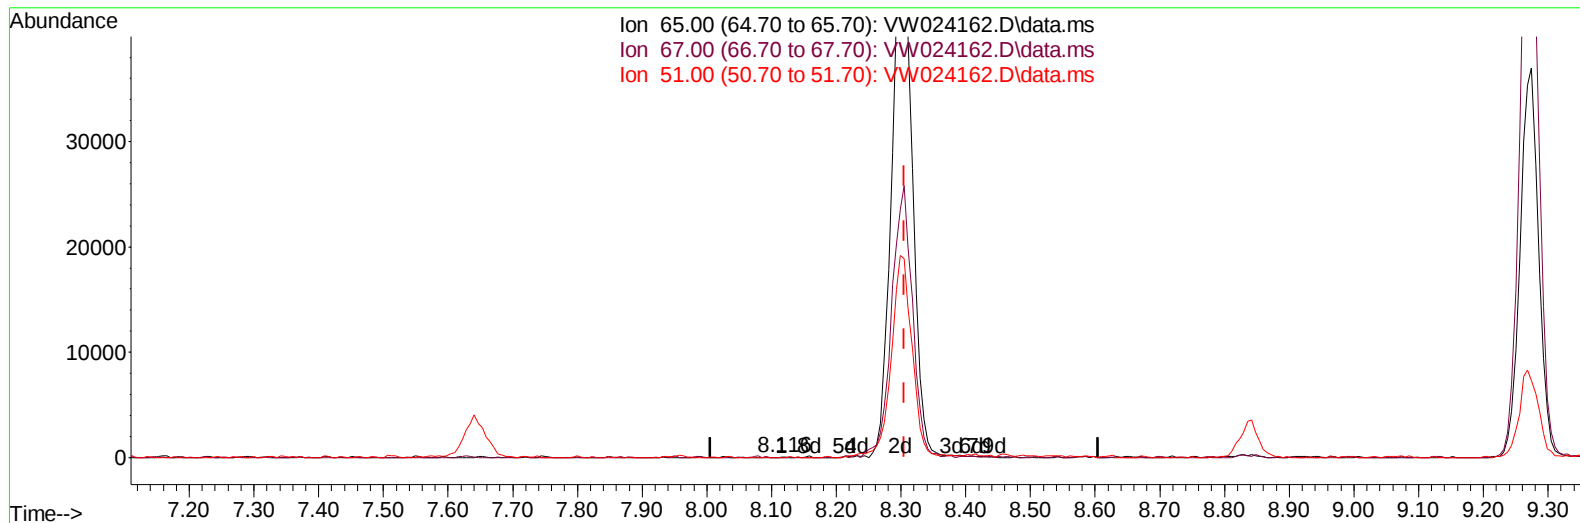

TIC: VW024162.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.116min (-0.189) 0.01 ug/L

response 43

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	62.79
51.00	95.20	81.40
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024162.D
 Acq On : 04 Aug 2022 15:24
 Operator : SY/VA
 Sample : VW0804SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

Quant Time: Aug 05 02:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

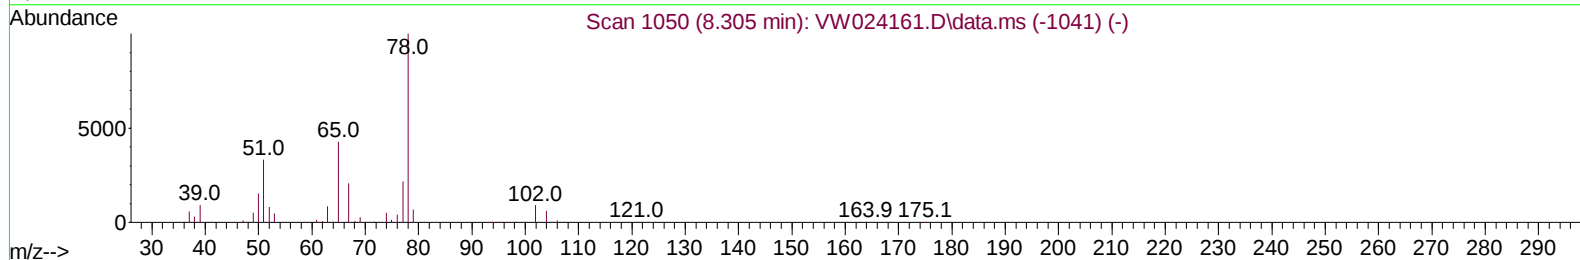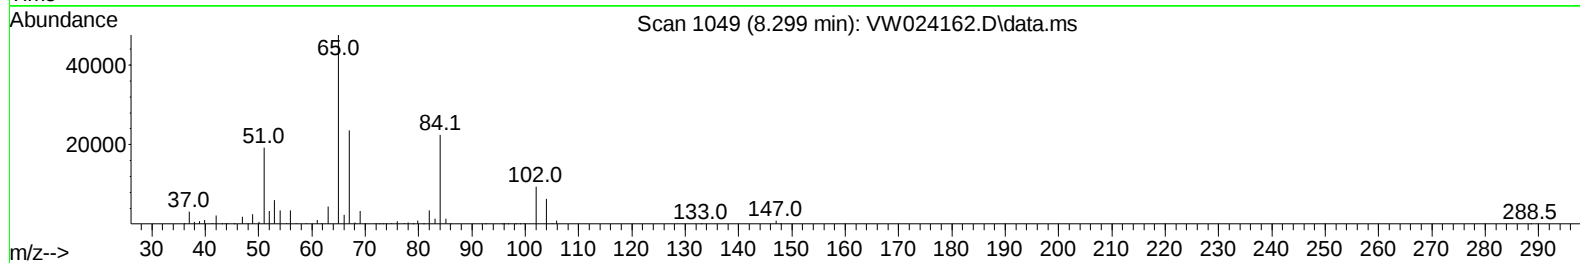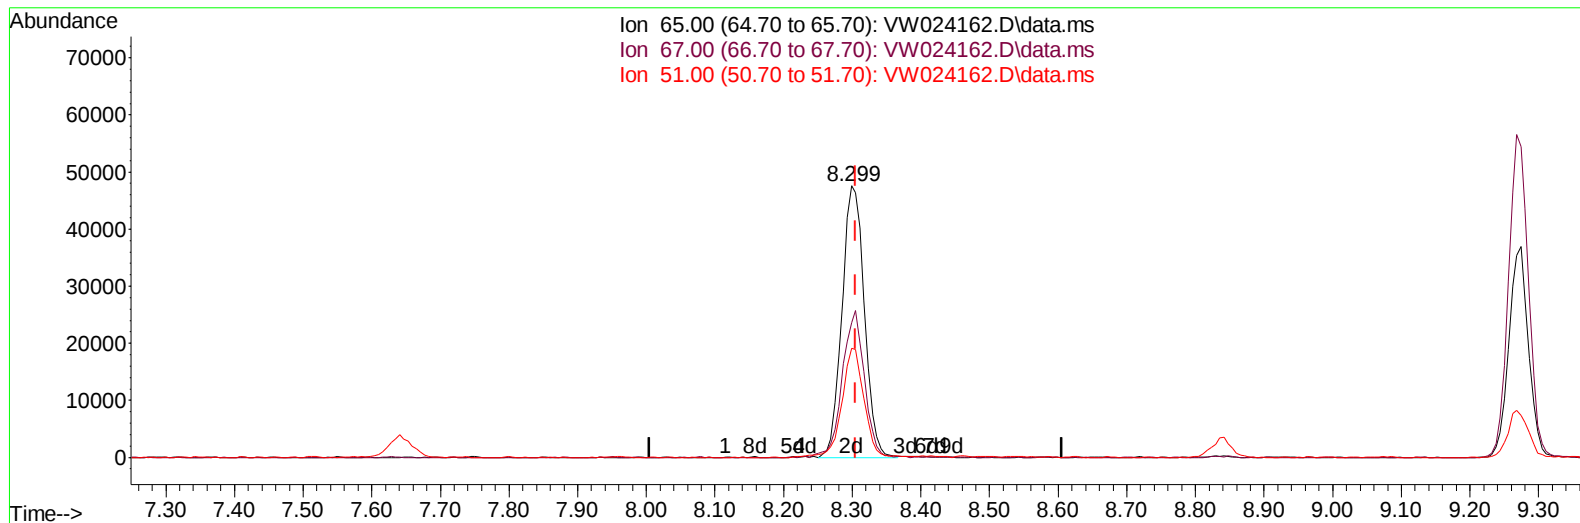

TIC: VW024162.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 20.96 ug/L m

response 107814

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.03#
51.00	95.20	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024162.D
 Acq On : 04 Aug 2022 15:24
 Operator : SY/VA
 Sample : VW0804SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

Quant Time: Aug 05 02:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.835	114		306221	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		298298	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		139829	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		156315	24.421	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	97.680%	
7) Chloroethane-d5	2.873	69		93165	23.365	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	93.480%	
11) 1,1-Dichloroethene-d2	4.001	63		121200	16.615	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	66.440%	
21) 2-Butanone-d5	7.074	46		52199	43.834	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	87.660%	
24) Chloroform-d	7.641	84		196380	21.195	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	84.760%	
26) 1,2-Dichloroethane-d4	8.299	65		107814m	20.959	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	83.840%	
32) Benzene-d6	8.268	84		384090	21.833	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	87.320%	
36) 1,2-Dichloropropane-d6	9.268	67		113826	21.914	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	87.640%	
41) Toluene-d8	10.323	98		353106	21.474	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	85.880%	
43) trans-1,3-Dichloroprop...	10.573	79		46969	20.645	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	82.560%	
47) 2-Hexanone-d5	10.920	63		40611	42.329	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	84.660%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		103271	20.492	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	81.960%	
66) 1,2-Dichlorobenzene-d4	13.853	152		120389	23.528	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	94.120%	
Target Compounds							
13) Acetone	4.117	43		3861m	4.404	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
Data File : VW024162.D
Acq On : 04 Aug 2022 15:24
Operator : SY/VA
Sample : VW0804SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK569

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/07/2022
Supervised By :Mahesh Dadoda 08/08/2022

Quant Time: Aug 05 02:51:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 01:00:42 2022
Response via : Initial Calibration

