




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024175.D
 Acq On : 04 Aug 2022 21:10
 Operator : SY/VA
 Sample : N4004-08
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY136

Manual IntegrationsAPPROVED

Quant Time: Aug 05 01:04:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

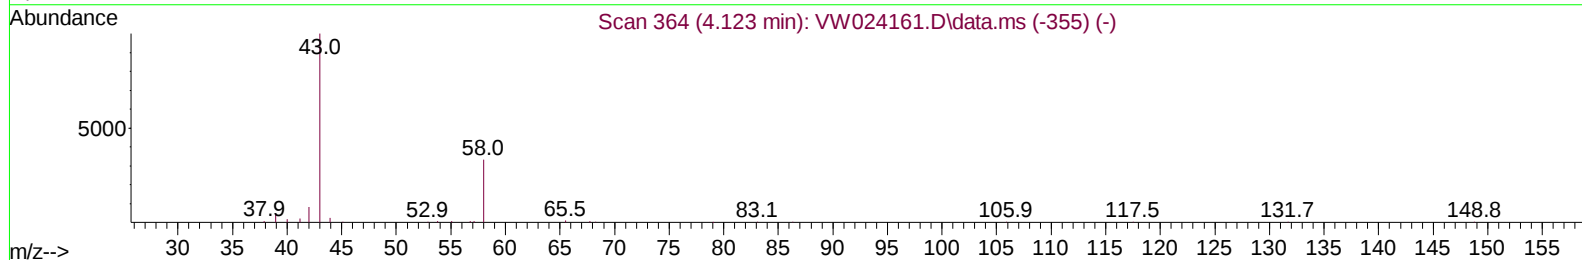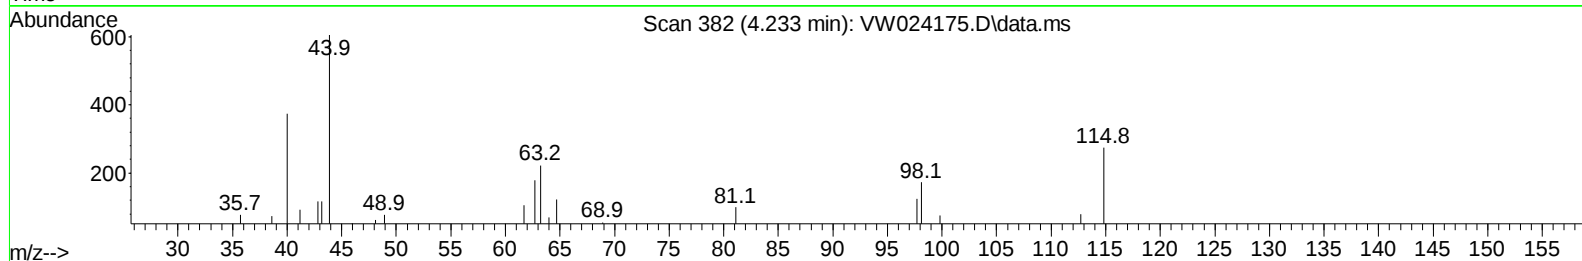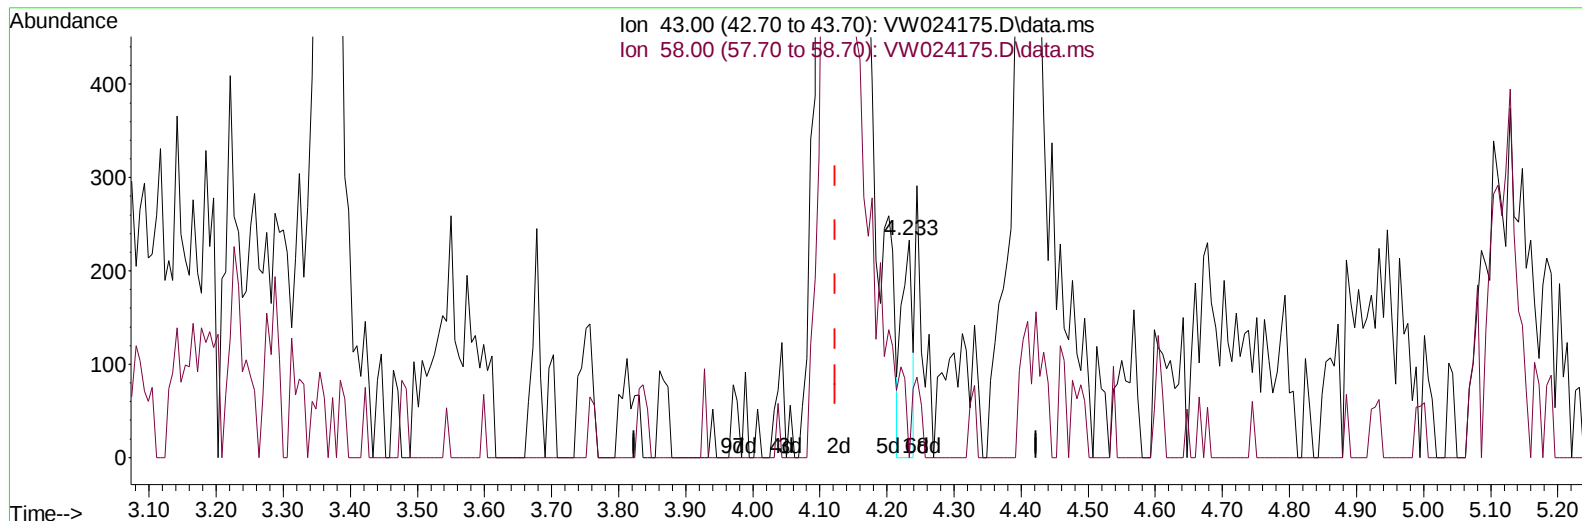

TIC: VW024175.D\data.ms

(13) Acetone (T)

4.233min (+ 0.110) 0.24 ug/L

response 253

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	26.48
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024175.D
 Acq On : 04 Aug 2022 21:10
 Operator : SY/VA
 Sample : N4004-08
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY136

Manual IntegrationsAPPROVED

Quant Time: Aug 05 01:04:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

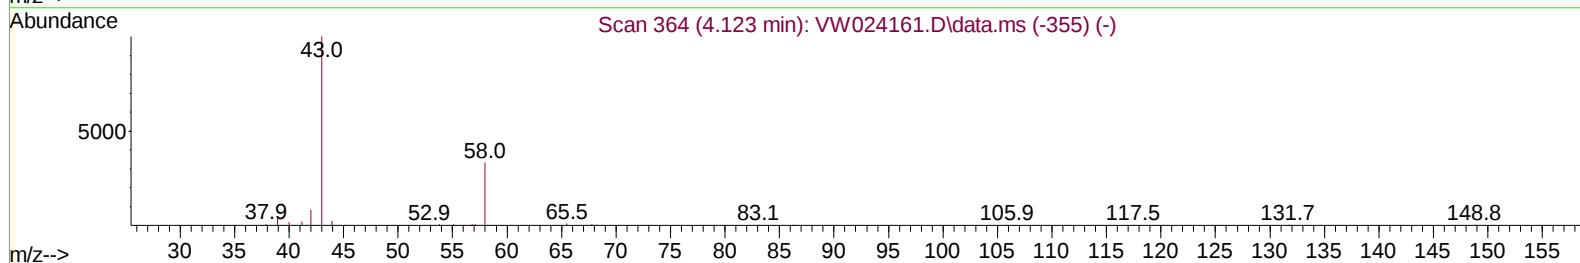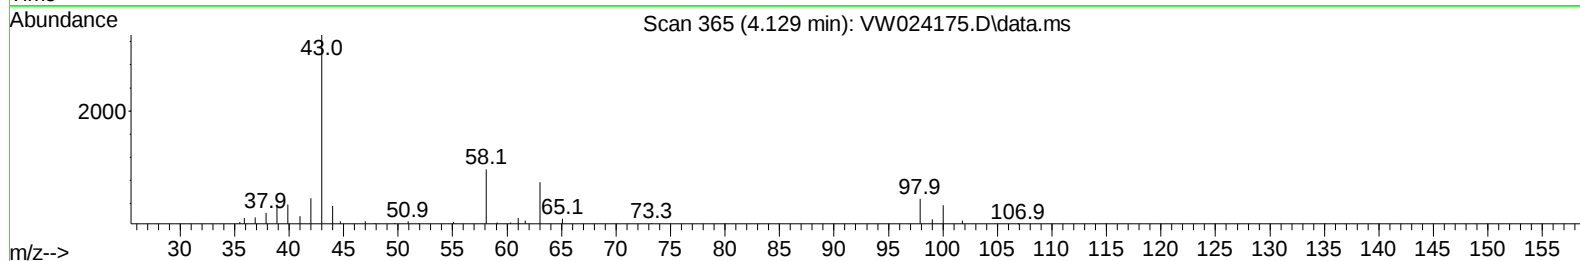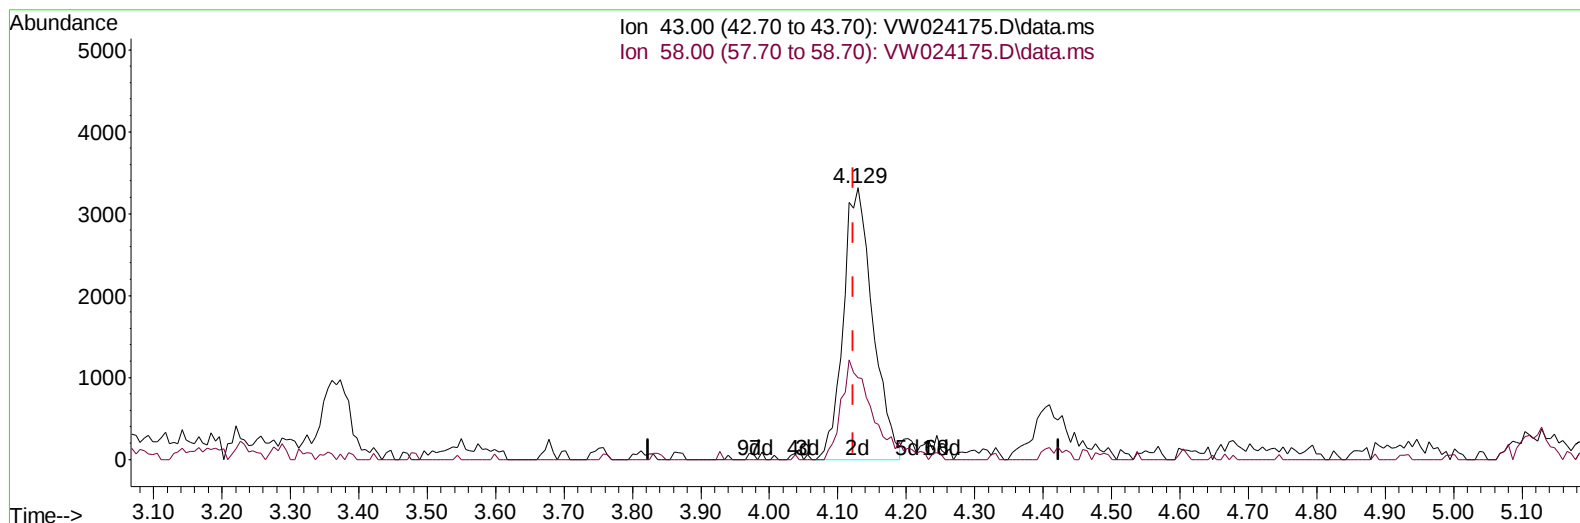

TIC: VW024175.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 9.29 ug/L m

response 9873

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	0.68
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024175.D
 Acq On : 04 Aug 2022 21:10
 Operator : SY/VA
 Sample : N4004-08
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY136

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

Quant Time: Aug 05 01:04:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.836	114		371248	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		308181	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		120086	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		211769	27.290	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	109.160%	
7) Chloroethane-d5	2.873	69		109624	22.678	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	90.720%	
11) 1,1-Dichloroethene-d2	4.007	63		173030	19.565	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	78.280%	
21) 2-Butanone-d5	7.080	46		94384	65.376	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	130.760%	
24) Chloroform-d	7.647	84		259544	23.105	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	92.440%	
26) 1,2-Dichloroethane-d4	8.305	65		155993	25.013	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	100.040%	
32) Benzene-d6	8.269	84		518848	28.547	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	114.200%	
36) 1,2-Dichloropropane-d6	9.275	67		153931	28.685	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	114.720%	
41) Toluene-d8	10.323	98		443649	26.115	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	104.440%	
43) trans-1,3-Dichloroprop...	10.579	79		62339	26.522	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	106.080%	
47) 2-Hexanone-d5	10.921	63		72357	73.000	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	146.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		148304	28.485	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	113.920%	
66) 1,2-Dichlorobenzene-d4	13.853	152		110947	25.247	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	101.000%	
Target Compounds							
13) Acetone	4.129	43		9873m	9.289	ug/L	
16) Methylene chloride	4.909	84		60360	9.220	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
Data File : VW024175.D
Acq On : 04 Aug 2022 21:10
Operator : SY/VA
Sample : N4004-08
Misc : 5.78g/10mL/MSVOA_W/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY136

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/07/2022
Supervised By :Mahesh Dadoda 08/08/2022

Quant Time: Aug 05 01:04:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 01:00:42 2022
Response via : Initial Calibration

