




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024179.D
 Acq On : 04 Aug 2022 22:48
 Operator : SY/VA
 Sample : N4004-12
 Misc : 3.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY142

Manual IntegrationsAPPROVED

Quant Time: Aug 05 01:05:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

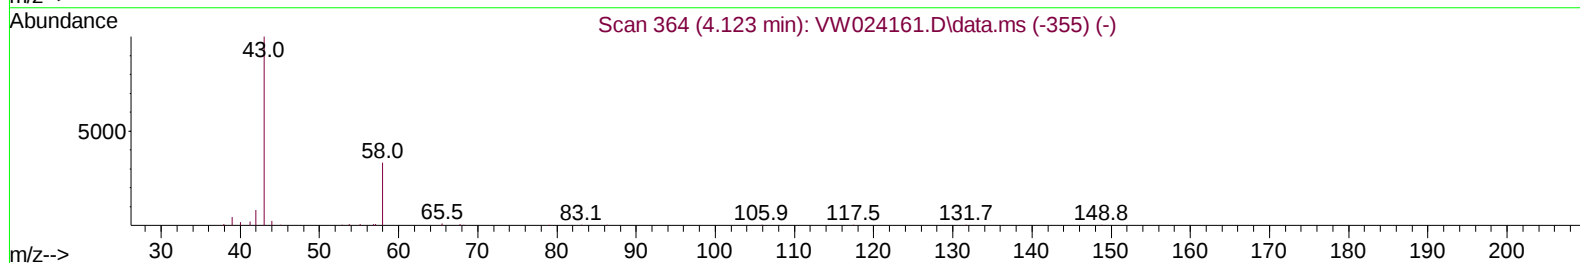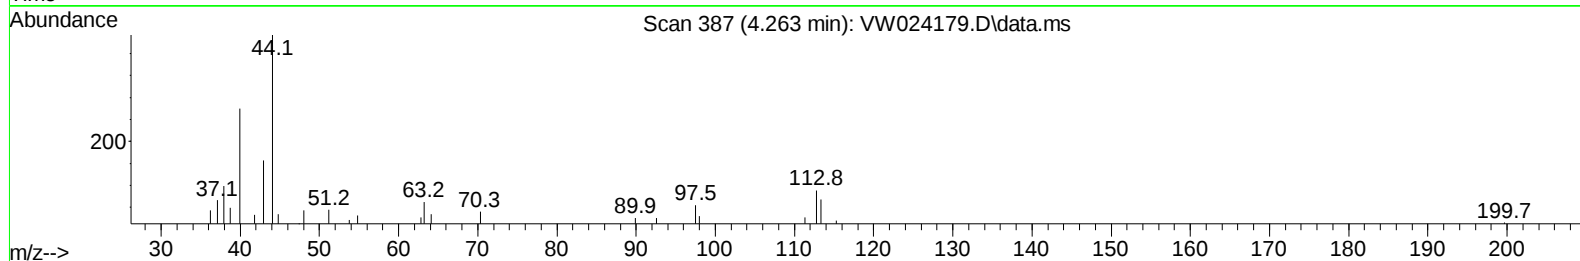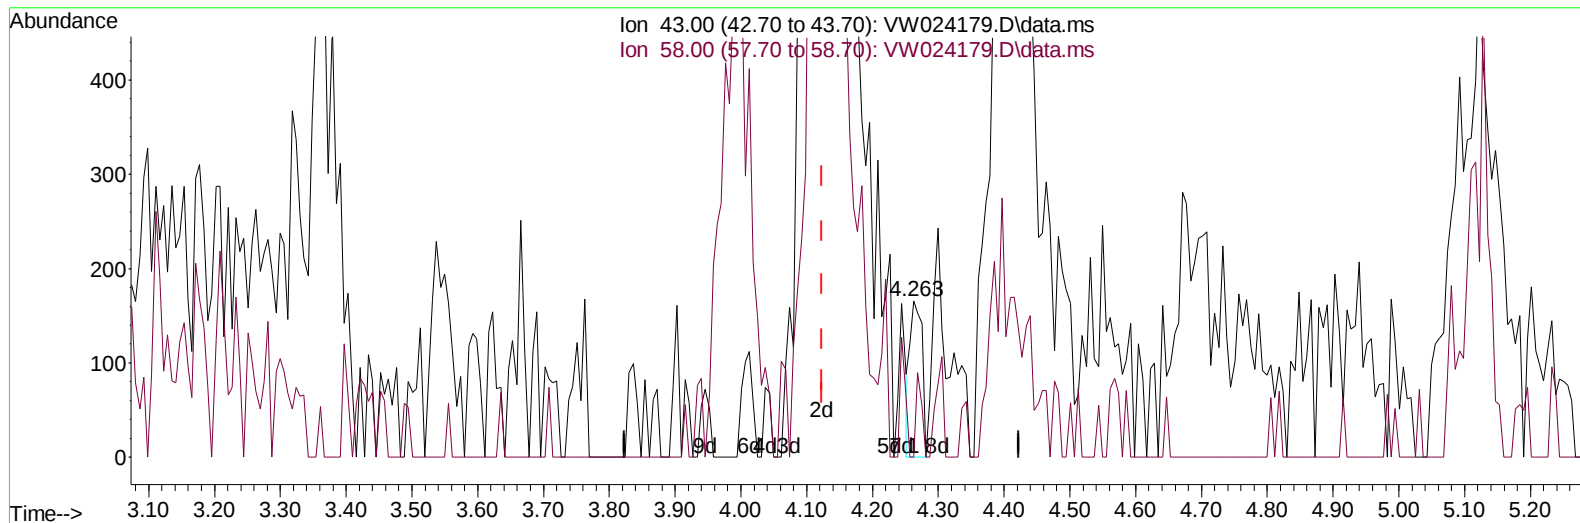

TIC: VW024179.D\data.ms

(13) Acetone (T)

4.263min (+ 0.140) 0.16 ug/L

response 213

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	24.88
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024179.D
 Acq On : 04 Aug 2022 22:48
 Operator : SY/VA
 Sample : N4004-12
 Misc : 3.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY142

Manual IntegrationsAPPROVED

Quant Time: Aug 05 01:05:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

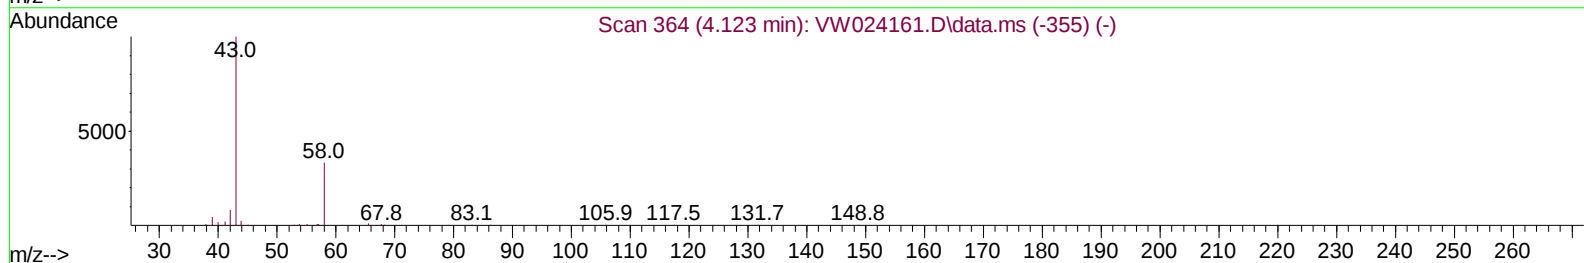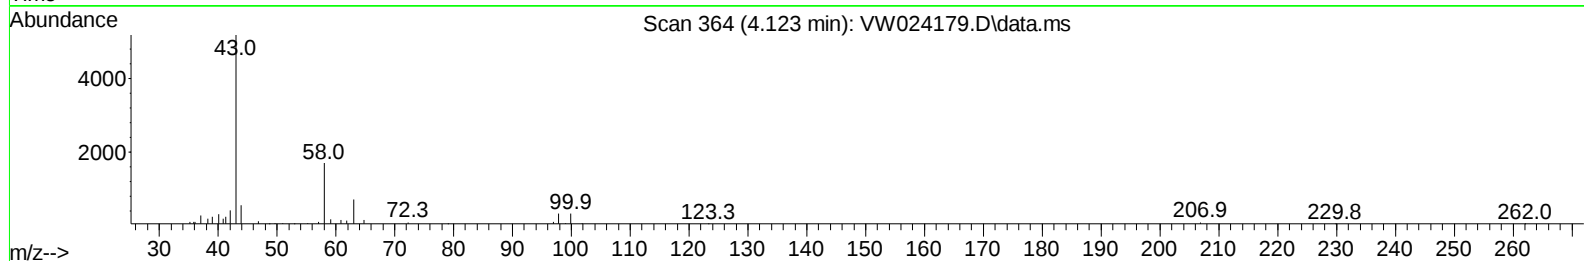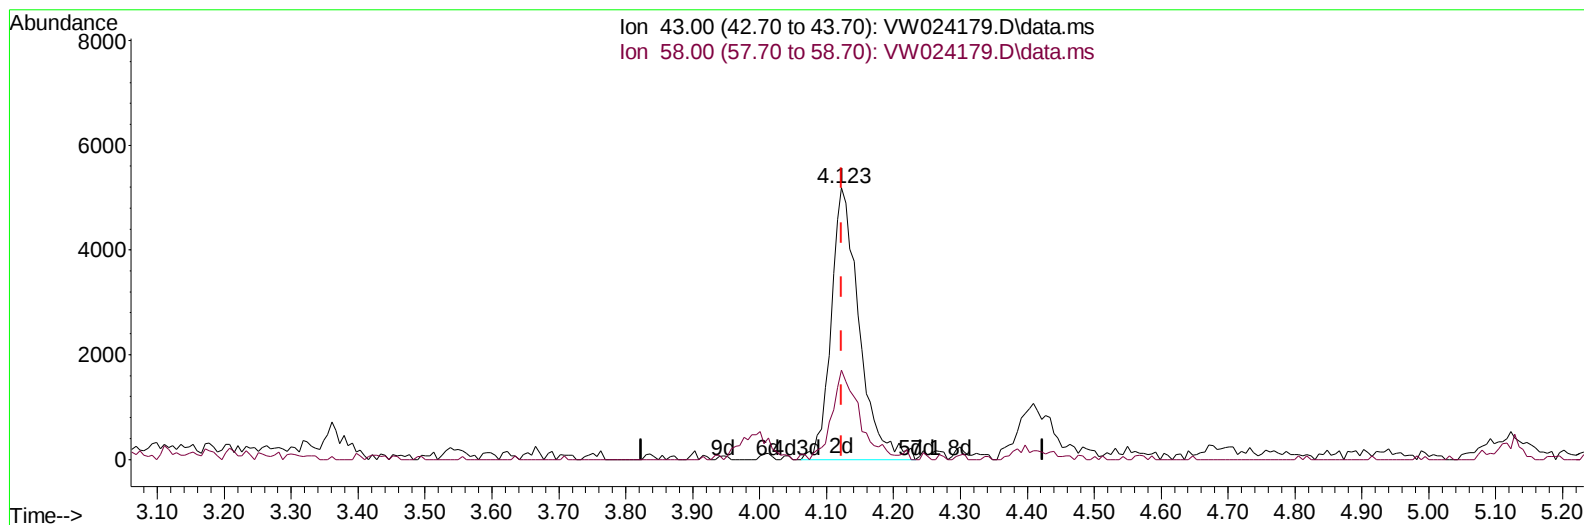

TIC: VW024179.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 11.60 ug/L m

response 15086

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	0.35
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024179.D
 Acq On : 04 Aug 2022 22:48
 Operator : SY/VA
 Sample : N4004-12
 Misc : 3.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY142

Manual IntegrationsAPPROVED

Quant Time: Aug 05 01:05:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 05 01:00:42 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/07/2022
 Supervised By :Mahesh Dadoda 08/08/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		454130	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117		354252	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		120159	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.342	65		260857	27.481	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	109.920%	
7) Chloroethane-d5	2.873	69		133593	22.592	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	90.360%	
11) 1,1-Dichloroethene-d2	4.001	63		200705	18.553	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	74.200%	
21) 2-Butanone-d5	7.079	46		91980	52.083	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	104.160%	
24) Chloroform-d	7.646	84		325502	23.689	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	94.760%	
26) 1,2-Dichloroethane-d4	8.299	65		180755	23.694	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	94.760%	
32) Benzene-d6	8.268	84		637070	30.493	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	121.960%	
36) 1,2-Dichloropropane-d6	9.268	67		185555	30.081	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	120.320%#	
41) Toluene-d8	10.323	98		532936	27.291	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	109.160%	
43) trans-1,3-Dichloroprop...	10.579	79		65479	24.235	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	96.920%	
47) 2-Hexanone-d5	10.920	63		68638	60.242	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	120.480%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		148632	24.835	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	99.320%	
66) 1,2-Dichlorobenzene-d4	13.853	152		125638	28.573	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	114.280%	
Target Compounds							
13) Acetone	4.123	43		15086m	11.603	ug/L	
16) Methylene chloride	4.903	84		54949	6.861	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
Data File : VW024179.D
Acq On : 04 Aug 2022 22:48
Operator : SY/VA
Sample : N4004-12
Misc : 3.78g/10mL/MSVOA_W/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY142

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/07/2022
Supervised By :Mahesh Dadoda 08/08/2022

Quant Time: Aug 05 01:05:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 05 01:00:42 2022
Response via : Initial Calibration

