
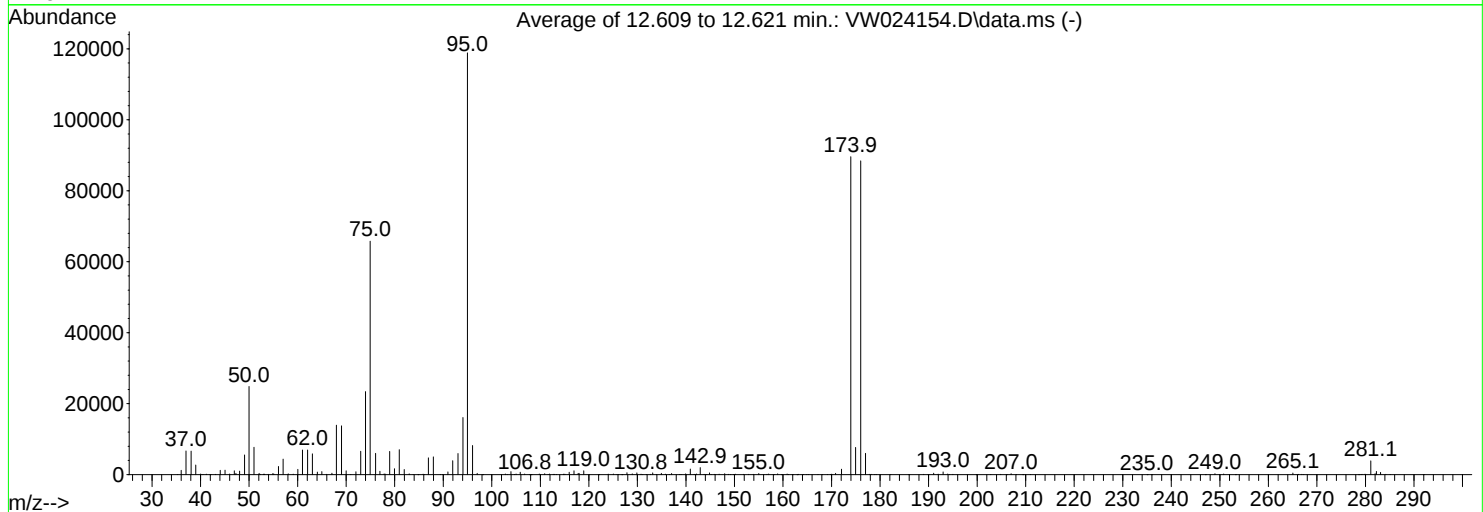


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080422\
 Data File : VW024154.D
 Acq On : 04 Aug 2022 08:26
 Operator : SY/VA
 Sample : BFB402
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB402

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Title : SFAM01.0
 Last Update : Fri Aug 05 23:43:03 2022

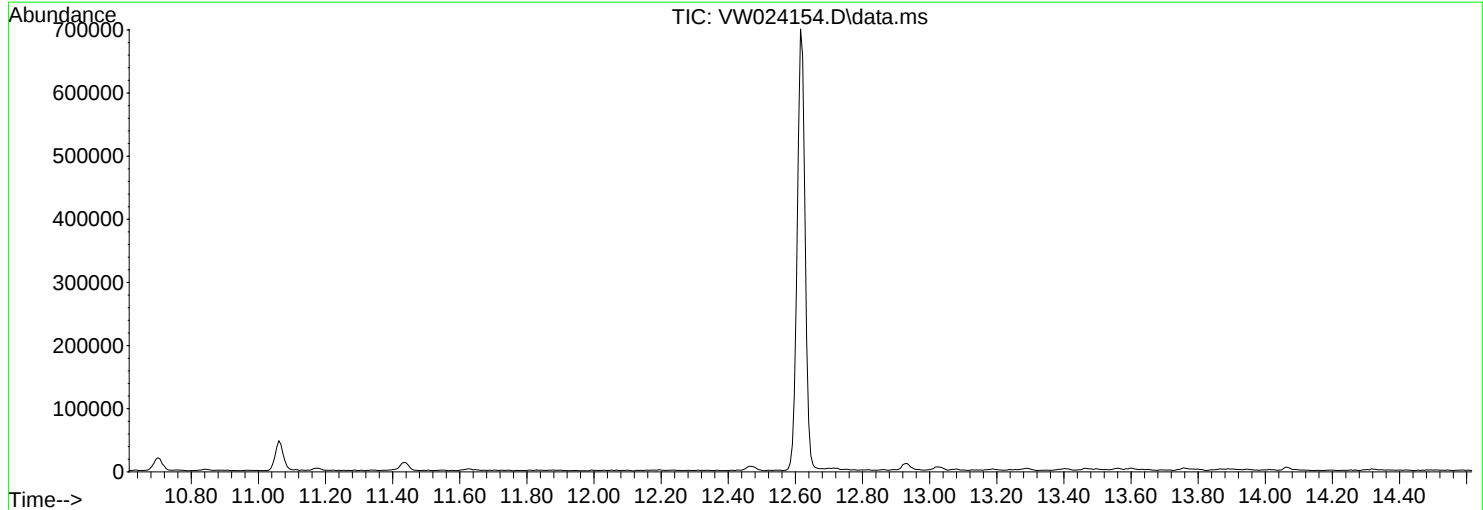

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	24842	PASS
75	95	30	80	55.4	65808	PASS
95	95	100	100	100.0	118867	PASS
96	95	5	9	6.9	8194	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.4	89605	PASS
175	174	5	9	8.6	7685	PASS
176	174	95	105	98.7	88400	PASS
177	176	5	10	6.8	6006	PASS

m/z	Abundance
36.00	72.0
39.90	235.0
40.90	85.0
42.00	99.0
42.60	84.0
43.80	253.0
45.30	58.0
46.50	129.0
47.70	52.0
50.10	59.0
59.70	57.0
63.70	98.0
68.70	52.0
70.00	57.0
73.00	109.0
74.90	77.0
87.10	90.0
91.10	53.0
115.50	71.0
155.90	69.0
187.50	91.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

m/z	Abundance
36.00	1154.0
37.00	6780.0
38.10	6652.0
39.00	2893.0
39.90	308.0
41.20	202.0
41.90	87.0
43.10	107.0
44.10	1291.0
45.00	1183.0
46.00	234.0
47.30	1135.0
48.10	912.0
49.00	4580.0
50.00	21912.0
51.00	7008.0
52.10	353.0
52.90	267.0
53.30	148.0
53.90	116.0
54.90	429.0
56.10	2199.0
57.00	3686.0
58.10	166.0
59.10	183.0
60.10	1695.0
61.00	5837.0
62.10	6061.0
63.00	5503.0
64.00	658.0
65.00	1003.0
66.00	167.0
67.10	386.0
68.00	12472.0
69.10	11736.0
70.00	1076.0
71.00	100.0
71.90	588.0
73.00	5678.0
74.00	19856.0
75.00	57976.0
76.00	5336.0
77.00	872.0
79.00	5857.0
80.00	1406.0
81.00	6779.0
82.00	1233.0
82.90	141.0
84.80	67.0
85.90	151.0
87.00	4388.0
87.90	4451.0
91.00	718.0
92.00	3124.0
93.10	5321.0
94.00	13090.0
95.00	97624.0
96.10	6642.0
97.00	331.0
102.80	179.0
104.00	729.0
105.00	256.0
105.90	658.0
107.00	143.0
109.90	217.0
111.00	264.0
111.60	111.0
112.60	138.0
113.30	114.0
114.70	152.0
115.10	205.0
115.90	507.0
116.90	1099.0
117.80	493.0
119.00	1029.0
124.00	124.0
125.20	143.0
125.80	129.0
127.80	525.0
129.00	173.0
129.90	276.0
131.10	175.0
133.10	669.0
134.90	328.0
135.80	107.0
137.10	219.0
139.10	124.0
140.00	141.0
140.90	1520.0
141.70	224.0
142.20	184.0
142.90	1733.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

143.80	107.0
144.30	120.0
144.90	637.0
145.90	143.0
146.90	241.0
148.00	226.0
149.20	193.0
150.20	194.0
151.90	135.0
153.90	69.0
155.00	245.0
155.80	133.0
156.70	221.0
158.80	205.0
160.90	259.0
161.90	62.0
163.20	199.0
164.20	58.0
165.30	59.0
170.10	169.0
170.90	475.0
172.00	1415.0
174.00	69208.0
175.00	5705.0
176.00	63752.0
177.00	5014.0
178.30	109.0
178.90	157.0
182.20	76.0
189.00	211.0
191.10	496.0
191.90	162.0
193.00	1189.0
194.00	321.0
195.00	152.0
202.80	74.0
204.80	176.0
206.00	69.0
207.00	438.0
208.10	154.0
209.40	51.0
235.00	54.0
247.00	51.0
249.00	334.0
250.90	259.0
253.20	59.0
265.00	689.0
266.30	111.0
267.30	119.0
278.60	55.0
279.10	175.0
280.00	91.0
281.10	5022.0
282.30	1417.0
283.10	840.0
284.20	133.0
285.10	83.0
291.90	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

m/z	Abundance
36.10	1394.0
37.00	6925.0
38.00	6718.0
39.00	2968.0
40.10	287.0
41.20	119.0
42.00	101.0
43.10	233.0
44.00	1267.0
45.10	1435.0
46.00	248.0
46.90	1866.0
48.10	958.0
49.00	6397.0
50.00	27704.0
51.00	8201.0
52.00	318.0
52.30	296.0
53.10	201.0
54.00	75.0
54.90	514.0
56.10	2486.0
57.00	5458.0
58.10	179.0
58.90	93.0
60.00	1177.0
61.00	8258.0
62.00	7719.0
63.00	6807.0
64.00	693.0
65.00	1045.0
65.80	78.0
66.90	307.0
68.00	15435.0
69.00	15798.0
70.10	1265.0
70.90	99.0
72.00	992.0
73.10	7697.0
74.00	26048.0
75.00	74640.0
76.10	6293.0
76.90	1090.0
77.80	592.0
78.90	7077.0
79.90	2067.0
80.90	7121.0
81.90	1710.0
83.00	264.0
83.80	115.0
85.80	107.0
86.10	111.0
87.00	5524.0
88.00	5040.0
89.50	69.0
90.90	1062.0
91.90	4456.0
93.00	6793.0
94.10	18480.0
95.00	134656.0
96.00	9250.0
97.00	410.0
102.70	121.0
103.20	187.0
103.90	784.0
104.90	172.0
105.90	767.0
106.80	182.0
107.80	65.0
109.70	158.0
110.80	278.0
111.90	267.0
112.70	186.0
115.00	202.0
115.90	635.0
116.90	1051.0
118.00	1039.0
118.90	1044.0
120.10	95.0
123.90	136.0
125.00	298.0
126.10	95.0
126.80	55.0
127.90	669.0
129.00	273.0
129.90	644.0
130.70	259.0
131.80	89.0
132.70	236.0
133.20	330.0
135.00	446.0
135.80	150.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

136.60	173.0
137.10	307.0
138.70	102.0
140.00	233.0
140.90	1616.0
142.10	324.0
143.00	2544.0
143.70	156.0
144.90	610.0
145.80	181.0
146.90	100.0
148.00	383.0
148.80	133.0
150.10	156.0
151.80	118.0
152.90	84.0
153.90	193.0
154.90	396.0
156.00	78.0
157.10	310.0
158.00	62.0
158.90	344.0
160.70	133.0
161.10	119.0
162.90	62.0
164.20	51.0
165.30	60.0
169.20	66.0
170.00	196.0
170.80	325.0
172.10	1642.0
174.00	96736.0
174.90	8785.0
176.00	100072.0
177.00	6264.0
178.10	233.0
179.20	101.0
185.90	51.0
189.00	53.0
191.10	358.0
192.00	209.0
193.00	673.0
193.90	165.0
195.00	104.0
202.80	76.0
204.90	129.0
207.00	279.0
211.00	76.0
235.90	55.0
249.10	331.0
250.80	145.0
251.90	65.0
265.10	433.0
266.20	91.0
266.90	110.0
279.30	121.0
279.90	185.0
281.10	4368.0
282.20	1283.0
283.20	691.0
284.20	90.0
285.10	91.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

m/z	Abundance
35.30	90.0
36.00	1390.0
37.00	6272.0
38.00	6495.0
39.00	2274.0
40.00	262.0
40.50	163.0
41.20	114.0
42.00	124.0
42.50	90.0
44.00	1125.0
45.10	1134.0
46.30	259.0
47.00	1437.0
47.90	1063.0
49.10	5639.0
50.00	25088.0
51.00	7957.0
52.10	358.0
53.00	182.0
53.90	69.0
55.10	494.0
56.00	2252.0
57.00	3943.0
58.00	314.0
59.20	188.0
60.10	1572.0
61.00	6768.0
62.00	7005.0
63.10	5352.0
64.10	829.0
65.10	513.0
65.90	93.0
67.10	476.0
68.00	13893.0
69.00	13748.0
70.00	1088.0
72.10	901.0
73.00	6695.0
74.00	24376.0
75.00	65040.0
76.10	6312.0
77.00	876.0
78.00	535.0
78.90	6629.0
80.00	1537.0
81.00	7270.0
82.00	1342.0
83.10	307.0
85.80	217.0
86.90	4615.0
88.00	5470.0
89.30	62.0
89.90	110.0
91.00	705.0
92.00	4244.0
93.00	5750.0
94.00	16728.0
95.00	124320.0
96.00	8691.0
97.00	309.0
98.10	69.0
102.90	257.0
103.90	1043.0
104.70	142.0
105.10	150.0
105.80	631.0
106.70	284.0
108.10	65.0
109.80	140.0
110.90	236.0
111.90	328.0
112.90	250.0
114.80	229.0
116.00	878.0
117.00	1067.0
117.80	587.0
119.00	1169.0
120.10	67.0
122.00	68.0
124.10	142.0
125.00	111.0
127.90	432.0
128.90	279.0
129.90	512.0
130.80	190.0
131.90	64.0
133.10	443.0
133.90	180.0
135.00	322.0
135.80	119.0
137.00	479.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

138.90	90.0
139.90	261.0
140.90	1559.0
141.90	211.0
142.90	1720.0
144.00	188.0
144.70	195.0
145.20	190.0
146.10	207.0
146.70	133.0
148.10	196.0
148.70	160.0
149.80	160.0
151.90	63.0
153.00	190.0
153.80	73.0
155.10	330.0
156.10	126.0
157.00	293.0
159.00	181.0
159.70	57.0
160.90	195.0
163.20	82.0
164.90	76.0
167.20	92.0
168.10	79.0
169.10	75.0
169.80	105.0
170.90	284.0
172.10	1504.0
173.90	102872.0
175.00	8566.0
176.00	101376.0
177.00	6739.0
177.90	220.0
179.20	110.0
189.90	58.0
190.90	313.0
192.00	75.0
193.10	395.0
194.30	79.0
194.90	52.0
199.80	57.0
207.10	148.0
248.90	208.0
249.90	73.0
250.70	100.0
252.00	92.0
265.00	186.0
266.10	83.0
266.90	117.0
279.30	128.0
279.80	78.0
281.10	2293.0
282.00	816.0
283.00	361.0
284.10	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402