

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080525\
 Data File : VW032020.D
 Acq On : 05 Aug 2025 17:53
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Quant Time: Aug 06 03:57:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W072225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 23 08:18:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.959	168	200982	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	405616	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.635	117	388915	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	188660	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	134840	44.350	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	88.700%
35) Dibromofluoromethane	7.898	113	120844	43.844	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	87.680%
50) Toluene-d8	10.325	98	474710	45.508	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	91.020%
62) 4-Bromofluorobenzene	12.617	95	180319	45.018	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	90.040%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080525\
Data File : VW032020.D
Acq On : 05 Aug 2025 17:53
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Quant Time: Aug 06 03:57:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W072225S.M
Quant Title : SW846 8260
QLast Update : Wed Jul 23 08:18:46 2025
Response via : Initial Calibration




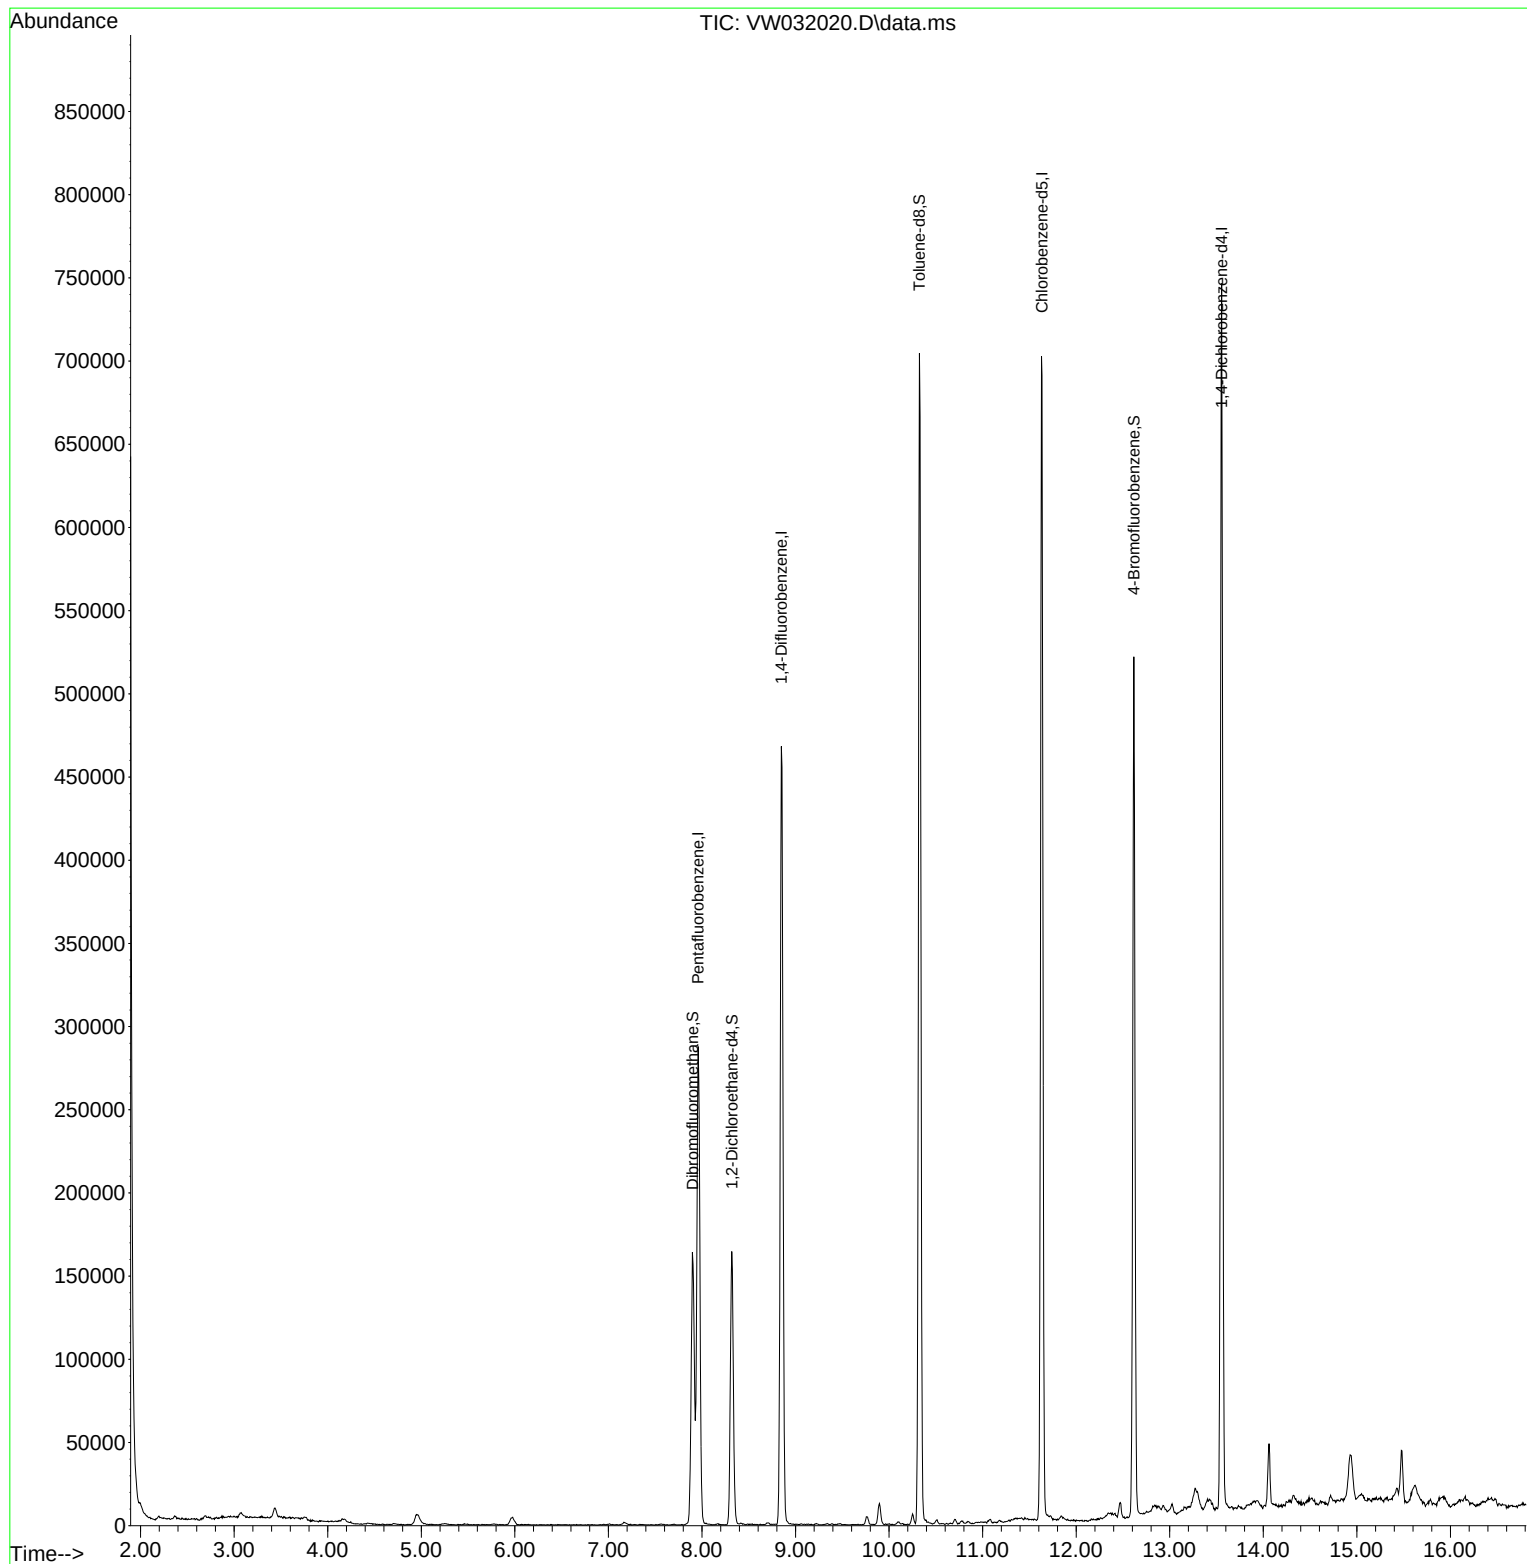


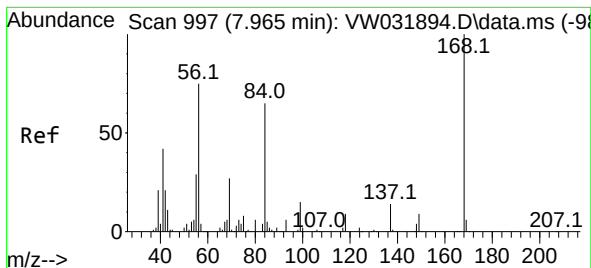

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.959 min Scan# 997
Delta R.T. -0.006 min
Lab File: VW032020.D
Acq: 05 Aug 2025 17:53




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 200982
Ion Ratio Lower Upper
168 100
99 66.4 48.2 72.2

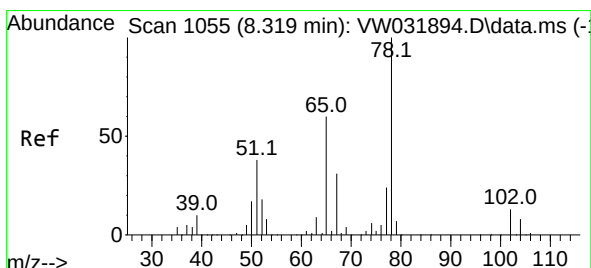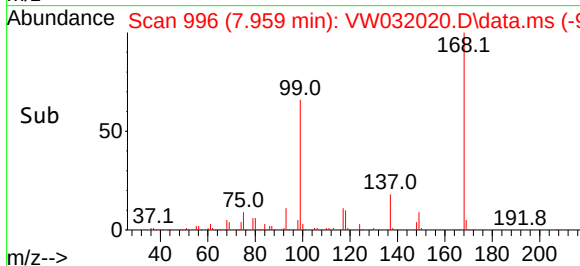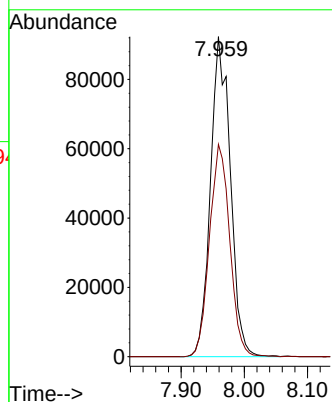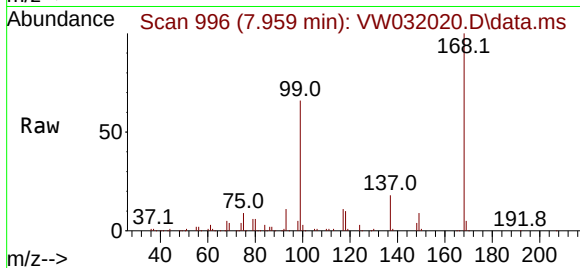

#33
1,2-Dichloroethane-d4
Concen: 44.350 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW032020.D
Acq: 05 Aug 2025 17:53

Tgt Ion: 65 Resp: 134840
Ion Ratio Lower Upper
65 100
67 51.7 0.0 101.4


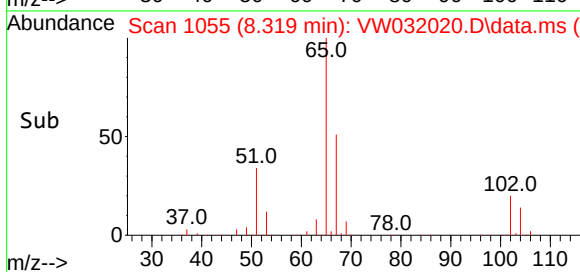
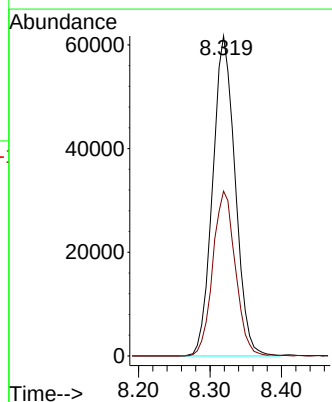
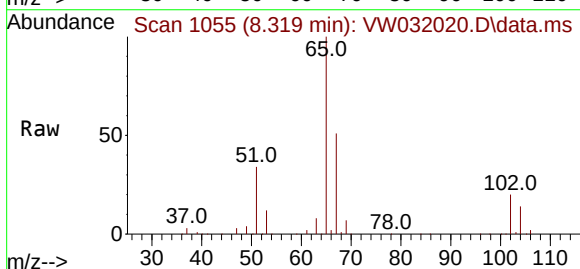


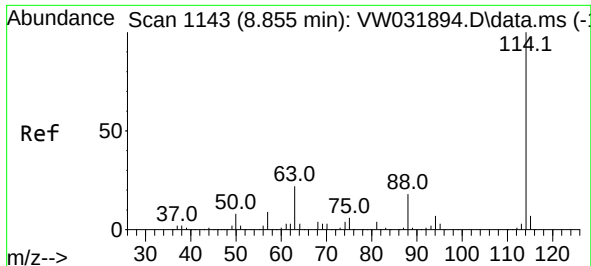

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.849 min Scan# 1143
Delta R.T. -0.006 min
Lab File: VW032020.D
Acq: 05 Aug 2025 17:53




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion:114 Resp: 405616
Ion Ratio Lower Upper
114 100
63 22.2 0.0 44.2
88 17.0 0.0 35.6

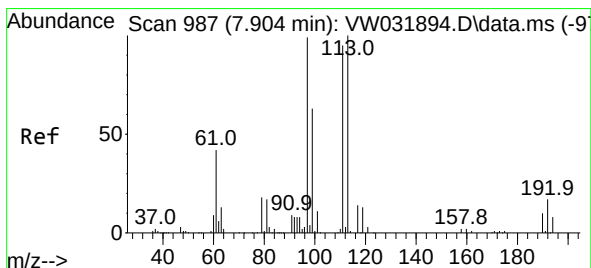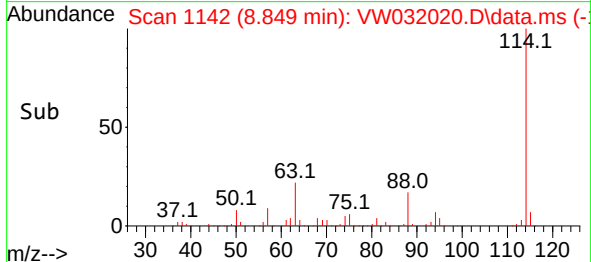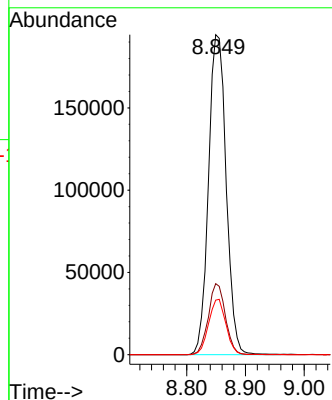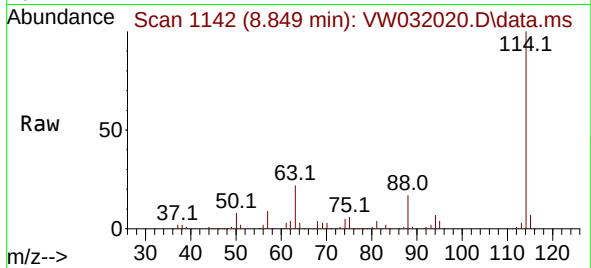

#35
Dibromofluoromethane
Concen: 43.844 ug/l
RT: 7.898 min Scan# 986
Delta R.T. -0.006 min
Lab File: VW032020.D
Acq: 05 Aug 2025 17:53

Tgt Ion:113 Resp: 120844
Ion Ratio Lower Upper
113 100
111 103.6 79.9 119.9
192 16.1 12.6 19.0


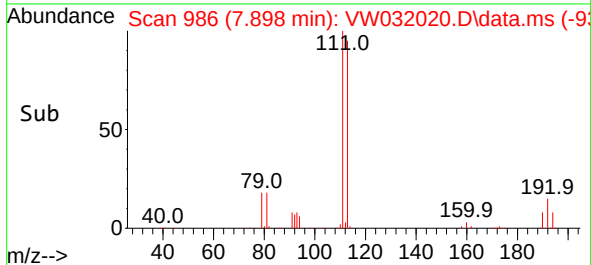
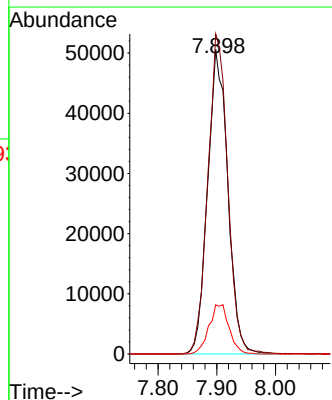
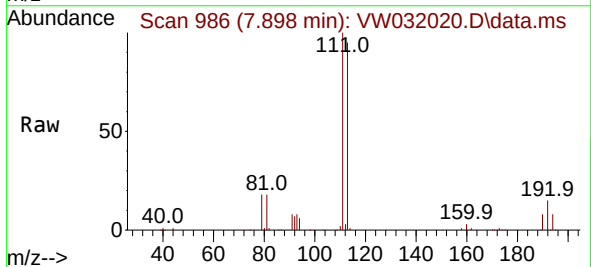


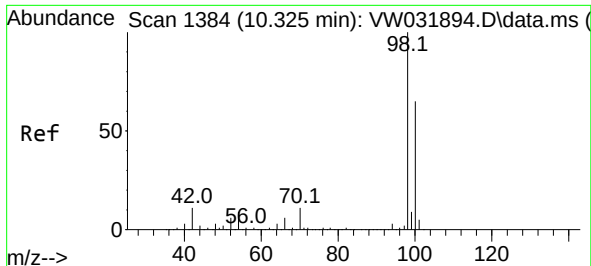

#50
Toluene-d8
Concen: 45.508 ug/l
RT: 10.325 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW032020.D
Acq: 05 Aug 2025 17:53




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 474710
Ion Ratio Lower Upper
98 100
100 66.8 51.7 77.5

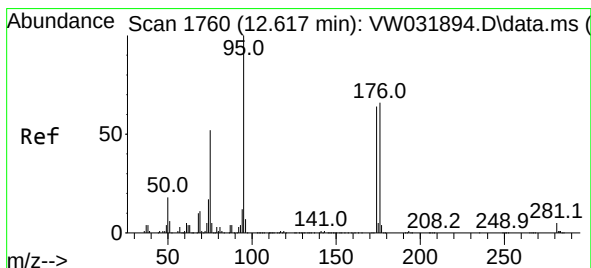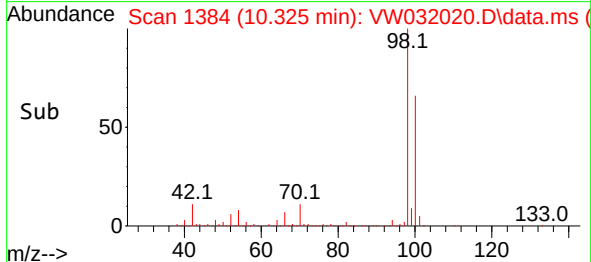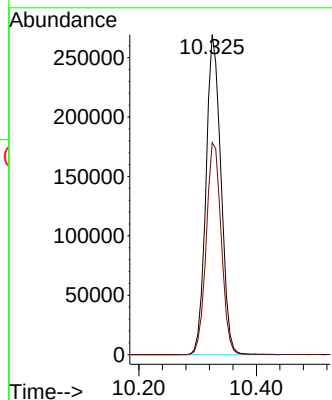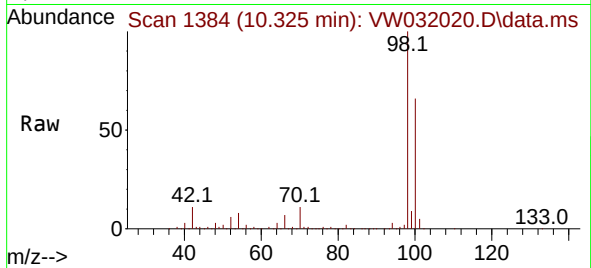

#62
4-Bromofluorobenzene
Concen: 45.018 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. -0.000 min
Lab File: VW032020.D
Acq: 05 Aug 2025 17:53

Tgt Ion: 95 Resp: 180319
Ion Ratio Lower Upper
95 100
174 68.5 0.0 129.8
176 64.3 0.0 130.4


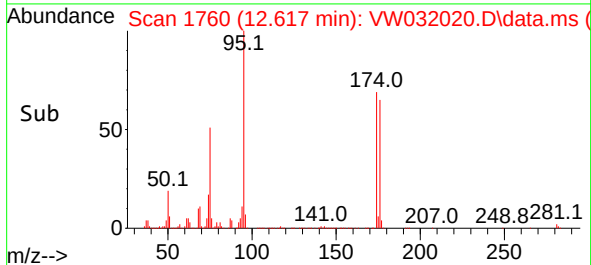
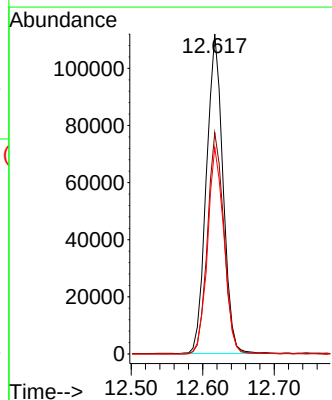
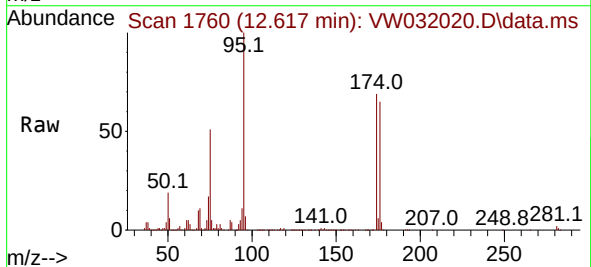


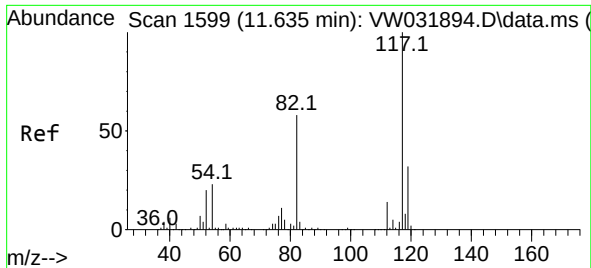

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW032020.D
Acq: 05 Aug 2025 17:53

Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 388915
Ion Ratio Lower Upper
117 100
82 54.2 46.5 69.7
119 32.2 25.8 38.6

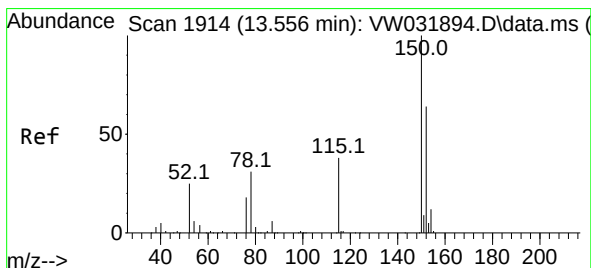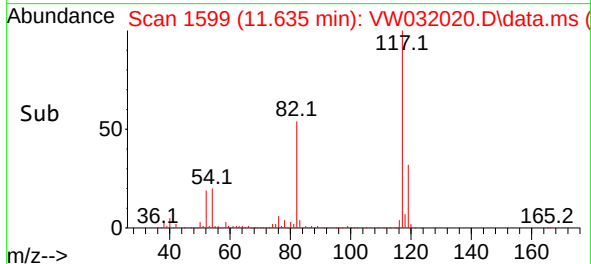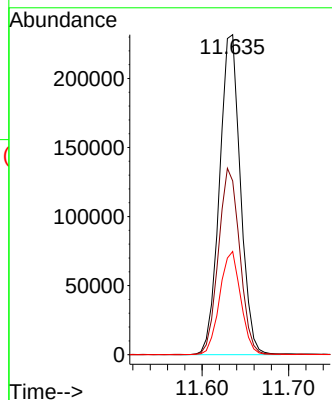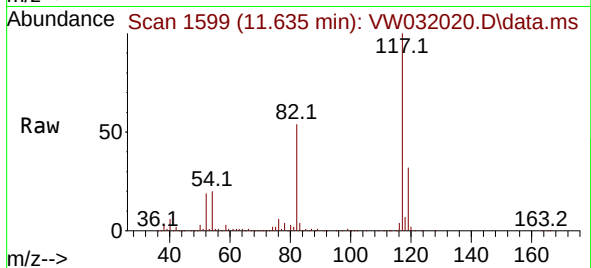

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. -0.000 min
Lab File: VW032020.D
Acq: 05 Aug 2025 17:53

Tgt Ion:152 Resp: 188660
Ion Ratio Lower Upper
152 100
115 65.7 33.4 100.1
150 158.0 0.0 352.2

