

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080822\
 Data File : VW024202.D
 Acq On : 08 Aug 2022 17:36
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK530

Quant Time: Aug 09 04:15:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 09 04:14:12 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	327237	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	317364	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	157330	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	134088	19.603	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	78.400%	
7) Chloroethane-d5	2.873	69	105509	24.762	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	99.040%	
11) 1,1-Dichloroethene-d2	4.172	63	456	0.058	ug/L	0.17
Spiked Amount	25.000	Range 45 - 110	Recovery	=	0.240%#	
21) 2-Butanone-d5	7.080	46	57717	45.355	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	90.720%	
24) Chloroform-d	7.641	84	216348	21.850	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	87.400%	
26) 1,2-Dichloroethane-d4	8.299	65	120643	21.946	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	87.800%	
32) Benzene-d6	8.268	84	419618	22.419	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	89.680%	
36) 1,2-Dichloropropane-d6	9.268	67	124146	22.465	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	89.840%	
41) Toluene-d8	10.323	98	382434	21.860	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	87.440%	
43) trans-1,3-Dichloroprop...	10.579	79	52322	21.616	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	86.480%	
47) 2-Hexanone-d5	10.927	63	47288	46.328	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	92.660%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	114938	21.437	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	85.760%	
66) 1,2-Dichlorobenzene-d4	13.853	152	140714	24.441	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	97.760%	
Target Compounds						
13) Acetone	4.117	43	4082	4.357	ug/L	92
34) Trichloroethene	8.835	95	10238	2.066	ug/L #	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080822\
Data File : VW024202.D
Acq On : 08 Aug 2022 17:36
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK530

Quant Time: Aug 09 04:15:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 09 04:14:12 2022
Response via : Initial Calibration

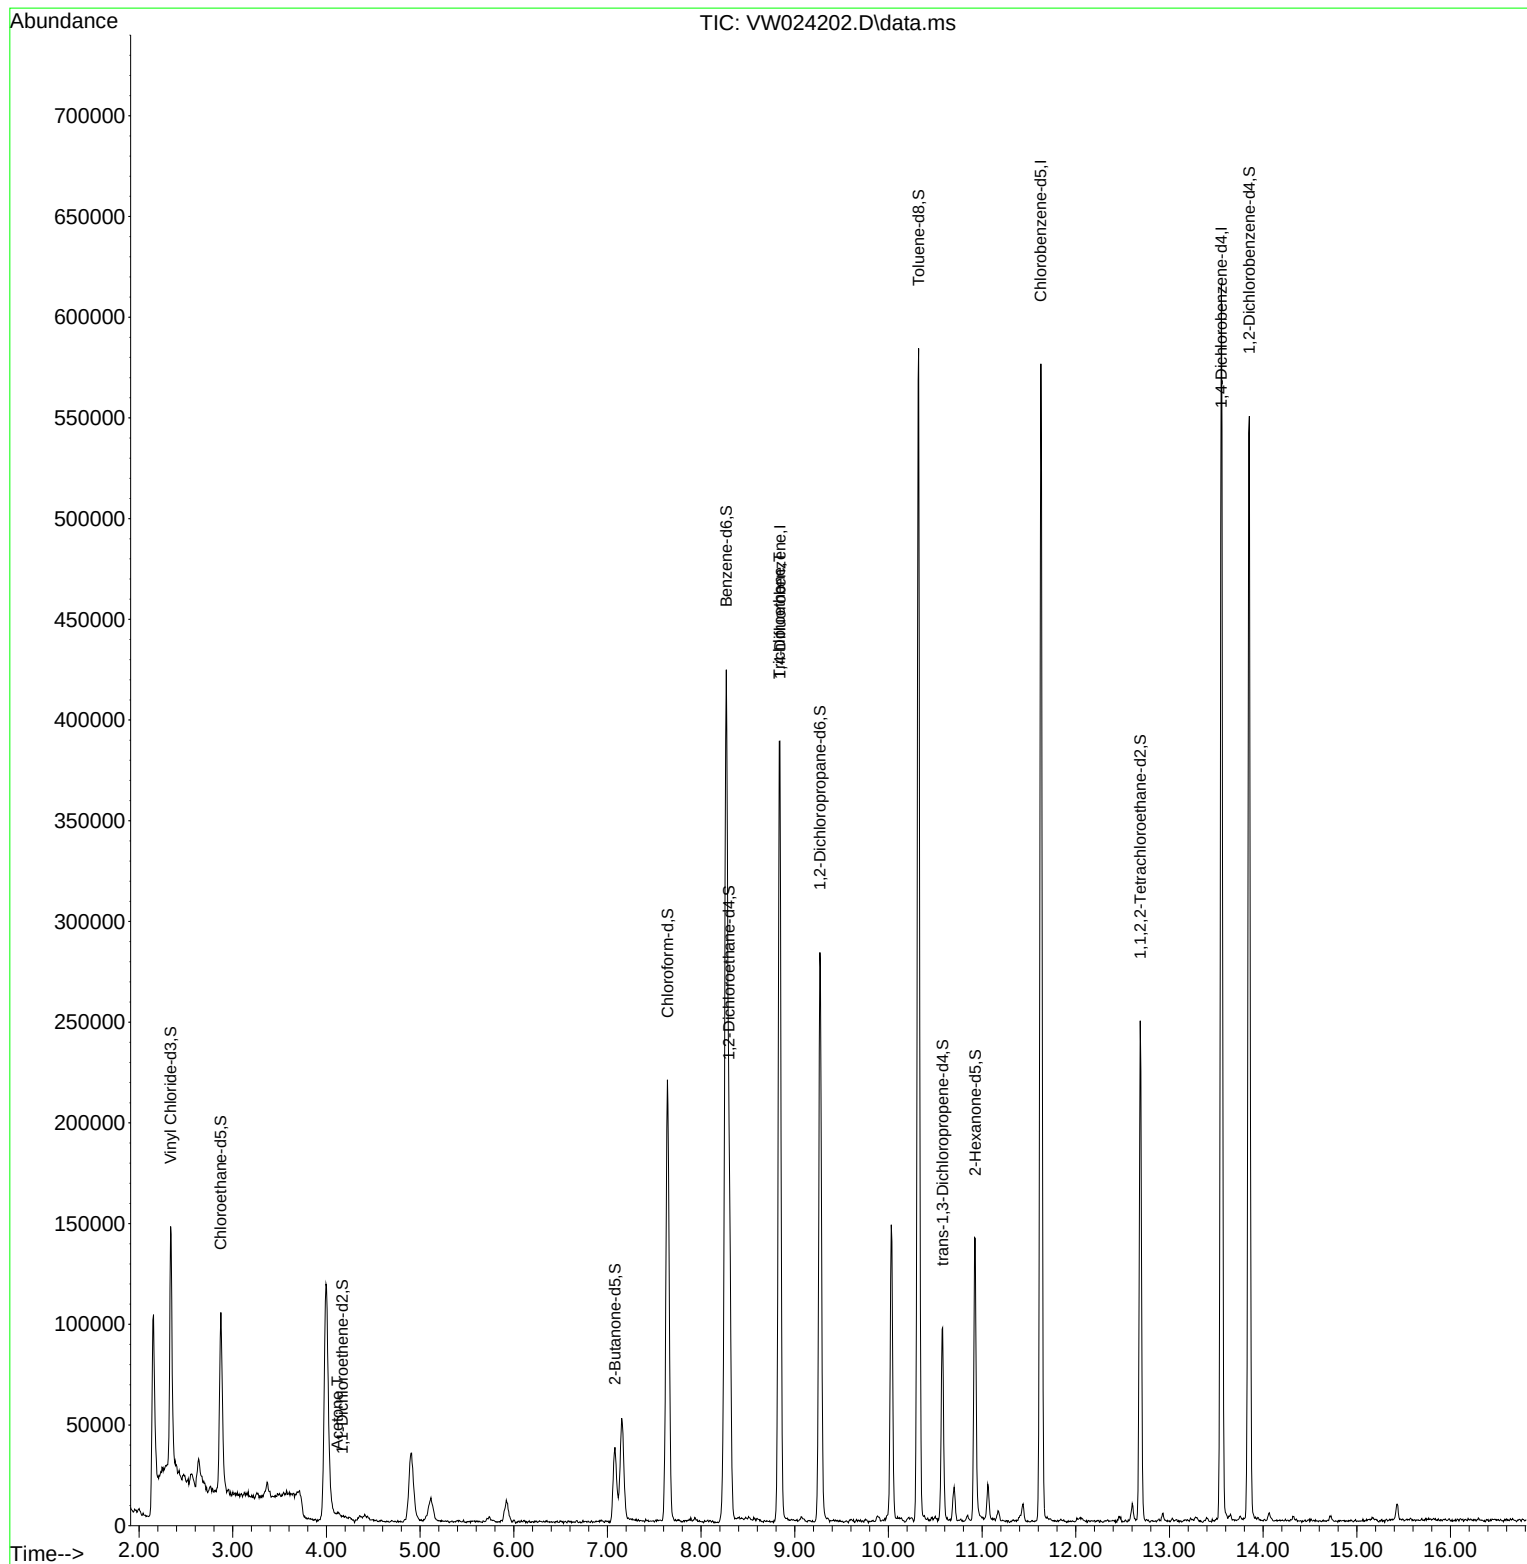

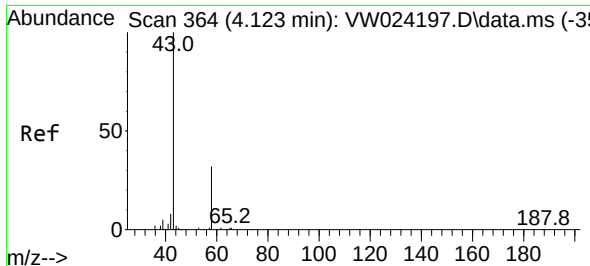

#13

Acetone

Concen: 4.357 ug/L

RT: 4.117 min Scan# 3

Delta R.T. -0.006 min

Lab File: VW024202.D

Acq: 08 Aug 2022 17:36

Instrument :

MSVOA_W

ClientSampleId :





VIBLK530

Tgt Ion: 43 Resp: 4082

Ion Ratio Lower Upper

43 100

58 12.4 0.0 31.8

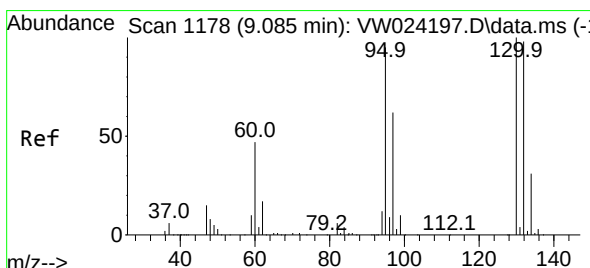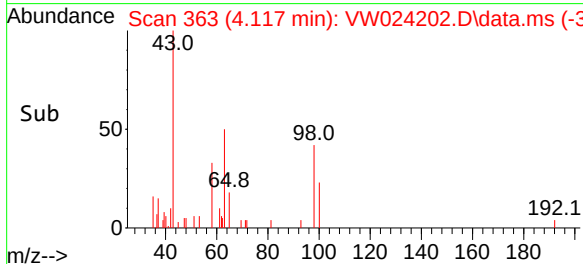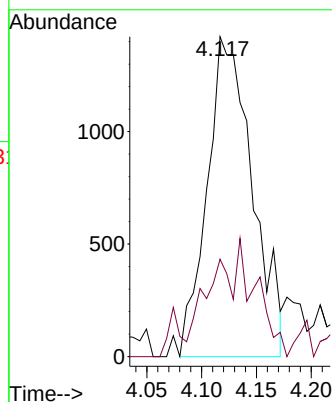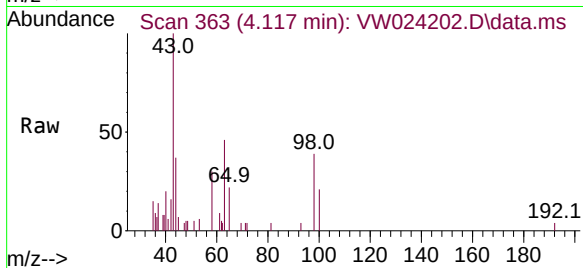

#34

Trichloroethene

Concen: 2.066 ug/L

RT: 8.835 min Scan# 1137

Delta R.T. -0.250 min

Lab File: VW024202.D

Acq: 08 Aug 2022 17:36

Tgt Ion: 95 Resp: 10238

Ion Ratio Lower Upper

95 100

97 0.0 41.6 77.2#

132 0.0 67.0 124.4#

130 0.0 73.1 135.8#

