

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080822\
 Data File : VW024203.D
 Acq On : 08 Aug 2022 18:01
 Operator : SY/VA
 Sample : N4008-03
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Aug 09 04:15:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 09 04:14:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	336851	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	334718	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	160794	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	131423	18.665	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.680%
7) Chloroethane-d5	2.873	69	93238	21.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.040%
11) 1,1-Dichloroethene-d2	4.001	63	110341	13.751	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.000%
21) 2-Butanone-d5	7.074	46	68228	52.085	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.160%
24) Chloroform-d	7.647	84	214433	21.039	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.160%
26) 1,2-Dichloroethane-d4	8.299	65	126505	22.356	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.440%
32) Benzene-d6	8.269	84	411741	20.858	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.440%
36) 1,2-Dichloropropane-d6	9.274	67	127477	21.872	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.480%
41) Toluene-d8	10.323	98	375836	20.369	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.480%
43) trans-1,3-Dichloroprop...	10.579	79	49478	19.381	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.520%
47) 2-Hexanone-d5	10.920	63	55433	51.491	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.980%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	127941	22.625	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	144234	24.513	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.040%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.995	85	2747	0.927	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080822\
Data File : VW024203.D
Acq On : 08 Aug 2022 18:01
Operator : SY/VA
Sample : N4008-03
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Aug 09 04:15:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 09 04:14:12 2022
Response via : Initial Calibration

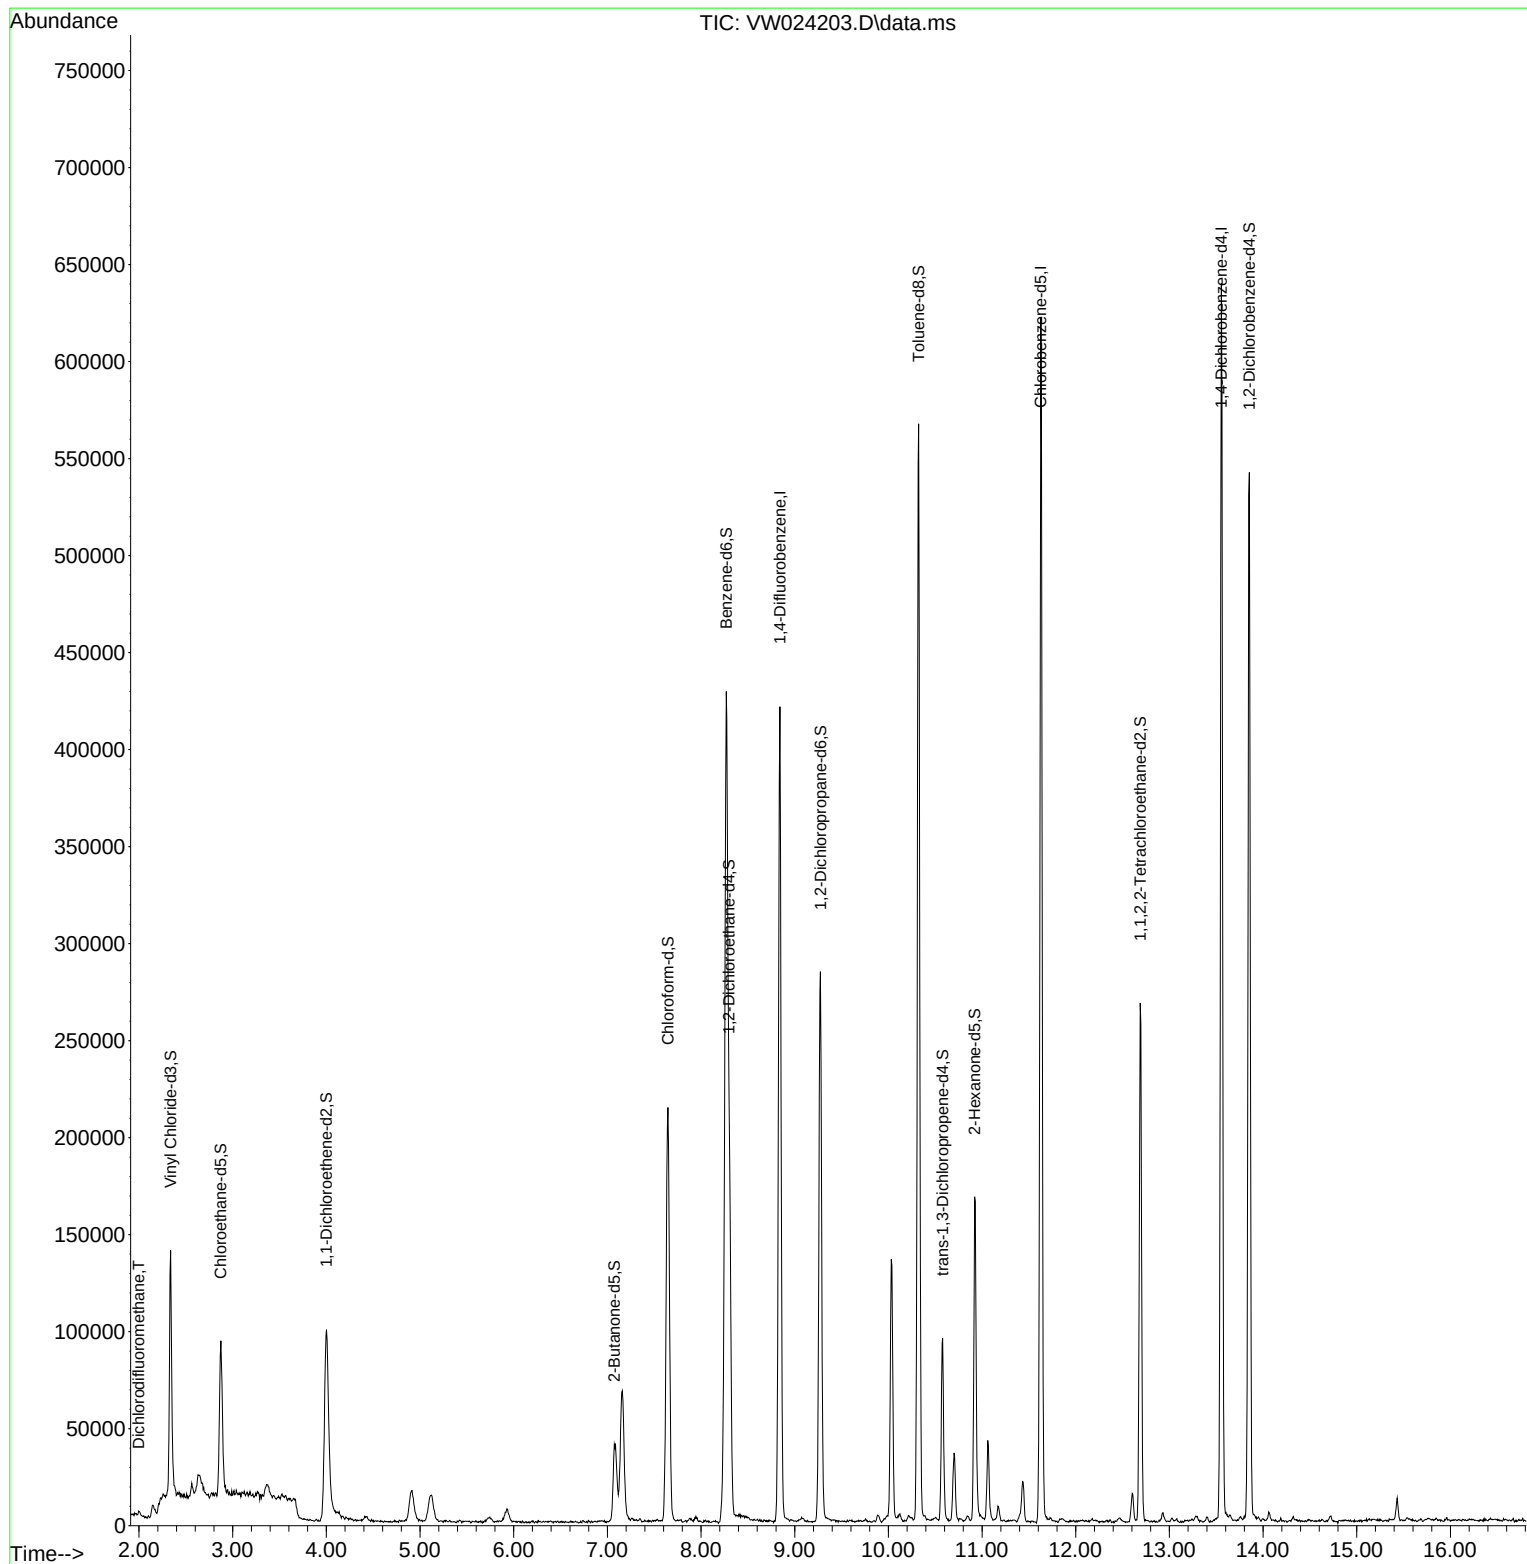

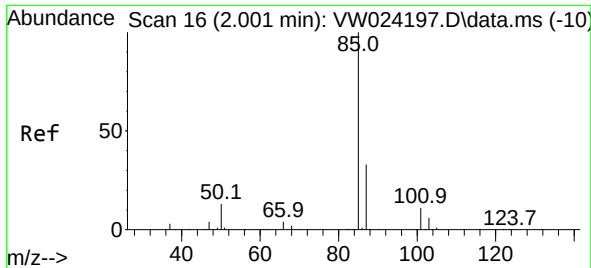

#2
 Dichlorodifluoromethane
 Concen: 0.927 ug/L
 RT: 1.995 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: VW024203.D
 Acq: 08 Aug 2022 18:01

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 85 Resp: 2747
 Ion Ratio Lower Upper
 85 100
 87 29.3 24.5 36.7

