




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080822\
 Data File : VW024200.D
 Acq On : 08 Aug 2022 11:44
 Operator : SY/VA
 Sample : N4030-04
 Misc : 4.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0QB4

Manual IntegrationsAPPROVED

Quant Time: Aug 09 04:15:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 09 04:14:12 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/09/2022
 Supervised By :Semsettin Yesilyurt 08/09/2022

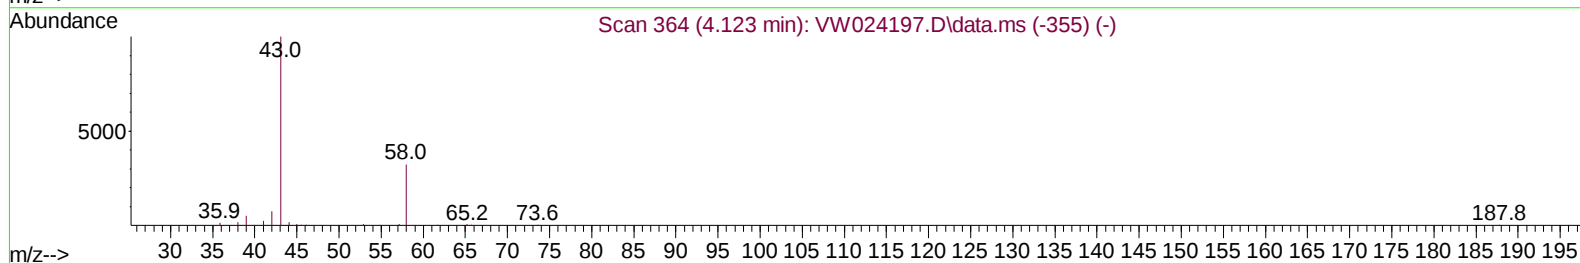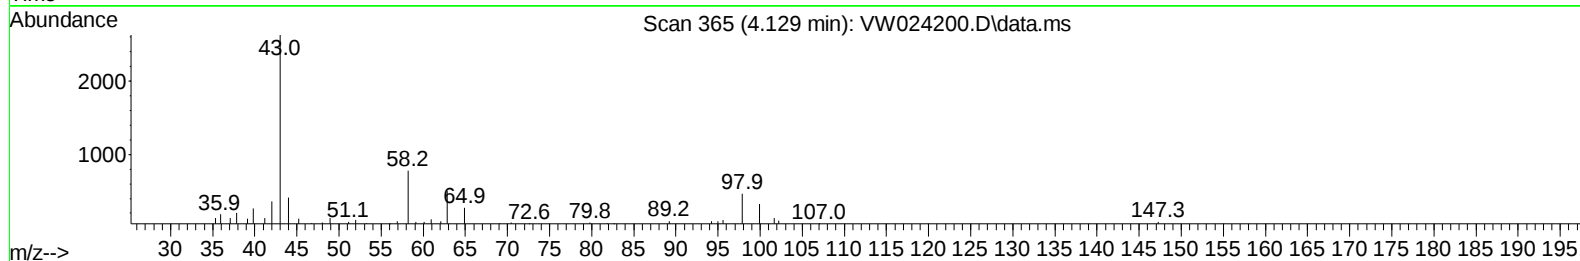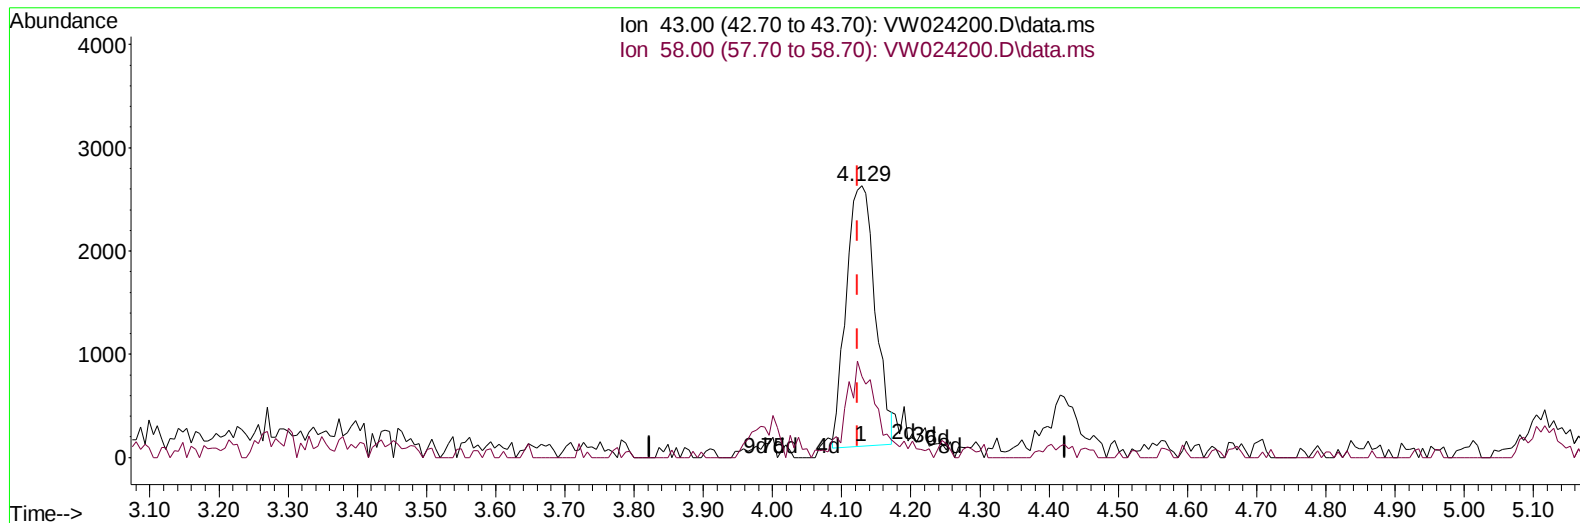

TIC: VW024200.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 6.11 ug/L

response 7323

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	16.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080822\
 Data File : VW024200.D
 Acq On : 08 Aug 2022 11:44
 Operator : SY/VA
 Sample : N4030-04
 Misc : 4.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0QB4

Manual IntegrationsAPPROVED

Quant Time: Aug 09 04:15:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 09 04:14:12 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/09/2022
 Supervised By :Semsettin Yesilyurt 08/09/2022

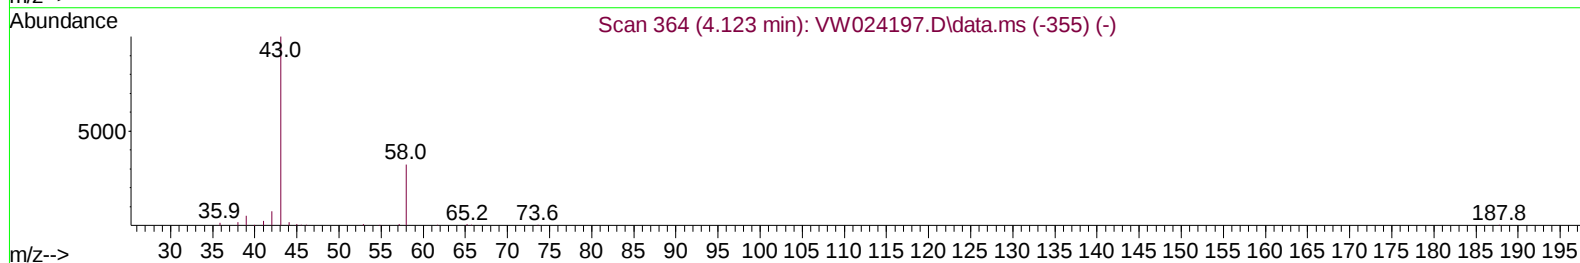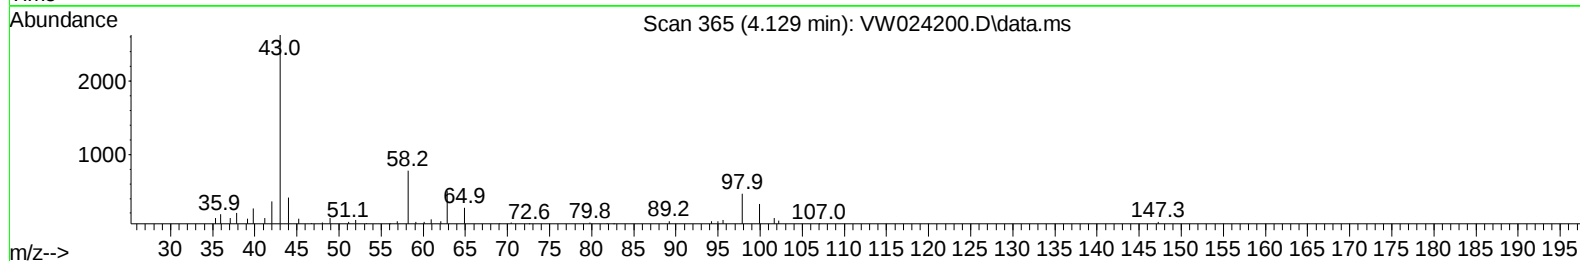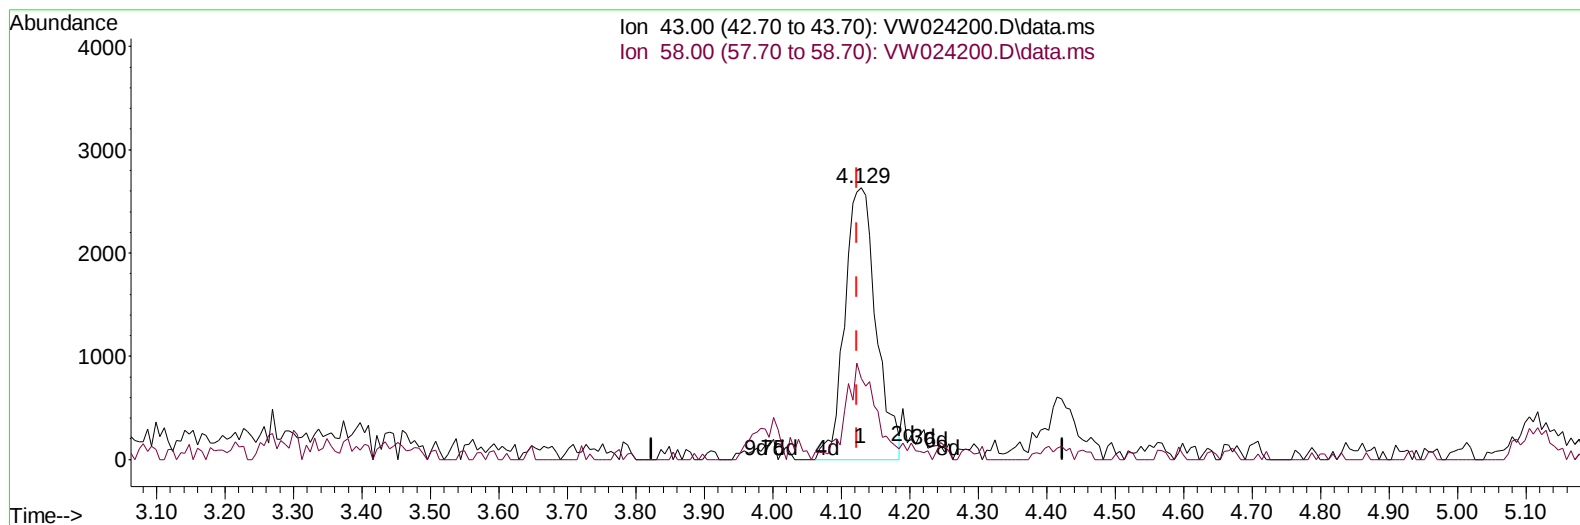

TIC: VW024200.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 6.96 ug/L m

response 8345

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	14.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080822\
 Data File : VW024200.D
 Acq On : 08 Aug 2022 11:44
 Operator : SY/VA
 Sample : N4030-04
 Misc : 4.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0QB4

Manual IntegrationsAPPROVED

Quant Time: Aug 09 04:15:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 09 04:14:12 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/09/2022
 Supervised By :Semsettin Yesilyurt 08/09/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.836	114		418781	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		404487	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		202748	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		230463	26.328	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	105.320%	
7) Chloroethane-d5	2.873	69		136206	24.978	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	99.920%	
11) 1,1-Dichloroethene-d2	4.001	63		170857	17.127	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	68.520%	
21) 2-Butanone-d5	7.074	46		80973	49.721	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	99.440%	
24) Chloroform-d	7.641	84		296964	23.436	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	93.760%	
26) 1,2-Dichloroethane-d4	8.305	65		165545	23.532	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	94.120%	
32) Benzene-d6	8.269	84		584736	24.512	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	98.040%	
36) 1,2-Dichloropropane-d6	9.268	67		172364	24.472	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	97.880%	
41) Toluene-d8	10.323	98		547374	24.549	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	98.200%	
43) trans-1,3-Dichloroprop...	10.573	79		76714	24.867	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	99.480%	
47) 2-Hexanone-d5	10.921	63		67676	52.021	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	104.040%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		152521	22.320	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	89.280%	
66) 1,2-Dichlorobenzene-d4	13.853	152		196077	26.428	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	105.720%	
Target Compounds							
13) Acetone	4.129	43		8345m	6.960	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080822\
Data File : VW024200.D
Acq On : 08 Aug 2022 11:44
Operator : SY/VA
Sample : N4030-04
Misc : 4.44g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0QB4

Manual IntegrationsAPPROVED

Quant Time: Aug 09 04:15:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 09 04:14:12 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/09/2022
Supervised By :Semsettin Yesilyurt 08/09/2022

