




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080824\
 Data File : VW029862.D
 Acq On : 08 Aug 2024 15:14
 Operator : SY/MD
 Sample : P3481-12
 Misc : 4.52g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AE6

Manual IntegrationsAPPROVED

Quant Time: Aug 09 00:51:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 09 00:48:13 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/09/2024
 Supervised By :Mahesh Dadoda 08/13/2024

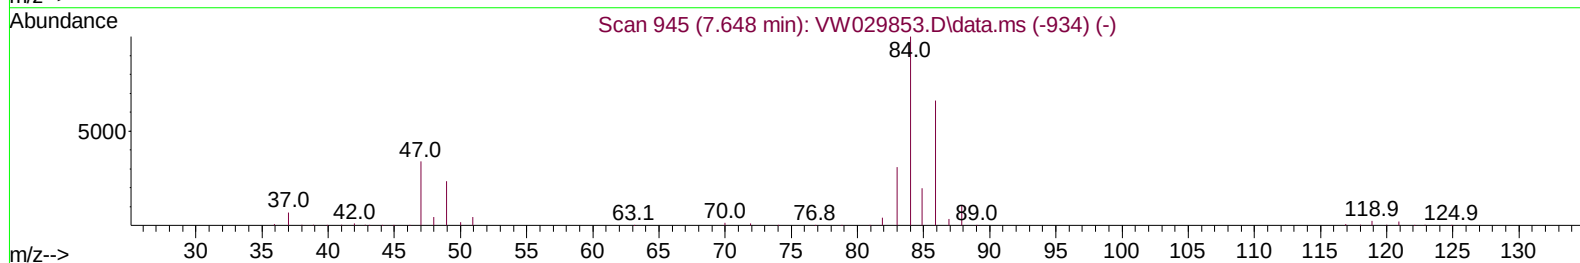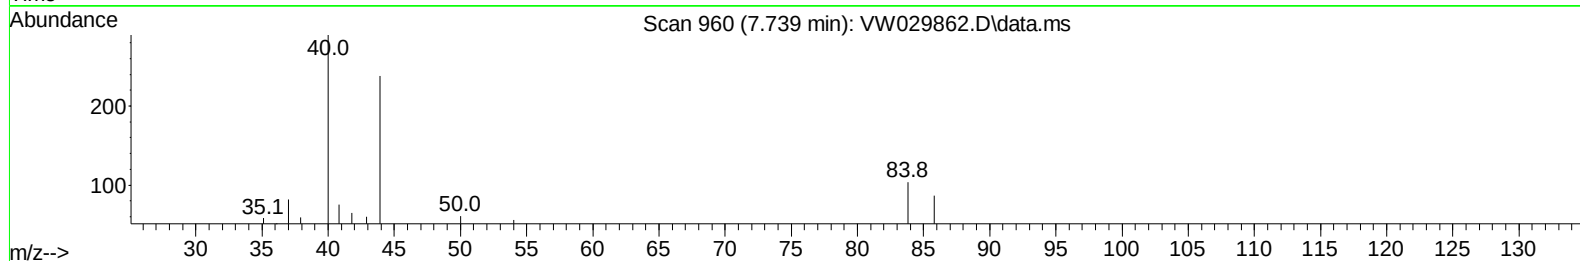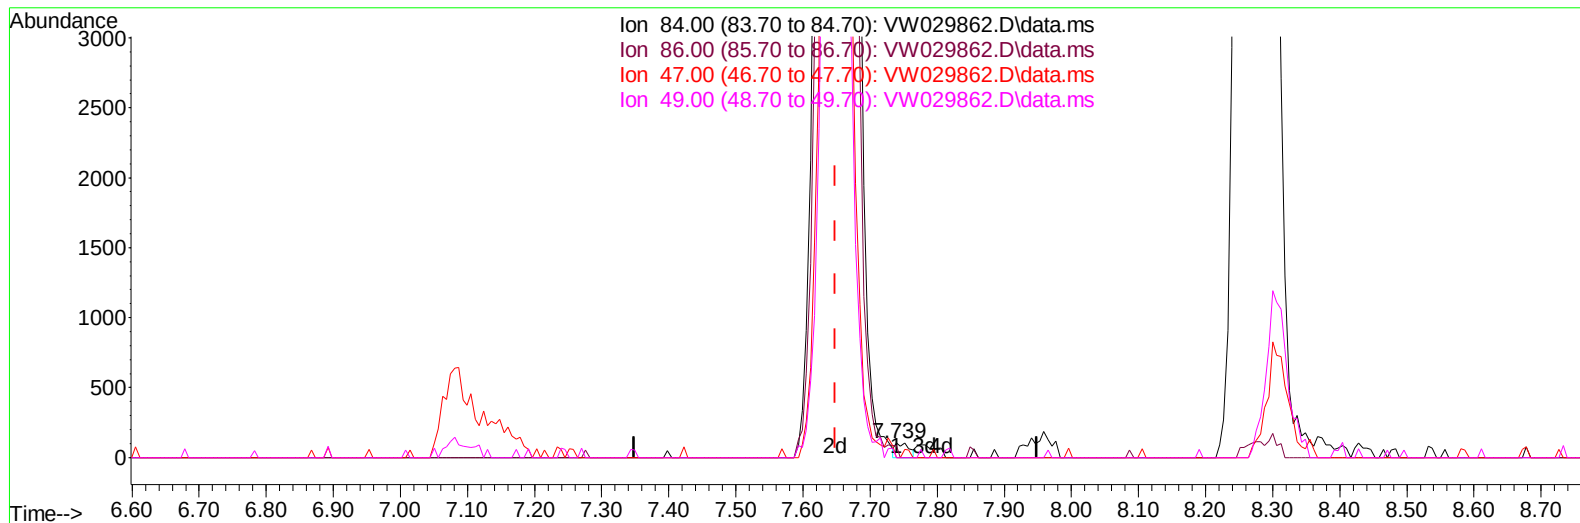

TIC: VW029862.D\data.ms

(24) Chloroform-d (S)

7.739min (+ 0.091) 0.02 ug/L

response 149

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.90	65.10
47.00	57.60	54.36
49.00	31.80	32.21




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080824\
Data File : VW029862.D
Acq On : 08 Aug 2024 15:14
Operator : SY/MD
Sample : P3481-12
Misc : 4.52g/10mL/MSVOA_W/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AE6

Manual IntegrationsAPPROVED

Quant Time: Aug 09 00:51:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 00:48:13 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/09/2024
Supervised By :Mahesh Dadoda 08/13/2024

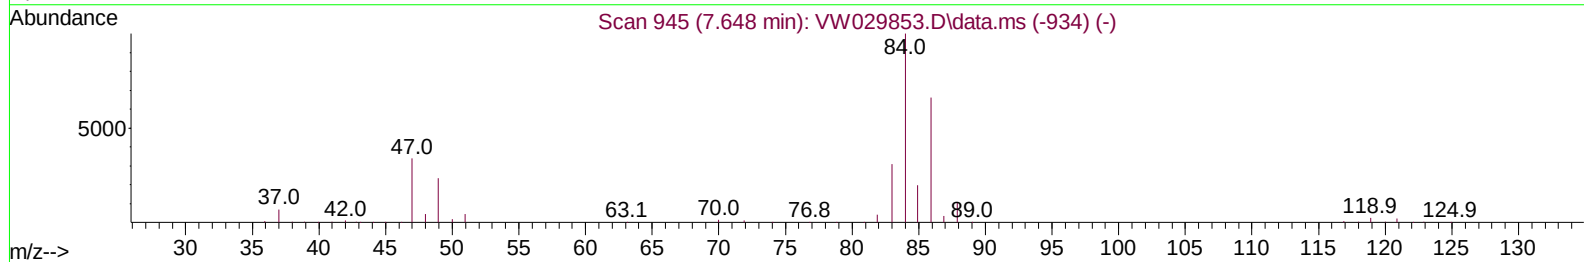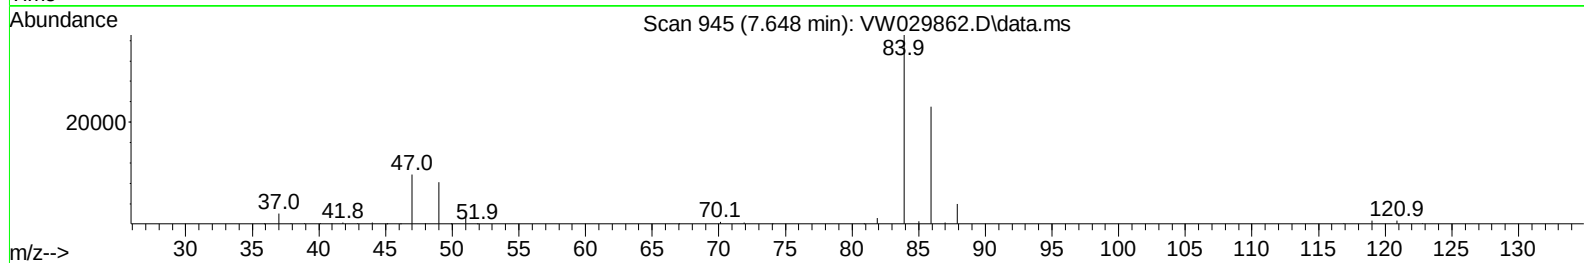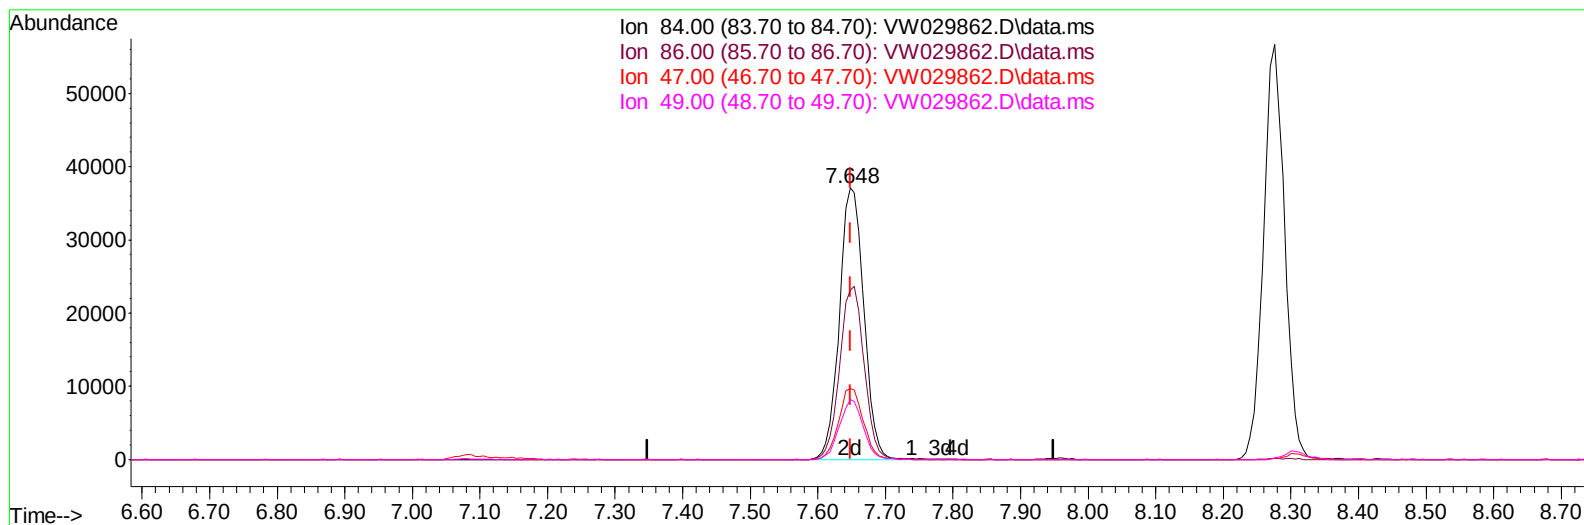

TIC: VW029862.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.001) 13.95 ug/L m

response 93000

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.90	0.10#
47.00	57.60	0.09#
49.00	31.80	0.05#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080824\
 Data File : VW029862.D
 Acq On : 08 Aug 2024 15:14
 Operator : SY/MD
 Sample : P3481-12
 Misc : 4.52g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AE6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/09/2024
 Supervised By :Mahesh Dadoda 08/13/2024

Quant Time: Aug 09 00:51:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 09 00:48:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	257592	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	185137	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	53022	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	17762	4.857	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	19.440%#	
7) Chloroethane-d5	2.893	69	21801	8.350	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	33.400%	
11) 1,1-Dichloroethene-d2	4.021	65	8634	5.172	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	20.680%#	
21) 2-Butanone-d5	7.081	46	61299	61.157	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	122.320%	
24) Chloroform-d	7.648	84	93000m	13.947	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	55.800%	
26) 1,2-Dichloroethane-d4	8.306	65	58618	15.434	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	61.720%#	
32) Benzene-d6	8.276	84	123542	12.350	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	49.400%	
36) 1,2-Dichloropropane-d6	9.276	67	57215	17.913	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	71.640%	
41) Toluene-d8	10.324	98	81425	9.154	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	36.600%	
43) trans-1,3-Dichloroprop...	10.574	79	17435	13.490	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	53.960%	
47) 2-Hexanone-d5	10.922	63	37890	71.941	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	143.880%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	62610	26.399	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	105.600%	
66) 1,2-Dichlorobenzene-d4	13.854	152	27269	16.563	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	66.240%#	
Target Compounds						
						Qvalue
13) Acetone	4.130	43	48609	39.024	ug/L	100
14) Carbon disulfide	4.392	76	4710	0.402	ug/L	99
22) 2-Butanone	7.178	43	18159	11.378	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080824\
Data File : VW029862.D
Acq On : 08 Aug 2024 15:14
Operator : SY/MD
Sample : P3481-12
Misc : 4.52g/10mL/MSVOA_W/SoIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AE6

Manual IntegrationsAPPROVED

Quant Time: Aug 09 00:51:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 00:48:13 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/09/2024
Supervised By :Mahesh Dadoda 08/13/2024

