




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029871.D
Acq On : 09 Aug 2024 13:31
Operator : SY/MD
Sample : P3481-05
Misc : 5.96g/10mL/MSVOA_W/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AD7

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:15:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 23:13:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/12/2024
Supervised By :Mahesh Dadoda 08/13/2024

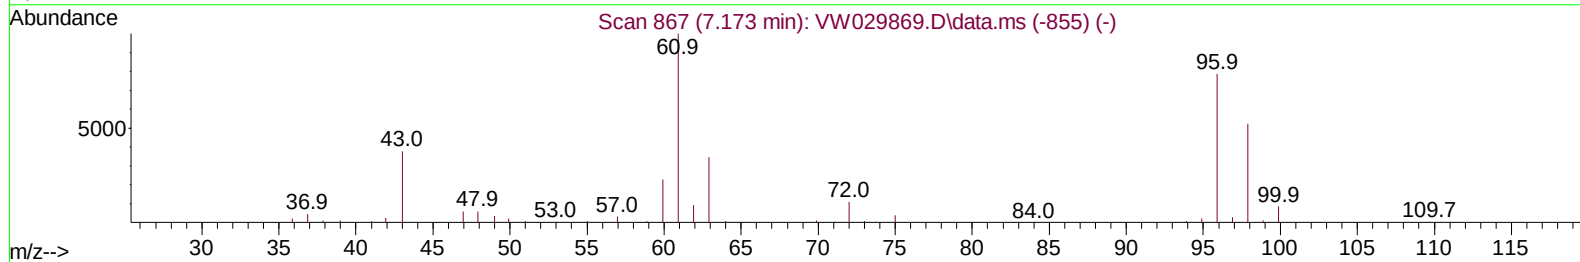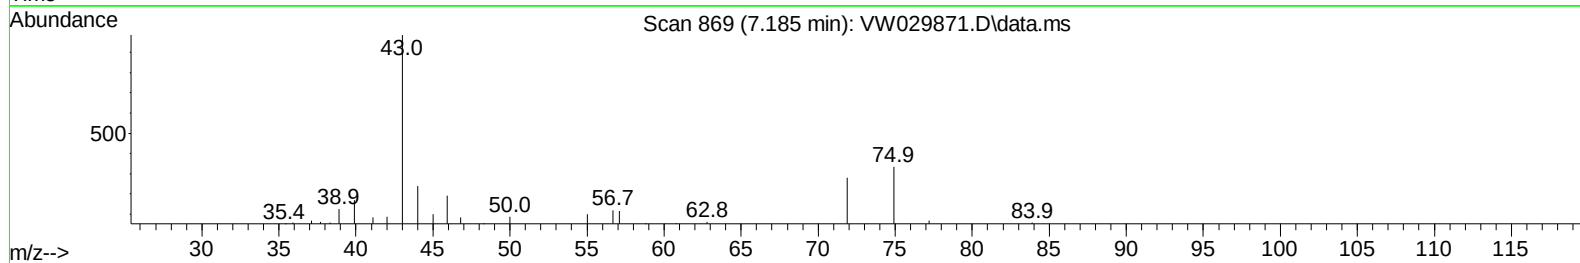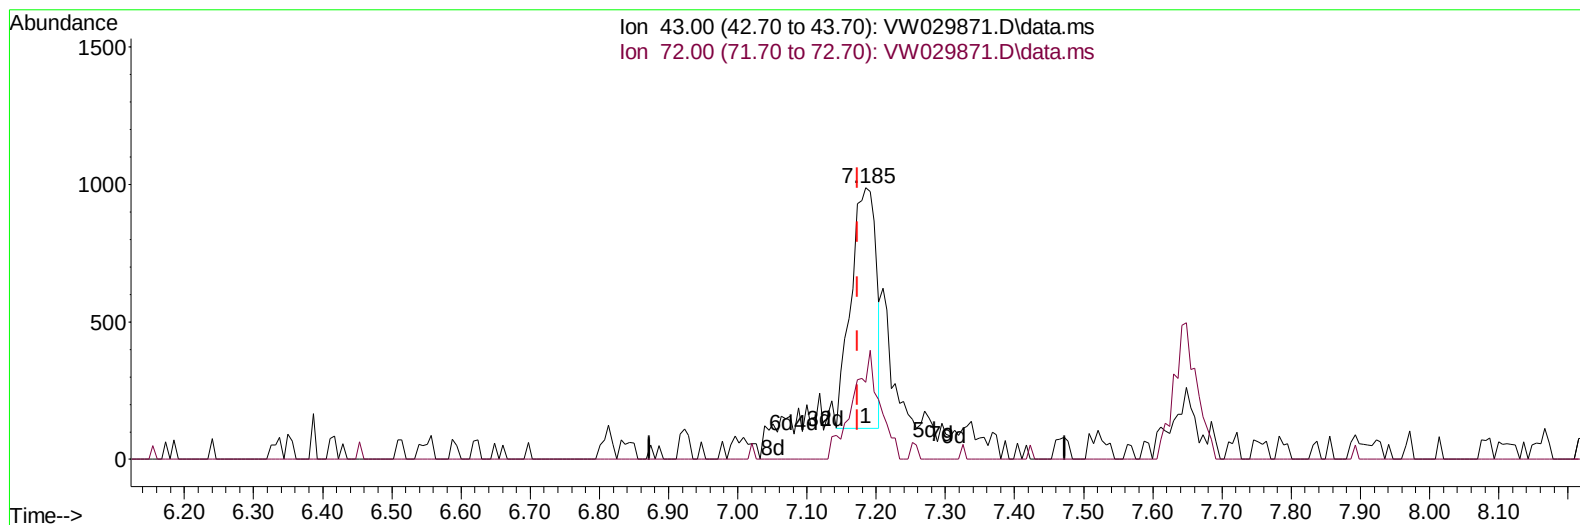

TIC: VW029871.D\data.ms

(22) 2-Butanone (T)

7.185min (+ 0.012) 2.31 ug/L

response 2201

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	23.40	21.76
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029871.D
Acq On : 09 Aug 2024 13:31
Operator : SY/MD
Sample : P3481-05
Misc : 5.96g/10mL/MSVOA_W/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AD7

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:15:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 23:13:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/12/2024
Supervised By :Mahesh Dadoda 08/13/2024

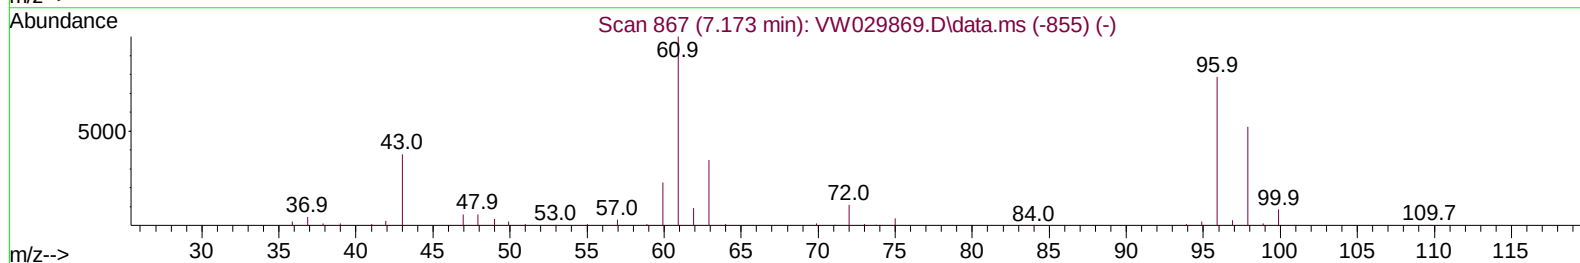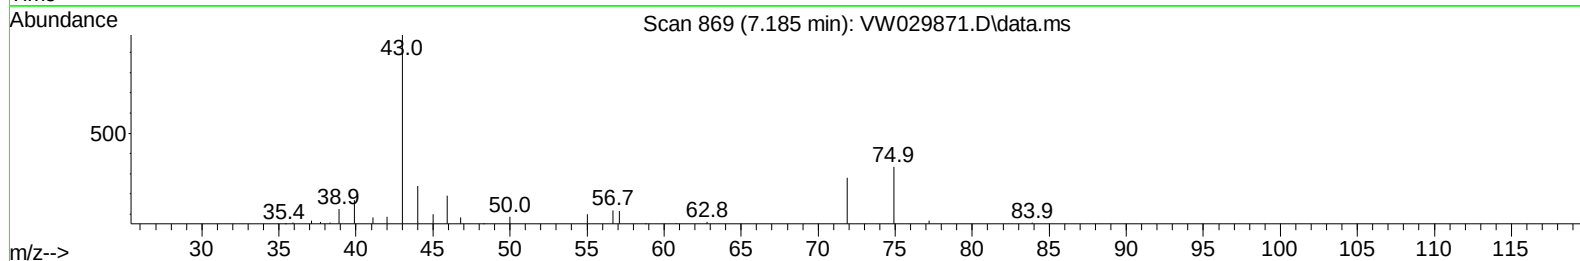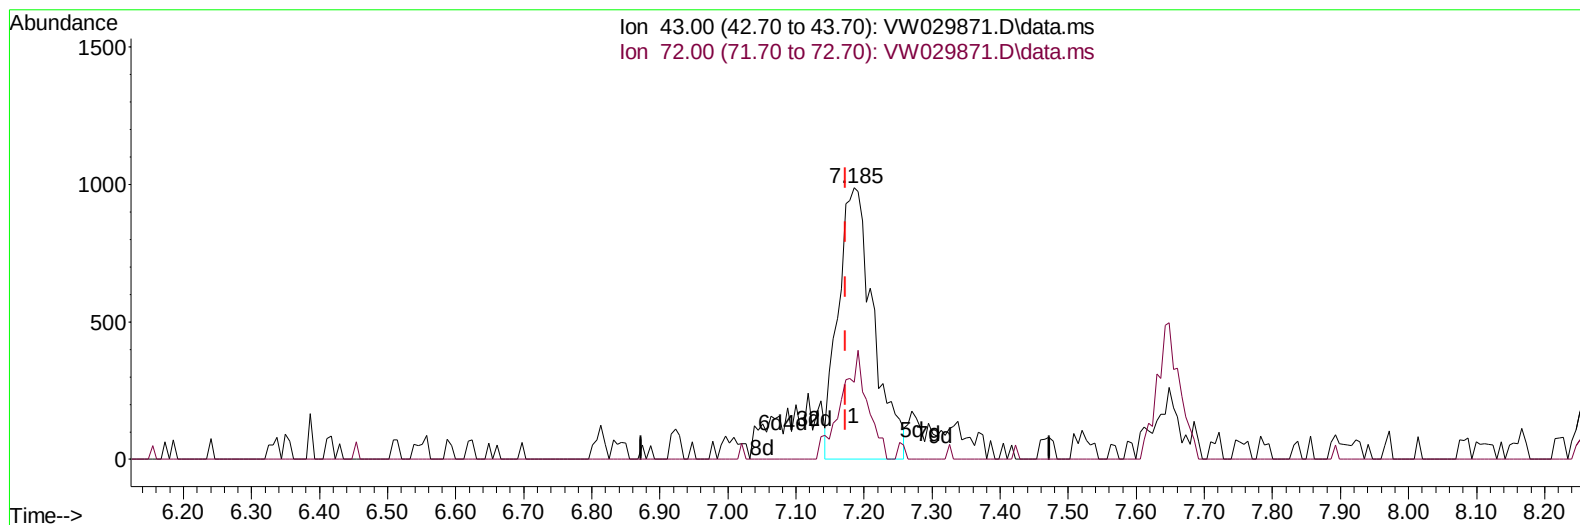

TIC: VW029871.D\data.ms

(22) 2-Butanone (T)

7.185min (+ 0.012) 3.71 ug/L m

response 3545

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	23.40	13.51
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
 Data File : VW029871.D
 Acq On : 09 Aug 2024 13:31
 Operator : SY/MD
 Sample : P3481-05
 Misc : 5.96g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AD7

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:15:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 09 23:13:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/12/2024
 Supervised By :Mahesh Dadoda 08/13/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	154052	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	117492	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	29595	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	84732	38.743	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	= 154.960%#		
7) Chloroethane-d5	2.899	69	66638	42.678	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	= 170.720%#		
11) 1,1-Dichloroethene-d2	4.015	65	33008	33.063	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	= 132.240%#		
21) 2-Butanone-d5	7.081	46	36039	60.122	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	= 120.240%		
24) Chloroform-d	7.648	84	143309	35.936	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	= 143.760%		
26) 1,2-Dichloroethane-d4	8.301	65	83342	36.691	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	= 146.760%#		
32) Benzene-d6	8.270	84	268869	42.353	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	= 169.400%#		
36) 1,2-Dichloropropane-d6	9.270	67	83595	41.240	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	= 164.960%#		
41) Toluene-d8	10.319	98	216954	38.435	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	= 153.760%#		
43) trans-1,3-Dichloroprop...	10.575	79	29787	36.315	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	= 145.280%#		
47) 2-Hexanone-d5	10.922	63	25061	74.978	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	= 149.960%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	62474	41.508	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	= 166.040%#		
66) 1,2-Dichlorobenzene-d4	13.849	152	37358	40.653	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	= 162.600%#		
Target Compounds						
						Qvalue
13) Acetone	4.131	43	16493	22.140	ug/L	94
14) Carbon disulfide	4.393	76	8995	1.284	ug/L	99
22) 2-Butanone	7.185	43	3545m	3.714	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029871.D
Acq On : 09 Aug 2024 13:31
Operator : SY/MD
Sample : P3481-05
Misc : 5.96g/10mL/MSVOA_W/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AD7

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/12/2024
Supervised By :Mahesh Dadoda 08/13/2024

Quant Time: Aug 09 23:15:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 23:13:22 2024
Response via : Initial Calibration

