




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029877.D
Acq On : 09 Aug 2024 16:19
Operator : SY/MD
Sample : P3481-20
Misc : 5.56g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AF6

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:16:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 23:13:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/12/2024
Supervised By :Mahesh Dadoda 08/13/2024

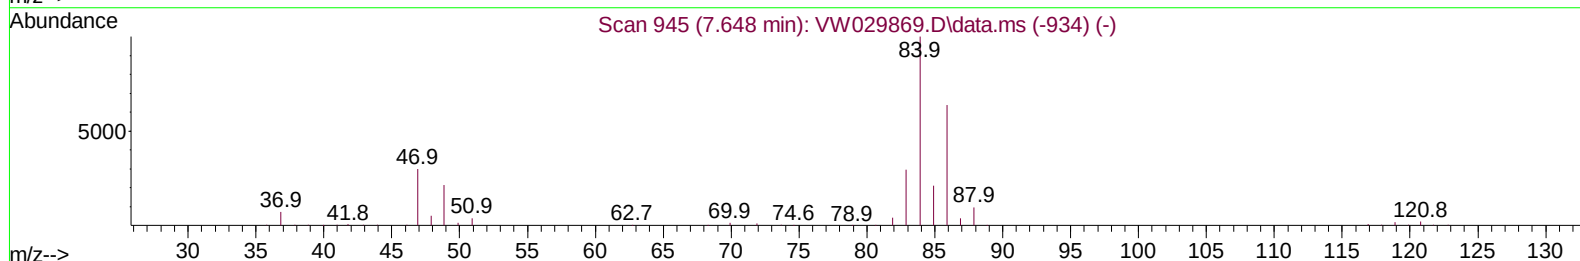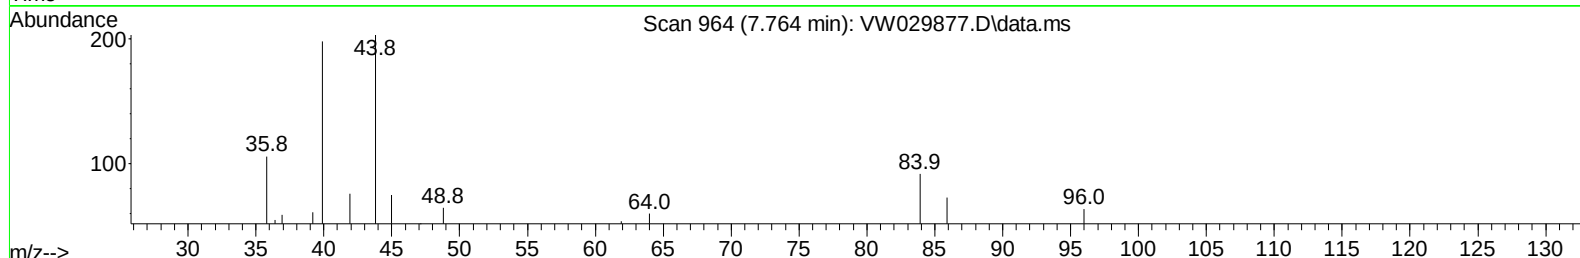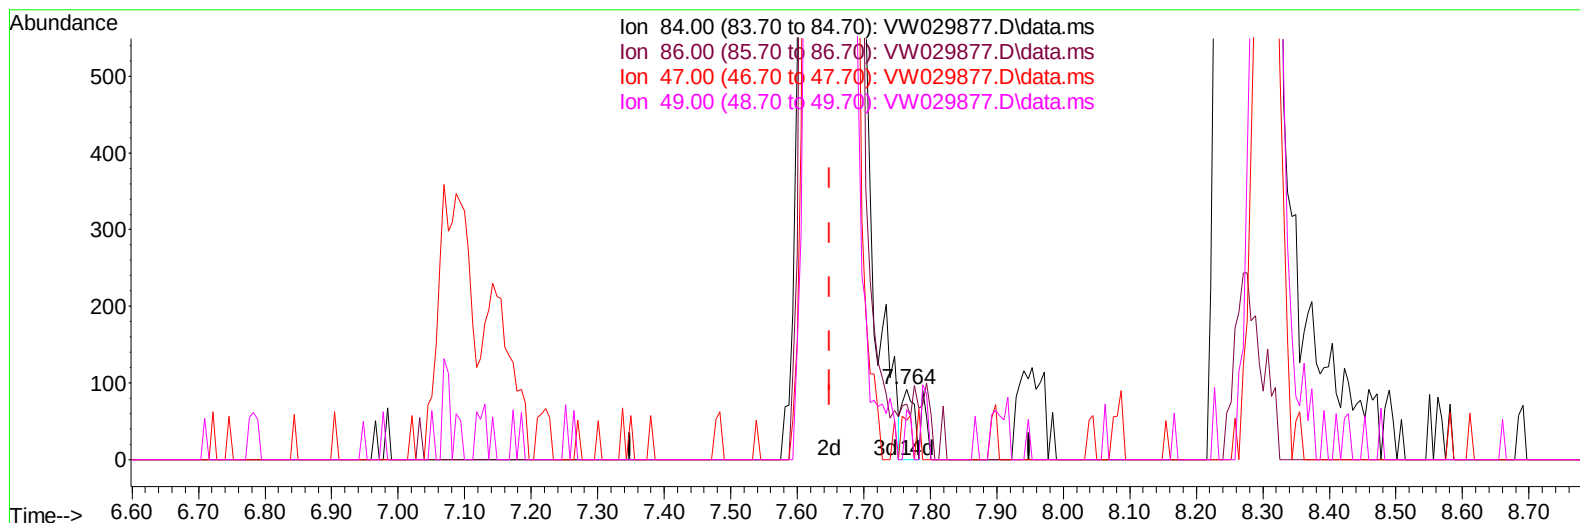

TIC: VW029877.D\data.ms

(24) Chloroform-d (S)

7.764min (+ 0.116) 0.02 ug/L

response 115

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.90	63.48
47.00	57.60	53.04
49.00	31.80	39.13




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029877.D
Acq On : 09 Aug 2024 16:19
Operator : SY/MD
Sample : P3481-20
Misc : 5.56g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AF6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/12/2024
Supervised By :Mahesh Dadoda 08/13/2024

Quant Time: Aug 09 23:16:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 23:13:22 2024
Response via : Initial Calibration

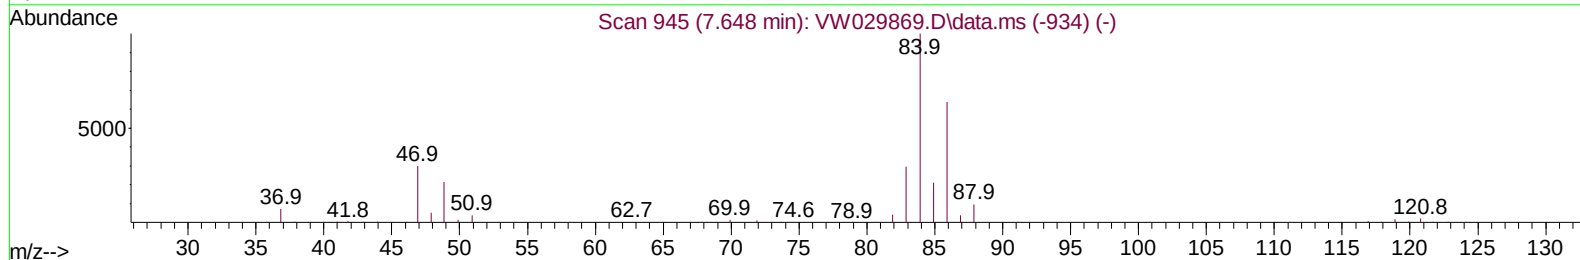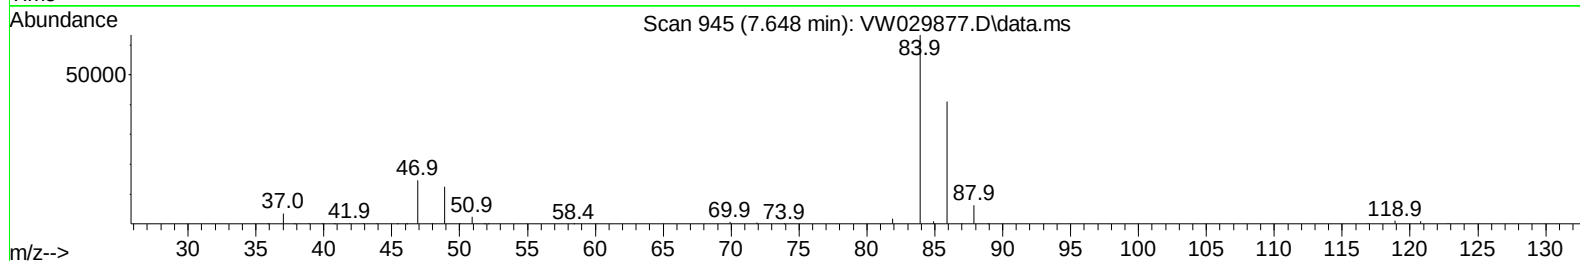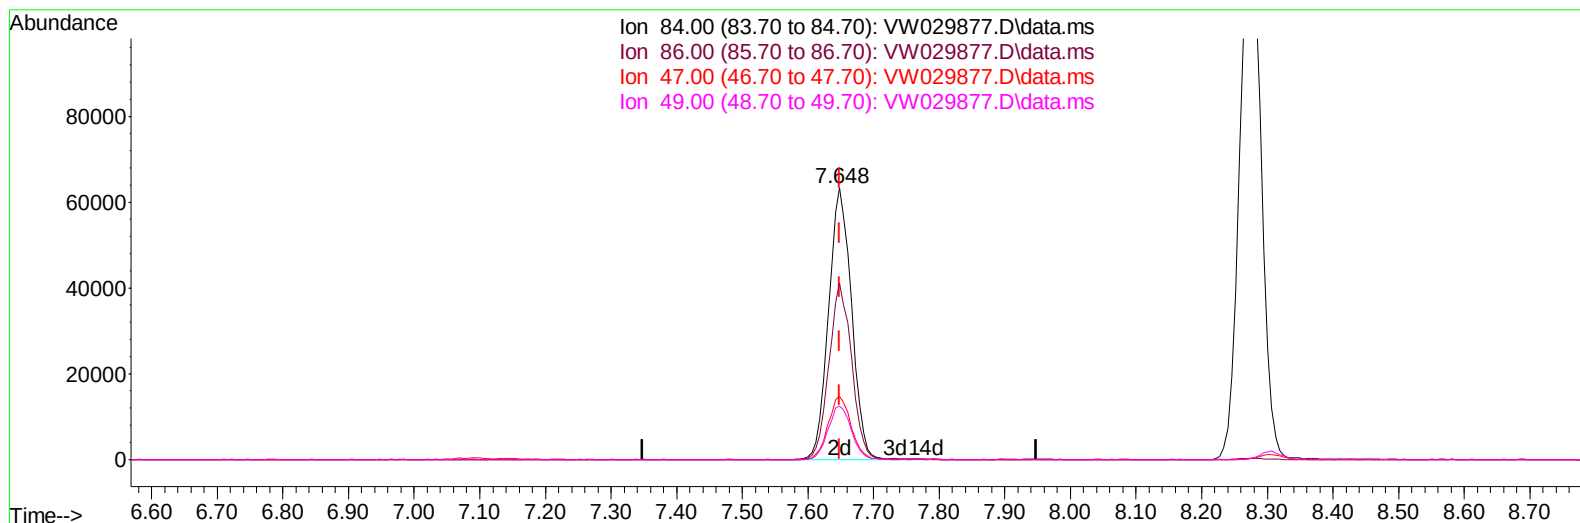

TIC: VW029877.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 22.27 ug/L m

response 153039

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.90	0.05#
47.00	57.60	0.04#
49.00	31.80	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
 Data File : VW029877.D
 Acq On : 09 Aug 2024 16:19
 Operator : SY/MD
 Sample : P3481-20
 Misc : 5.56g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AF6

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:16:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 09 23:13:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/12/2024
 Supervised By :Mahesh Dadoda 08/13/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	265519	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	186441	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	44314	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	87150	23.120	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	92.480%	
7) Chloroethane-d5	2.899	69	69929	25.985	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	103.920%	
11) 1,1-Dichloroethene-d2	4.021	65	34364	19.971	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	79.880%	
21) 2-Butanone-d5	7.081	46	39011	37.759	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	75.520%	
24) Chloroform-d	7.648	84	153039m	22.265	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	89.080%	
26) 1,2-Dichloroethane-d4	8.307	65	88260	22.544	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.160%	
32) Benzene-d6	8.276	84	285645	28.355	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	113.440%	
36) 1,2-Dichloropropane-d6	9.276	67	88710	27.579	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	110.320%	
41) Toluene-d8	10.325	98	227778	25.430	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	101.720%	
43) trans-1,3-Dichloroprop...	10.581	79	31110	23.902	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	95.600%	
47) 2-Hexanone-d5	10.922	63	26852	50.627	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.260%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	61828	25.887	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	103.560%	
66) 1,2-Dichlorobenzene-d4	13.848	152	32826	23.856	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	95.440%	
Target Compounds						
					Qvalue	
13) Acetone	4.137	43	32797	25.544	ug/L	97
22) 2-Butanone	7.179	43	12242	7.441	ug/L	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029877.D
Acq On : 09 Aug 2024 16:19
Operator : SY/MD
Sample : P3481-20
Misc : 5.56g/10mL/MSVOA_W/soil/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AF6

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:16:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 23:13:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/12/2024
Supervised By :Mahesh Dadoda 08/13/2024

