

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
 Data File : VW029873.D
 Acq On : 09 Aug 2024 14:19
 Operator : SY/MD
 Sample : P3481-16
 Misc : 5.65g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AF1

Quant Time: Aug 09 23:15:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 09 23:13:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	351908	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	305948	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	107609	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	86384	17.291	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.160%
7) Chloroethane-d5	2.893	69	71345	20.003	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.000%
11) 1,1-Dichloroethene-d2	4.021	65	34382	15.076	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.320%
21) 2-Butanone-d5	7.081	46	35117	25.646	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	51.300%
24) Chloroform-d	7.648	84	163863	17.988	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.960%
26) 1,2-Dichloroethane-d4	8.307	65	95713	18.446	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.800%
32) Benzene-d6	8.270	84	304542	18.423	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.680%
36) 1,2-Dichloropropane-d6	9.276	67	95788	18.147	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	72.600%
41) Toluene-d8	10.325	98	275616	18.751	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.000%
43) trans-1,3-Dichloroprop...	10.574	79	37553	17.582	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.320%
47) 2-Hexanone-d5	10.922	63	26531	30.483	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.960%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	71623	18.274	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.080%
66) 1,2-Dichlorobenzene-d4	13.848	152	65628	19.641	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.560%
Target Compounds					Qvalue	
13) Acetone	4.137	43	8047	4.729	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029873.D
Acq On : 09 Aug 2024 14:19
Operator : SY/MD
Sample : P3481-16
Misc : 5.65g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AF1

Quant Time: Aug 09 23:15:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 23:13:22 2024
Response via : Initial Calibration

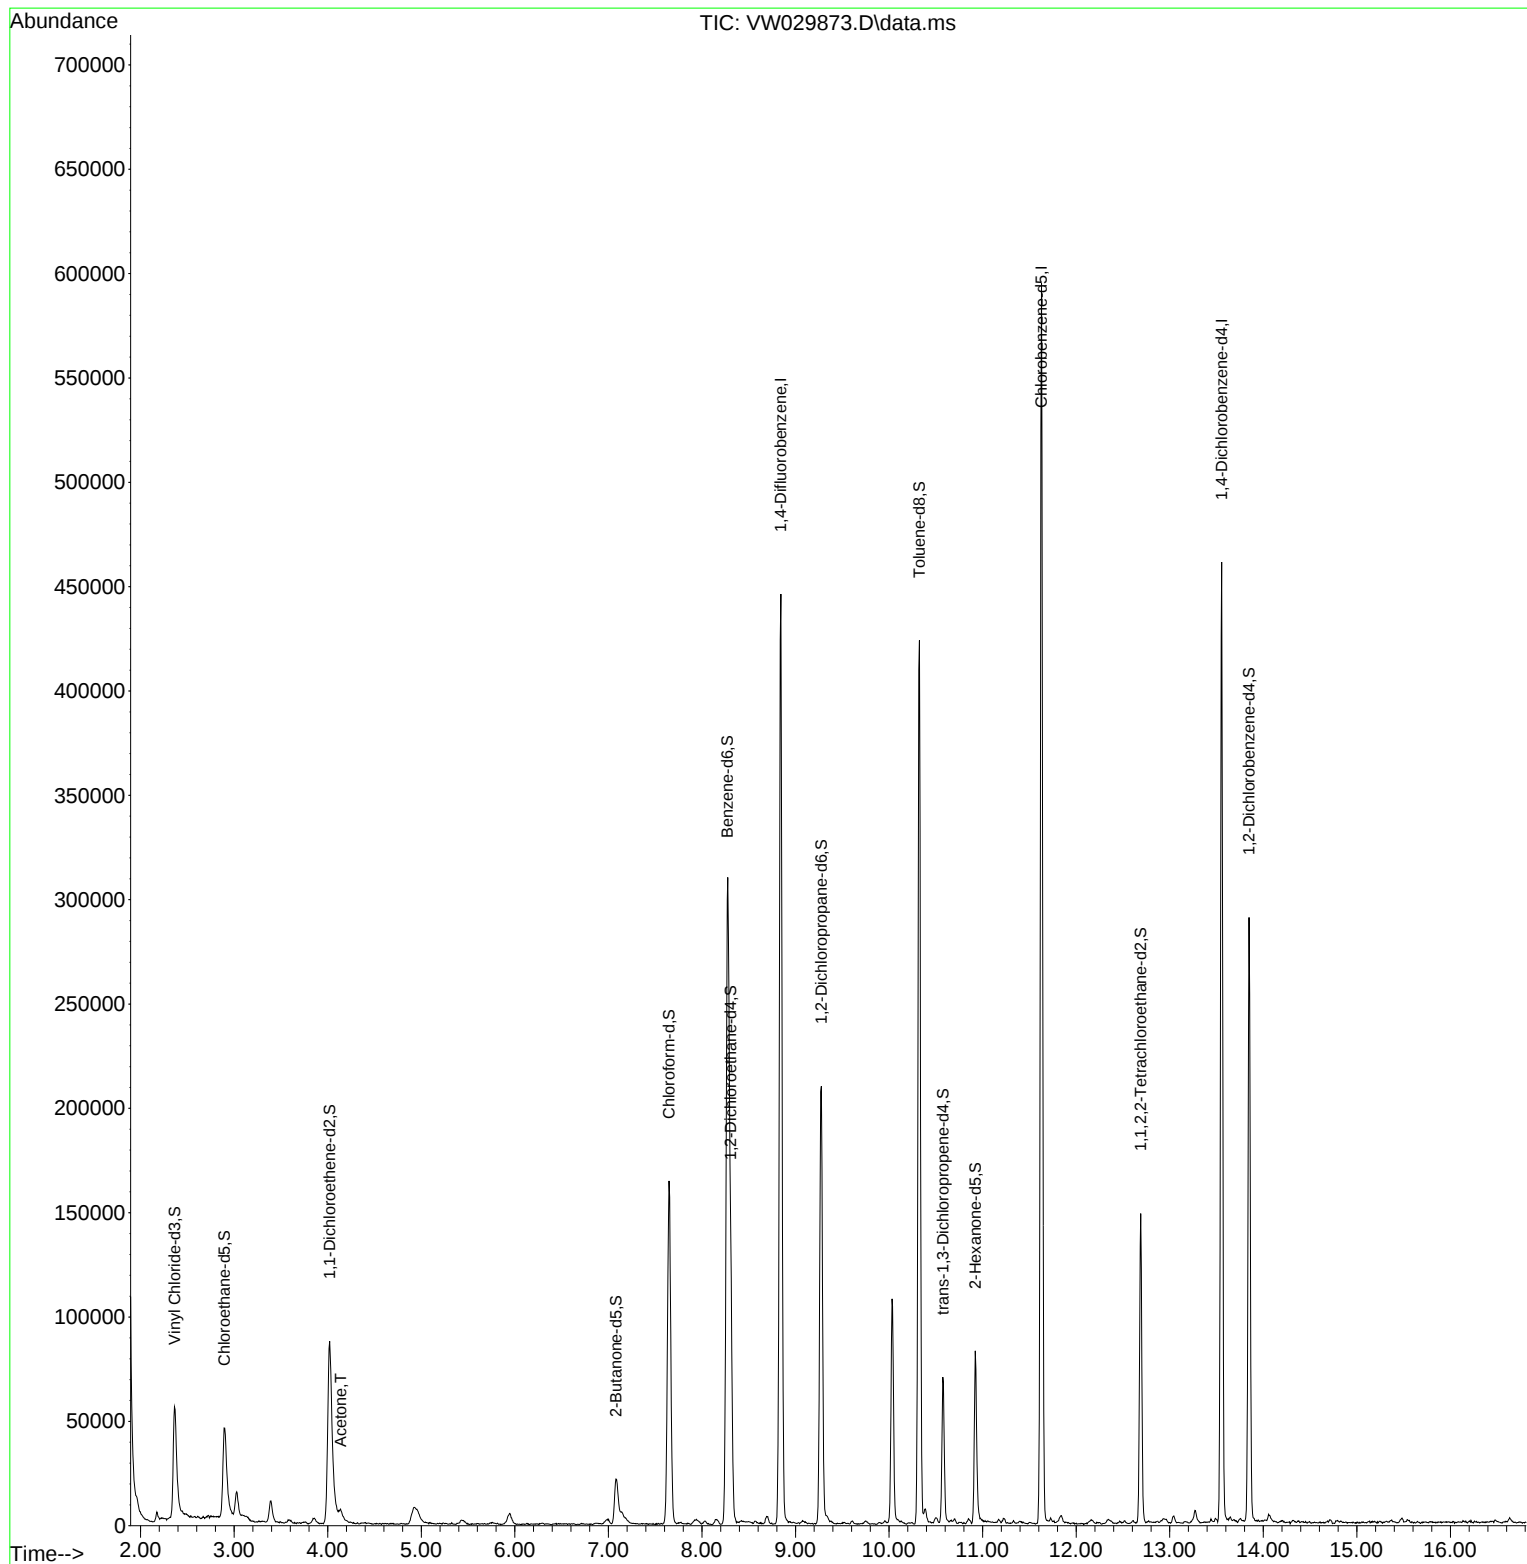

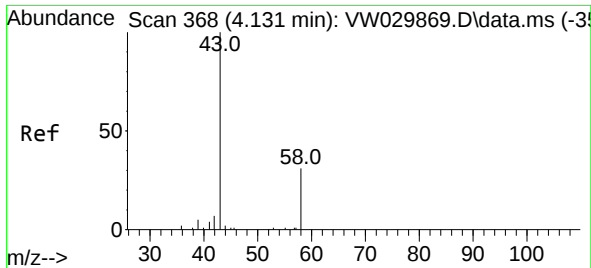

#13
 Acetone
 Concen: 4.729 ug/L
 RT: 4.137 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW029873.D
 Acq: 09 Aug 2024 14:19

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AF1

Tgt Ion: 43 Resp: 8047
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 57.6

