

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
 Data File : VW029881.D
 Acq On : 09 Aug 2024 17:55
 Operator : SY/MD
 Sample : P3481-08RE
 Misc : 6.21g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AE4RE

Quant Time: Aug 09 23:18:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 09 23:13:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	118510	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	99100	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	34170	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	40380	24.001	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.000%
7) Chloroethane-d5	2.893	69	31173	25.952	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.800%
11) 1,1-Dichloroethene-d2	4.021	65	15700	20.443	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.760%
21) 2-Butanone-d5	7.081	46	14066	30.503	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.000%
24) Chloroform-d	7.648	84	63751	20.781	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.120%
26) 1,2-Dichloroethane-d4	8.307	65	36102	20.661	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.640%
32) Benzene-d6	8.276	84	118643	22.157	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.640%
36) 1,2-Dichloropropane-d6	9.276	67	36205	21.176	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.720%
41) Toluene-d8	10.325	98	99831	20.968	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.880%
43) trans-1,3-Dichloroprop...	10.581	79	12348	17.848	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.400%
47) 2-Hexanone-d5	10.922	63	9226	32.725	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.460%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	27395	21.579	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	23413	22.067	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.280%
Target Compounds					Qvalue	
13) Acetone	4.125	43	7746	13.517	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029881.D
Acq On : 09 Aug 2024 17:55
Operator : SY/MD
Sample : P3481-08RE
Misc : 6.21g/10mL/MSVOA_W/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AE4RE

Quant Time: Aug 09 23:18:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 09 23:13:22 2024
Response via : Initial Calibration

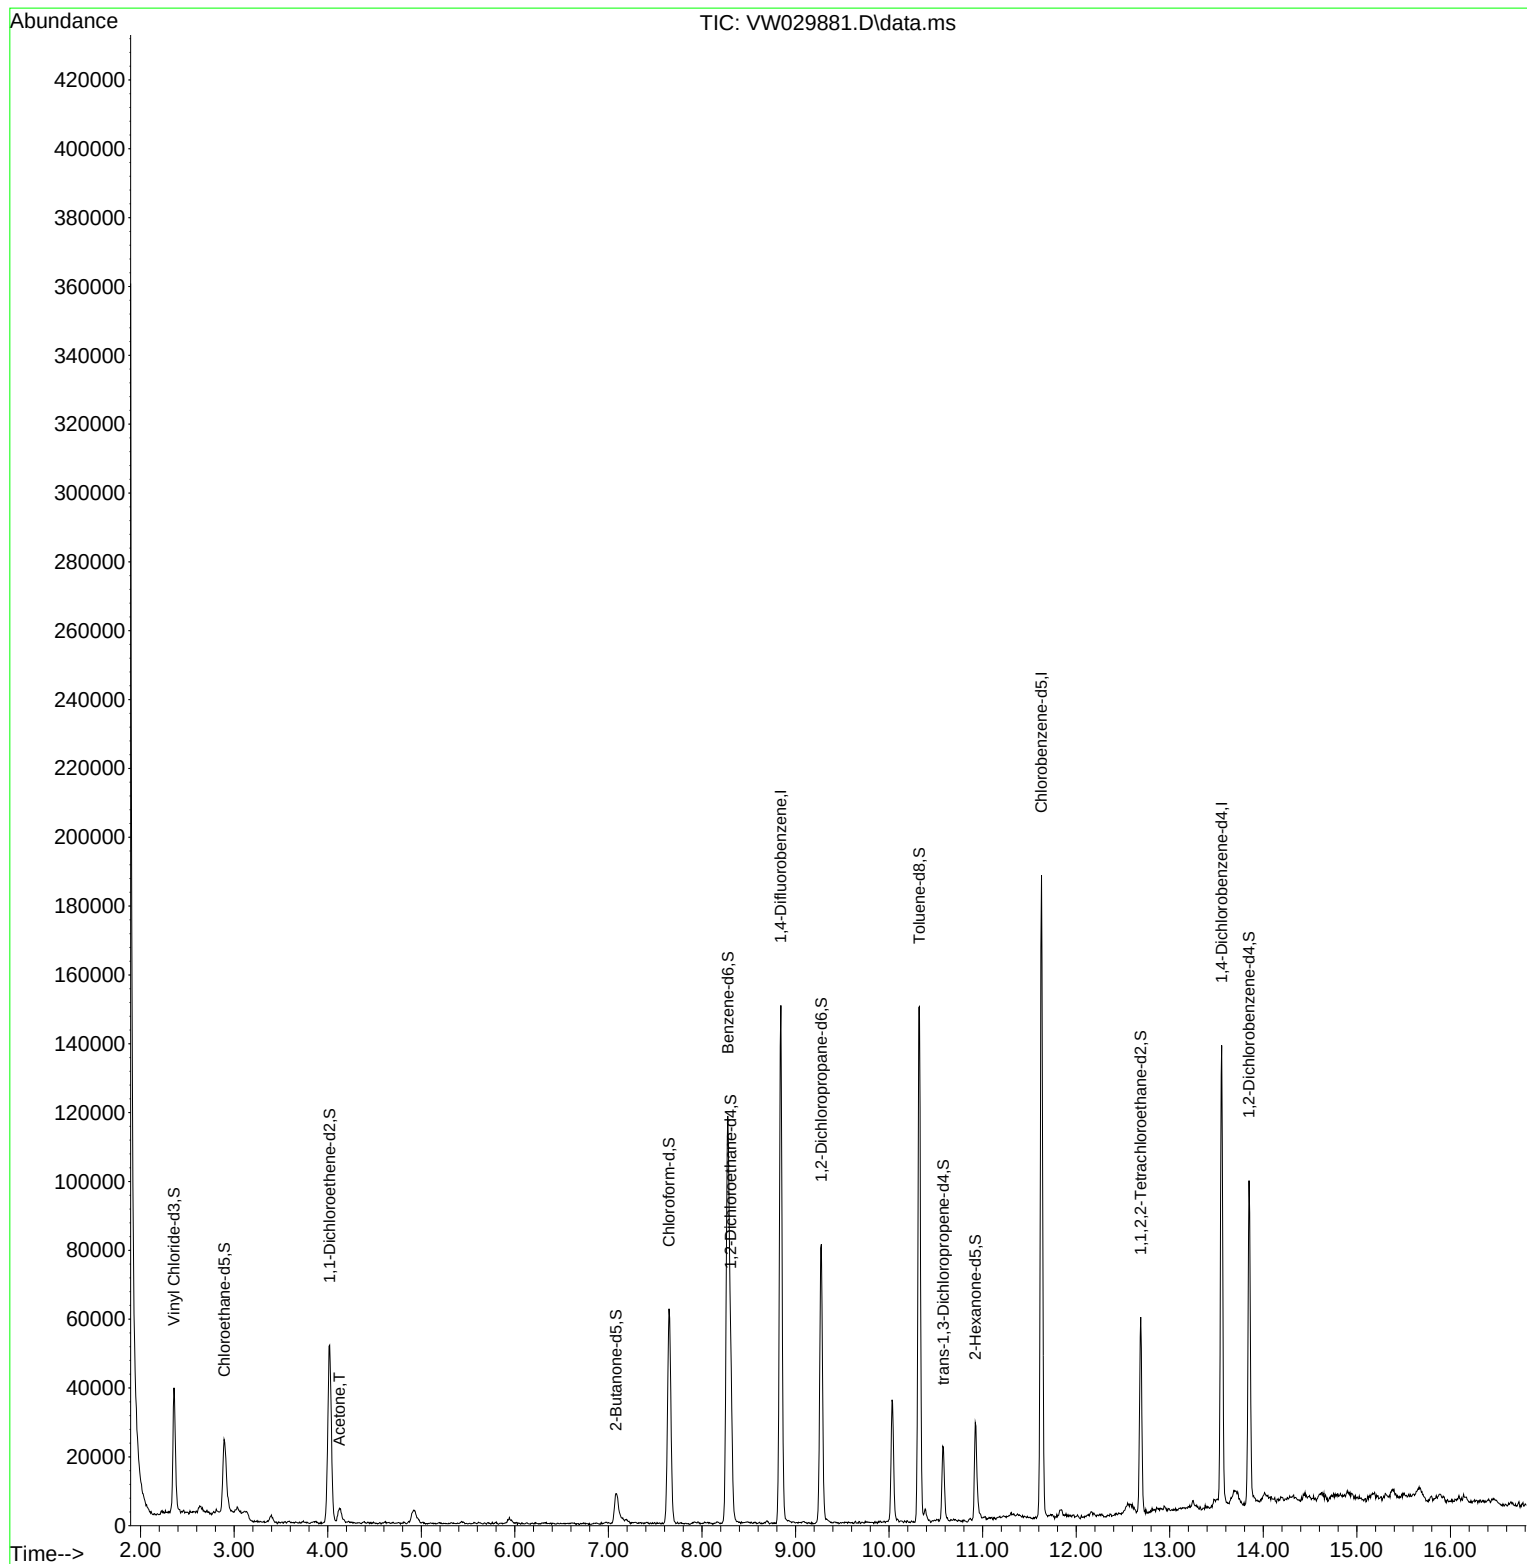

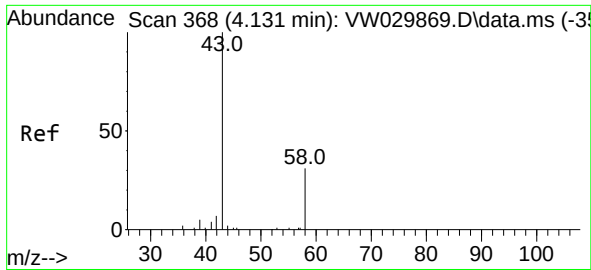

#13
 Acetone
 Concen: 13.517 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW029881.D
 Acq: 09 Aug 2024 17:55

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AE4RE

Tgt Ion: 43 Resp: 7746
 Ion Ratio Lower Upper
 43 100
 58 31.8 0.0 57.6

