
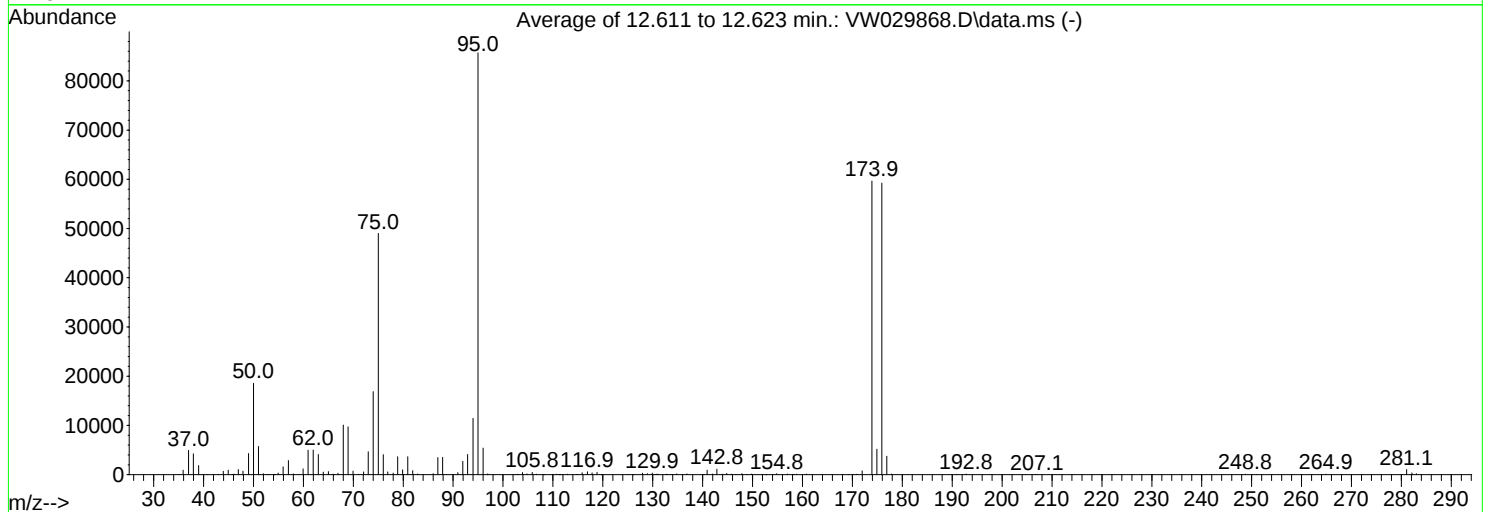


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080924\
Data File : VW029868.D
Acq On : 09 Aug 2024 11:07
Operator : SY/MD
Sample : BFB542
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB542

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Title : SFAM01.0
Last Update : Tue Aug 13 01:26:37 2024

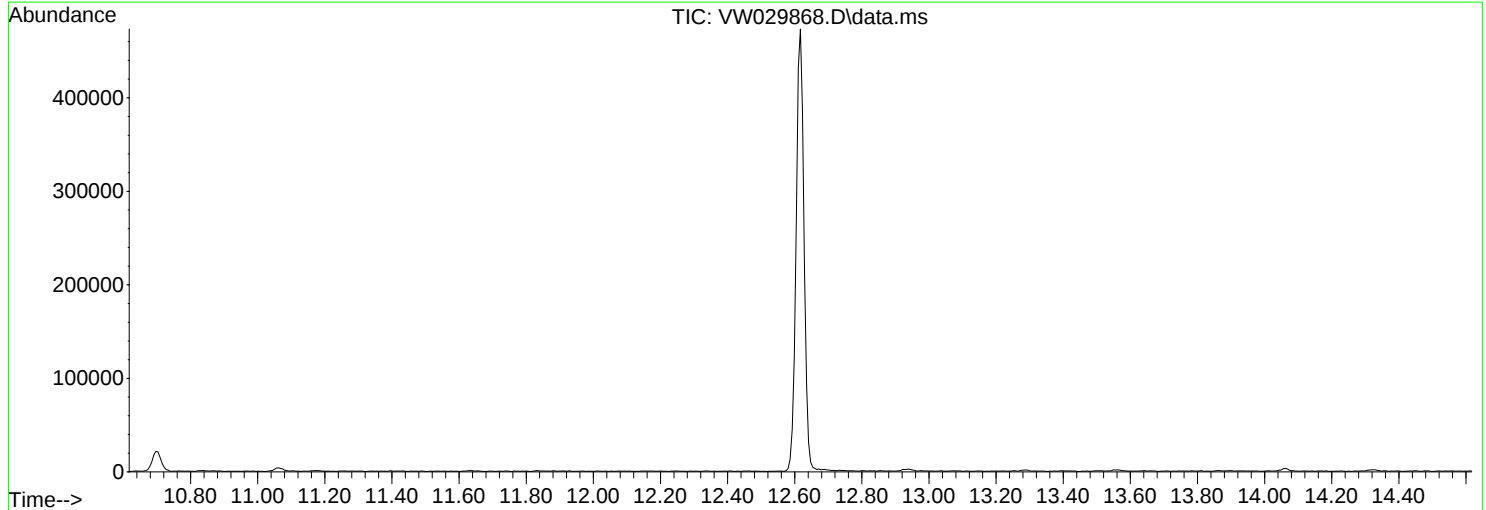

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	18565	PASS
75	95	30	80	57.2	49013	PASS
95	95	100	100	100.0	85693	PASS
96	95	5	9	6.3	5401	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.6	59653	PASS
175	174	5	9	8.7	5162	PASS
176	174	95	101	99.3	59235	PASS
177	176	5	9	6.3	3726	PASS

m/z	Abundance
35.90	65.0
37.60	52.0
37.90	51.0
40.00	168.0
41.10	73.0
43.00	56.0
43.90	197.0
50.00	52.0
52.10	56.0
68.90	54.0
84.30	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB542

m/z	Abundance
35.90	1036.0
37.00	5028.0
38.00	4731.0
39.00	1998.0
39.90	201.0
43.10	116.0
44.00	996.0
45.00	1025.0
46.10	188.0
47.00	1199.0
47.90	796.0
49.00	4692.0
50.00	20264.0
51.00	5613.0
51.90	273.0
52.70	62.0
53.10	74.0
55.00	266.0
56.00	1606.0
57.00	2869.0
58.00	219.0
59.10	85.0
59.90	1212.0
61.00	5107.0
62.00	5546.0
63.00	4466.0
64.00	584.0
65.00	764.0
65.90	121.0
66.90	237.0
68.00	10330.0
69.00	9954.0
69.90	715.0
72.00	719.0
73.00	5000.0
74.00	16680.0
75.00	50968.0
76.00	4191.0
76.90	613.0
78.00	416.0
78.90	4032.0
79.90	1108.0
80.90	4091.0
81.90	855.0
82.90	128.0
86.00	220.0
86.90	3811.0
87.90	3761.0
88.70	137.0
90.90	385.0
92.00	2681.0
92.90	4289.0
94.00	11590.0
95.00	85184.0
96.00	5695.0
96.90	145.0
102.90	108.0
103.90	482.0
104.80	208.0
105.90	566.0
106.80	85.0
110.00	110.0
110.80	155.0
112.00	75.0
113.00	111.0
114.80	141.0
115.90	449.0
116.90	616.0
117.90	289.0
118.80	496.0
119.70	53.0
123.80	66.0
125.00	77.0
127.90	286.0
128.90	170.0
129.90	297.0
130.60	106.0
131.10	153.0
132.80	206.0
133.60	88.0
134.70	154.0
136.80	144.0
140.90	835.0
142.10	118.0
142.90	1153.0
143.90	71.0
144.80	304.0
145.70	141.0
146.90	75.0
148.00	193.0
148.90	90.0
149.80	148.0

Instrument :
MSVOA_W
ClientSampleId :
BFB542

152.70	57.0
154.00	70.0
154.80	235.0
156.90	92.0
158.80	98.0
160.80	134.0
169.20	55.0
170.10	103.0
171.00	206.0
172.00	746.0
173.90	56888.0
174.90	4867.0
175.90	53224.0
176.90	3643.0
177.90	132.0
191.00	71.0
192.90	244.0
204.70	60.0
207.10	108.0
248.70	119.0
251.00	82.0
264.90	199.0
281.10	1519.0
282.10	550.0
283.00	300.0
284.10	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB542

m/z	Abundance
35.10	119.0
36.00	1072.0
37.00	5641.0
38.00	4669.0
39.00	2032.0
39.90	195.0
42.90	151.0
44.00	954.0
44.90	998.0
46.10	143.0
46.90	1074.0
47.90	786.0
49.00	4581.0
50.00	20480.0
51.00	6364.0
52.00	281.0
53.10	97.0
54.00	64.0
55.00	343.0
55.90	1694.0
57.00	3216.0
58.00	139.0
60.00	1432.0
61.00	5440.0
61.90	5436.0
63.00	4448.0
63.90	576.0
65.00	626.0
66.00	135.0
66.90	351.0
68.00	11702.0
69.00	11212.0
70.00	725.0
71.10	111.0
72.10	594.0
73.00	4990.0
74.00	19496.0
75.00	55056.0
76.00	4682.0
76.90	682.0
78.00	356.0
78.90	3819.0
79.90	1031.0
80.90	3847.0
81.90	979.0
82.90	162.0
86.10	215.0
86.90	3766.0
87.90	3697.0
90.90	463.0
91.90	2957.0
92.90	4329.0
94.00	12167.0
95.00	95904.0
96.00	5931.0
96.90	182.0
102.90	119.0
103.90	395.0
104.90	170.0
105.80	530.0
106.70	123.0
110.00	135.0
110.70	61.0
111.90	63.0
112.80	142.0
114.80	77.0
115.80	413.0
116.90	627.0
117.90	383.0
118.80	525.0
123.90	71.0
127.90	354.0
129.00	194.0
129.90	437.0
130.80	189.0
133.00	153.0
134.00	87.0
134.80	190.0
136.90	185.0
140.90	1047.0
141.90	146.0
142.80	1153.0
143.90	115.0
144.90	299.0
145.90	207.0
146.60	84.0
147.80	194.0
148.80	52.0
149.90	115.0
154.10	54.0
154.80	162.0
157.00	153.0

Instrument :
MSVOA_W
ClientSampleId :
BFB542

158.30	61.0
158.80	101.0
160.80	109.0
169.20	51.0
171.90	927.0
173.90	63960.0
174.90	5769.0
175.90	64024.0
176.90	3949.0
177.80	113.0
191.00	84.0
192.70	151.0
206.60	74.0
207.00	67.0
248.80	139.0
250.90	51.0
264.80	64.0
281.00	1216.0
282.10	413.0
283.10	185.0
284.10	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB542

m/z	Abundance
36.00	849.0
37.00	4122.0
38.00	3473.0
39.00	1544.0
39.90	191.0
40.80	86.0
41.30	55.0
42.80	87.0
44.00	659.0
45.00	693.0
45.80	126.0
47.00	881.0
47.90	559.0
49.00	3658.0
50.00	15106.0
51.00	5224.0
52.00	222.0
53.00	74.0
54.20	54.0
54.90	333.0
56.00	1477.0
57.00	2544.0
58.00	160.0
60.00	832.0
60.90	4392.0
62.00	4081.0
63.00	3406.0
64.10	457.0
65.00	511.0
66.20	94.0
67.00	310.0
68.00	8179.0
69.00	8161.0
70.00	700.0
71.00	96.0
72.00	397.0
73.00	3920.0
74.00	14436.0
75.00	41016.0
76.00	3353.0
76.90	379.0
77.90	237.0
78.90	3112.0
79.90	792.0
80.90	3005.0
81.90	608.0
82.90	122.0
85.90	137.0
87.00	2846.0
87.90	3048.0
91.00	424.0
91.90	2474.0
92.90	3700.0
94.00	10532.0
95.00	75992.0
96.00	4578.0
97.00	172.0
102.40	67.0
103.10	75.0
103.90	397.0
104.70	116.0
105.80	329.0
106.60	110.0
108.10	58.0
110.80	113.0
111.30	52.0
112.80	79.0
115.00	138.0
115.90	318.0
116.90	564.0
117.80	361.0
118.90	364.0
126.00	57.0
128.00	250.0
128.90	194.0
129.90	236.0
130.90	208.0
132.70	78.0
134.90	120.0
136.90	179.0
140.10	98.0
140.90	846.0
141.80	140.0
142.90	994.0
143.90	73.0
144.90	199.0
145.70	145.0
146.60	60.0
147.80	180.0
148.80	74.0
149.90	108.0
154.90	206.0

Instrument :
MSVOA_W
ClientSampleId :
BFB542

157.00	121.0
158.90	79.0
160.80	116.0
170.80	131.0
171.90	643.0
173.90	58112.0
174.90	4849.0
175.90	60456.0
176.90	3585.0
177.80	121.0
190.90	76.0
206.70	85.0
265.00	56.0
281.00	403.0
282.00	120.0
282.90	134.0

Instrument :
MSVOA_W
ClientSampleId :
BFB542