


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081118\
 Data File : VW004557.D
 Acq On : 09 Aug 2018 15:01
 Operator : SY/AP
 Sample : BFB94
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB94

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Title : VOC Analysis
 Last Update : Fri Aug 10 05:02:45 2018

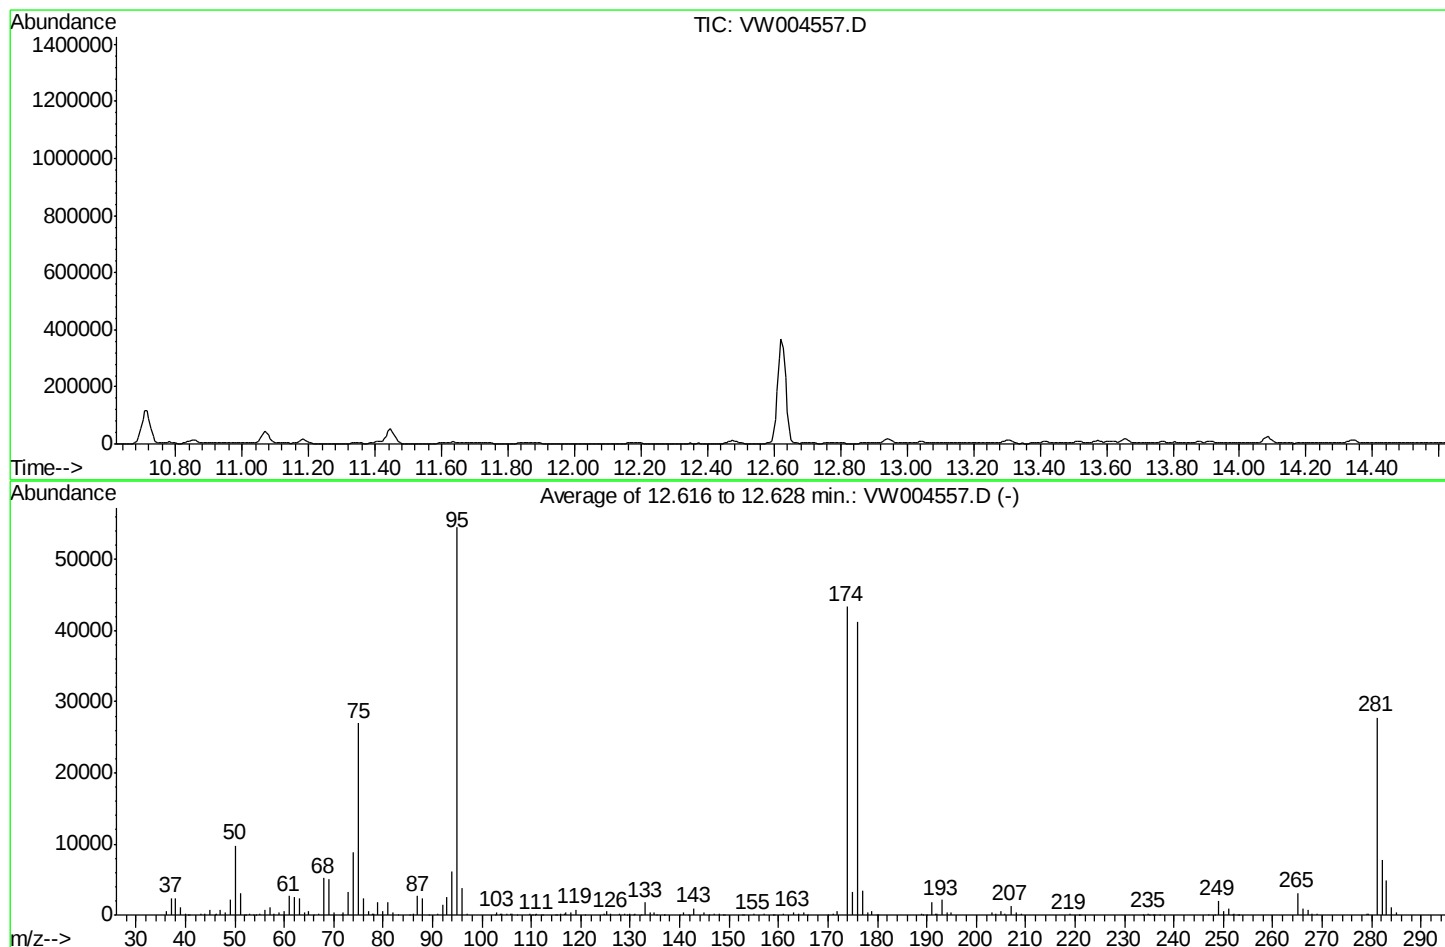

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9788	PASS
75	95	30	80	49.5	26981	PASS
95	95	100	100	100.0	54552	PASS
96	95	5	9	6.9	3786	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.4	43328	PASS
175	174	5	9	7.5	3246	PASS
176	174	95	101	95.4	41344	PASS
177	176	5	9	8.2	3403	PASS

Scan 1802 (12.573 min): VW004557.D
BFB94

m/z	Abundance
36.10	81.0
39.00	56.0
40.00	442.0
41.00	137.0
42.30	77.0
44.00	764.0
45.10	73.0
55.10	84.0
57.10	86.0
69.10	93.0
73.00	177.0
207.20	241.0
280.80	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

m/z	Abundance
36.00	552.0
37.10	2384.0
38.00	2318.0
39.10	960.0
40.10	611.0
41.20	104.0
43.10	213.0
43.90	840.0
45.00	964.0
46.30	151.0
46.90	469.0
48.00	272.0
49.00	1984.0
50.00	8714.0
51.10	2912.0
51.90	131.0
53.00	140.0
54.10	58.0
55.00	194.0
56.10	696.0
57.00	993.0
58.10	110.0
59.00	391.0
59.90	421.0
61.00	2295.0
62.00	2441.0
63.10	2175.0
64.00	275.0
65.00	453.0
67.00	177.0
68.00	4839.0
69.00	3926.0
70.00	273.0
71.70	185.0
73.10	3317.0
74.00	7484.0
75.00	24064.0
76.00	1775.0
77.10	283.0
77.90	162.0
78.90	1392.0
79.90	471.0
80.90	1448.0
81.90	447.0
83.00	54.0
85.20	86.0
86.00	214.0
87.00	2607.0
88.00	1630.0
89.10	161.0
91.00	186.0
92.10	1236.0
93.00	2318.0
94.00	4995.0
95.00	45672.0
96.00	3278.0
97.10	108.0
103.00	541.0
103.80	363.0
105.00	198.0
106.00	162.0
107.10	103.0
109.80	259.0
111.10	289.0
112.40	154.0
114.90	183.0
115.90	173.0
116.80	645.0
117.90	402.0
119.00	787.0
121.00	99.0
124.80	669.0
126.30	152.0
127.80	243.0
128.90	114.0
130.00	183.0
130.70	145.0
131.10	184.0
132.10	94.0
133.10	2298.0
134.90	321.0
136.80	93.0
140.10	65.0
140.80	405.0
142.90	733.0
145.00	371.0
146.00	105.0
146.80	268.0
148.10	181.0
149.10	226.0
152.70	63.0
154.90	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

156.90	70.0
158.80	64.0
160.90	266.0
162.90	546.0
163.90	105.0
165.10	351.0
171.10	183.0
172.10	352.0
173.90	31984.0
175.00	2411.0
175.90	31264.0
177.00	3118.0
178.00	268.0
178.90	583.0
180.20	109.0
188.90	205.0
190.00	52.0
191.00	2562.0
191.80	476.0
193.00	2552.0
194.00	553.0
195.00	426.0
203.00	371.0
204.00	130.0
205.00	649.0
205.80	208.0
207.00	1670.0
208.10	437.0
209.00	284.0
219.00	201.0
221.10	148.0
234.80	429.0
235.90	102.0
246.80	67.0
249.00	2206.0
249.90	460.0
251.00	1109.0
252.00	375.0
253.20	75.0
265.00	3968.0
266.10	1012.0
267.00	868.0
267.90	171.0
269.10	166.0
279.10	468.0
281.10	31256.0
282.10	8765.0
283.00	5413.0
284.10	1308.0
285.20	327.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

m/z	Abundance
36.00	648.0
37.10	2394.0
38.00	2398.0
39.00	1208.0
40.10	592.0
40.60	132.0
41.10	131.0
43.00	161.0
44.00	1027.0
45.00	764.0
46.10	320.0
47.00	1137.0
48.00	315.0
49.10	2262.0
50.00	11220.0
51.10	3378.0
51.90	141.0
52.90	125.0
54.20	59.0
55.10	298.0
56.10	817.0
57.10	1282.0
58.00	92.0
59.00	317.0
60.00	434.0
61.00	3057.0
62.00	2591.0
63.00	2535.0
64.10	670.0
65.10	545.0
66.90	176.0
67.10	198.0
68.00	5636.0
69.00	5864.0
70.10	501.0
72.00	383.0
73.00	3826.0
74.00	9918.0
75.00	29096.0
76.00	2648.0
77.10	512.0
78.10	336.0
78.90	2270.0
80.00	484.0
80.90	2185.0
81.80	509.0
86.00	124.0
87.00	2573.0
88.00	2919.0
91.00	111.0
91.90	1688.0
92.90	2825.0
94.00	7087.0
95.00	60328.0
96.10	4087.0
103.00	754.0
104.10	270.0
105.00	181.0
105.70	217.0
107.10	78.0
110.10	133.0
110.90	169.0
112.10	143.0
115.10	240.0
115.90	339.0
117.00	519.0
117.80	502.0
118.90	828.0
120.80	69.0
125.20	1211.0
126.10	307.0
127.90	234.0
128.80	128.0
129.40	74.0
130.00	177.0
131.00	145.0
133.00	2038.0
133.90	457.0
134.70	149.0
135.20	230.0
136.80	55.0
140.10	86.0
140.90	455.0
142.00	103.0
142.80	900.0
145.10	546.0
146.10	61.0
146.90	333.0
147.90	200.0
148.80	131.0
152.90	126.0
154.90	189.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

157.00	155.0
159.00	64.0
160.90	316.0
162.80	389.0
164.00	122.0
165.00	367.0
165.80	63.0
170.10	56.0
171.00	203.0
171.90	610.0
173.90	47880.0
175.00	3717.0
175.90	44896.0
176.90	3618.0
177.90	364.0
179.00	578.0
179.90	108.0
188.90	273.0
190.00	83.0
191.00	1886.0
192.00	373.0
193.00	2378.0
194.00	421.0
194.90	280.0
203.10	436.0
204.10	167.0
205.00	599.0
207.00	2030.0
208.20	360.0
209.00	220.0
218.90	150.0
220.80	143.0
233.80	82.0
235.10	252.0
236.10	54.0
237.10	78.0
248.20	95.0
249.00	2111.0
250.00	679.0
251.00	702.0
252.10	272.0
252.90	98.0
265.00	3347.0
266.00	1195.0
266.90	773.0
268.00	287.0
268.90	71.0
279.30	337.0
281.10	31256.0
282.00	8452.0
283.00	5179.0
284.10	935.0
285.10	370.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

m/z	Abundance
36.10	661.0
37.00	2488.0
38.10	2406.0
39.00	1256.0
39.90	333.0
40.10	338.0
40.80	98.0
43.00	143.0
44.00	845.0
45.10	759.0
45.90	77.0
46.20	88.0
46.90	798.0
48.00	371.0
49.00	2270.0
50.00	9430.0
51.00	2769.0
52.10	189.0
52.80	118.0
53.80	73.0
55.00	199.0
56.00	916.0
57.00	1329.0
57.90	131.0
58.90	221.0
60.00	643.0
61.00	2690.0
62.00	2720.0
63.00	2489.0
64.00	370.0
64.90	536.0
65.90	81.0
67.10	195.0
68.00	5092.0
69.00	5538.0
70.00	360.0
72.00	482.0
73.00	3093.0
74.00	9326.0
75.00	27784.0
76.00	2596.0
76.90	585.0
77.80	276.0
78.90	1862.0
79.90	766.0
80.90	1912.0
82.00	386.0
85.30	78.0
87.00	2737.0
88.00	2406.0
91.00	307.0
92.00	1337.0
93.00	2463.0
94.00	6236.0
95.00	57656.0
96.00	3994.0
97.00	189.0
102.70	85.0
104.00	252.0
104.90	96.0
105.70	97.0
106.10	152.0
109.80	172.0
110.80	101.0
112.00	144.0
114.80	70.0
116.00	293.0
117.00	638.0
117.80	280.0
119.00	605.0
125.00	631.0
126.00	178.0
127.90	180.0
128.80	137.0
129.90	228.0
130.90	161.0
133.20	1023.0
134.00	423.0
134.80	372.0
137.00	65.0
140.00	55.0
140.90	506.0
141.80	142.0
142.90	1075.0
144.90	401.0
146.10	120.0
146.80	111.0
147.80	113.0
148.60	107.0
152.90	113.0
155.00	192.0
157.00	133.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

159.10	75.0
160.90	176.0
163.00	285.0
163.90	71.0
165.00	148.0
171.00	156.0
172.00	816.0
173.90	50120.0
174.90	3610.0
175.90	47872.0
176.90	3474.0
177.90	254.0
178.90	372.0
179.80	69.0
188.90	108.0
189.30	53.0
190.90	996.0
191.90	206.0
193.00	1473.0
194.10	356.0
195.10	208.0
203.00	206.0
204.90	311.0
205.70	87.0
207.00	1015.0
208.20	255.0
209.00	220.0
233.70	62.0
234.80	174.0
236.20	130.0
237.20	61.0
248.10	64.0
248.90	1695.0
249.90	272.0
251.10	756.0
251.80	203.0
252.90	53.0
265.00	2143.0
266.00	660.0
267.10	556.0
267.90	161.0
268.90	75.0
279.20	228.0
281.10	20776.0
282.10	6095.0
283.00	3866.0
284.00	763.0
285.00	207.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94