

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081125\
 Data File : VW032058.D
 Acq On : 11 Aug 2025 11:30
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Quant Time: Aug 12 04:12:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W081125S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 12 04:04:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.965	168	176488	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	360864	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.629	117	330434	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	156308	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	127081	49.787	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	99.580%
35) Dibromofluoromethane	7.904	113	117071	50.217	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	100.440%
50) Toluene-d8	10.325	98	424673	49.250	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	98.500%
62) 4-Bromofluorobenzene	12.617	95	152918	48.123	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	96.240%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081125\
Data File : VW032058.D
Acq On : 11 Aug 2025 11:30
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Quant Time: Aug 12 04:12:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W081125S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 12 04:04:48 2025
Response via : Initial Calibration




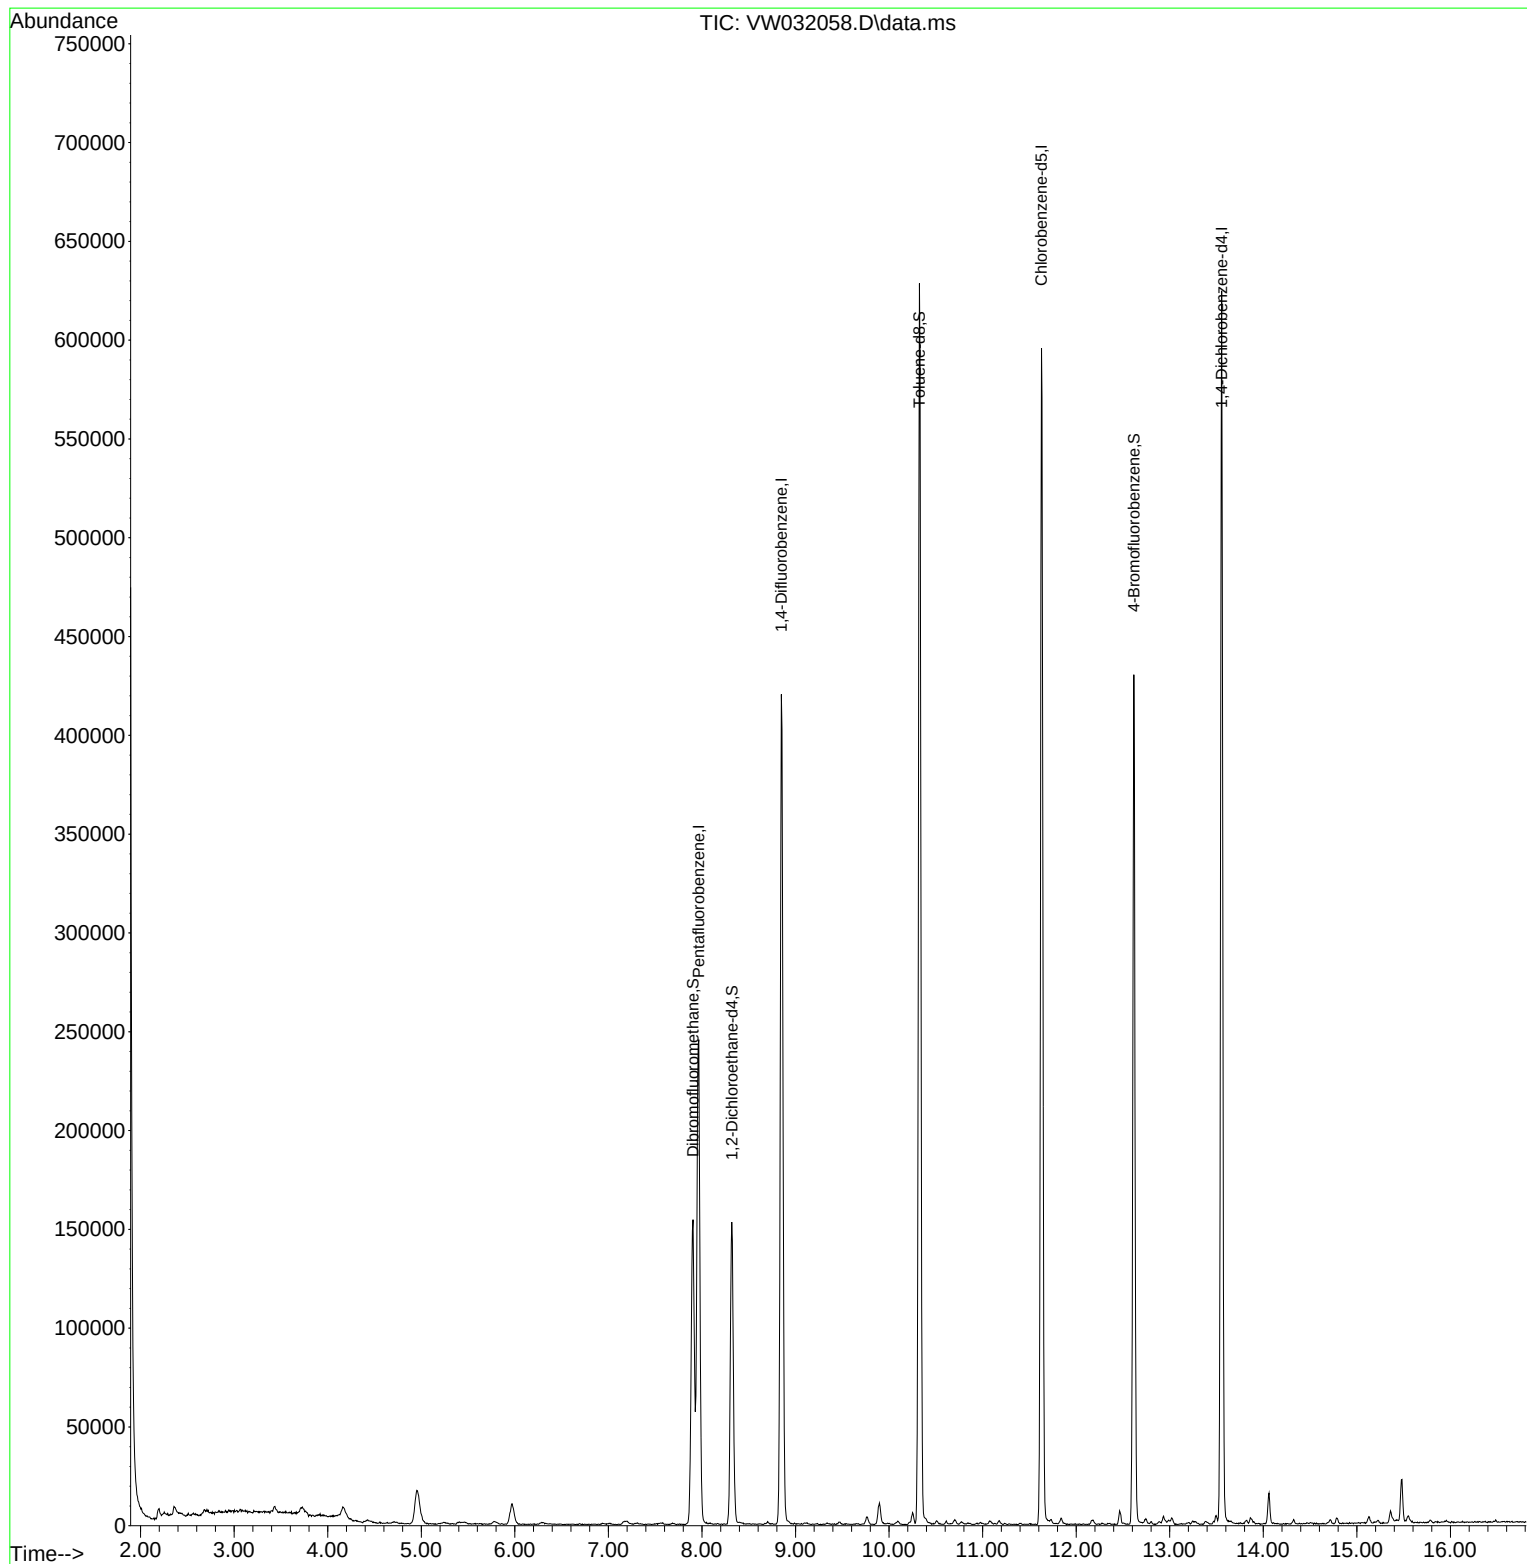


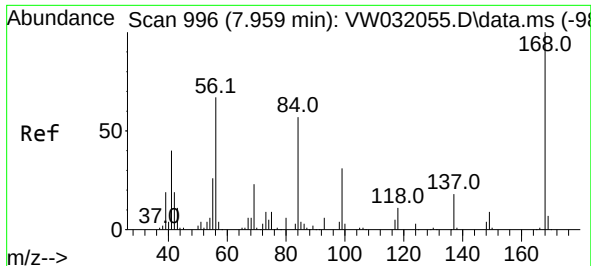

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.965 min Scan# 996
Delta R.T. 0.006 min
Lab File: VW032058.D
Acq: 11 Aug 2025 11:30




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 176488
Ion Ratio Lower Upper
168 100
99 60.5 56.0 84.0

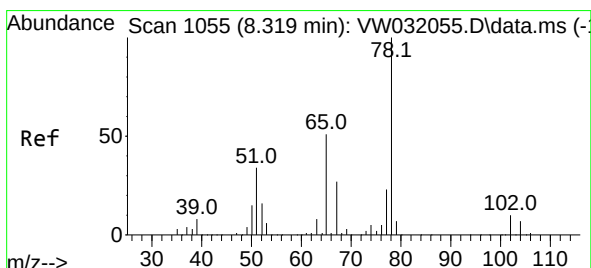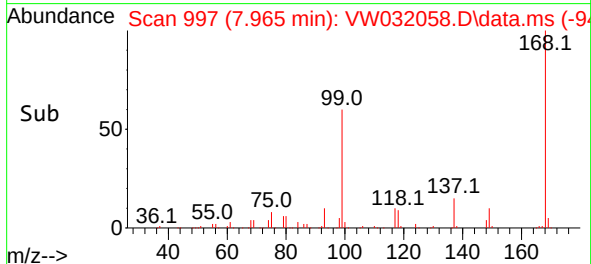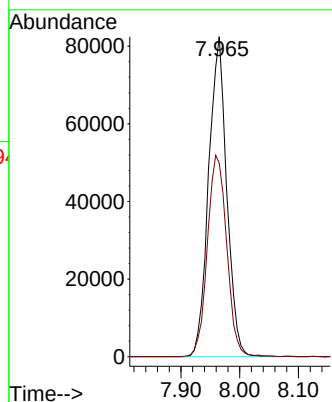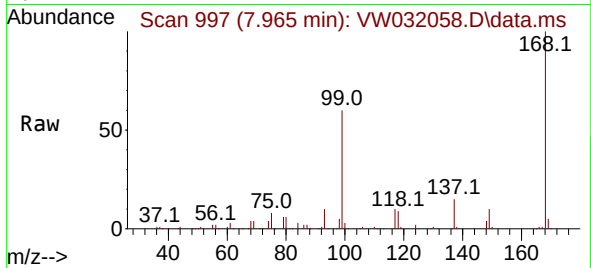

#33
1,2-Dichloroethane-d4
Concen: 49.787 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. -0.000 min
Lab File: VW032058.D
Acq: 11 Aug 2025 11:30

Tgt Ion: 65 Resp: 127081
Ion Ratio Lower Upper
65 100
67 50.8 0.0 102.4

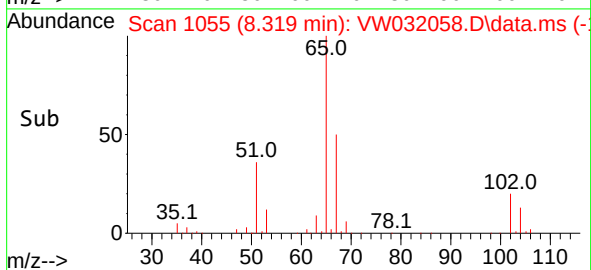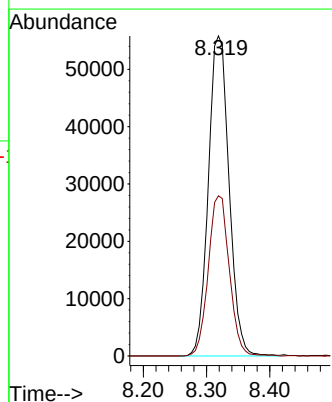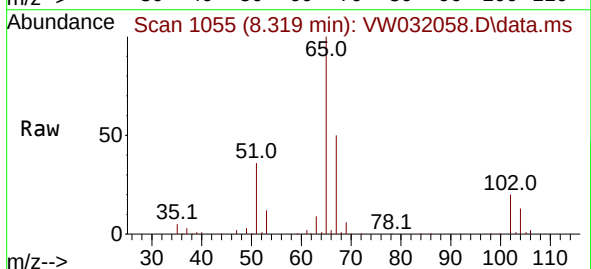

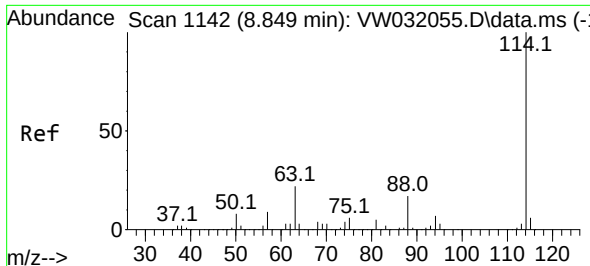

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.849 min Scan# 1142

Delta R.T. -0.000 min

Lab File: VW032058.D

Acq: 11 Aug 2025 11:30

Instrument :

MSVOA_W

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 360864

Ion Ratio Lower Upper

114 100

63 20.6 0.0 43.0

88 16.2 0.0 33.8

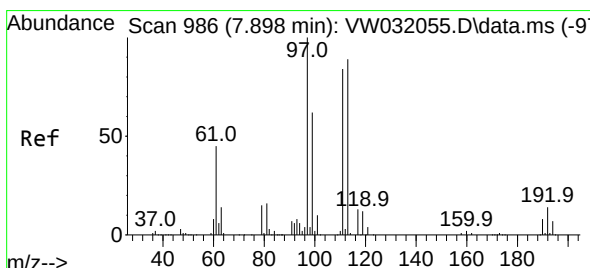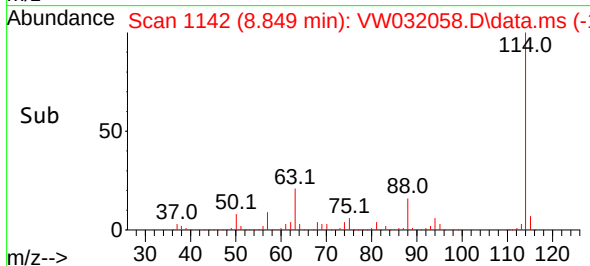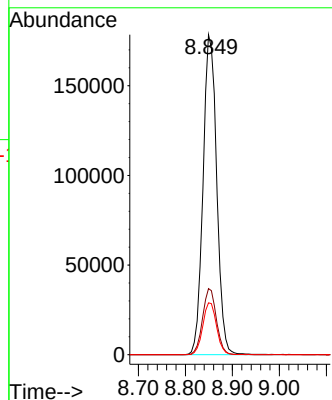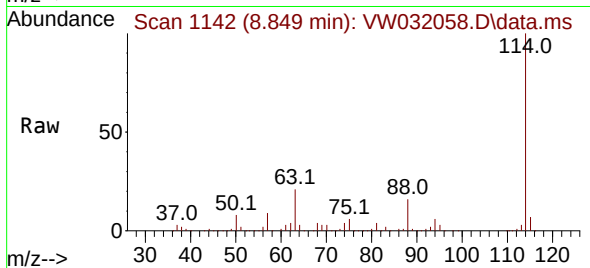

#35

Dibromofluoromethane

Concen: 50.217 ug/l

RT: 7.904 min Scan# 987

Delta R.T. 0.006 min

Lab File: VW032058.D

Acq: 11 Aug 2025 11:30




Tgt Ion:113 Resp: 117071


Ion Ratio Lower Upper

113 100

111 99.8 80.1 120.1

192 16.1 13.1 19.7


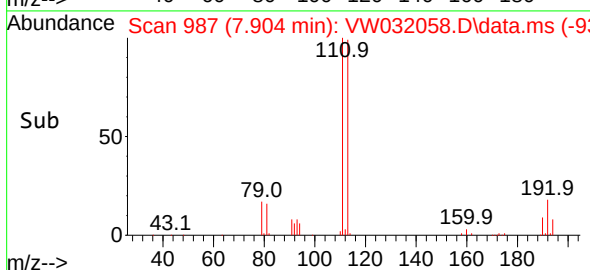
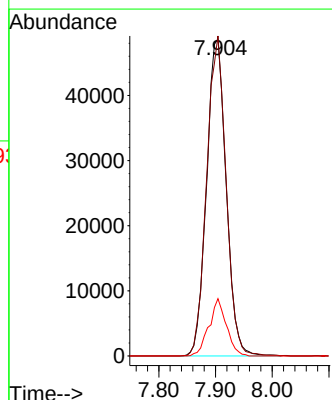
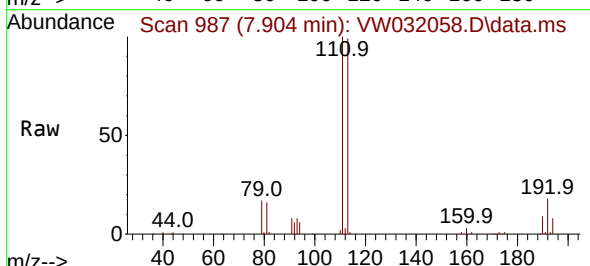


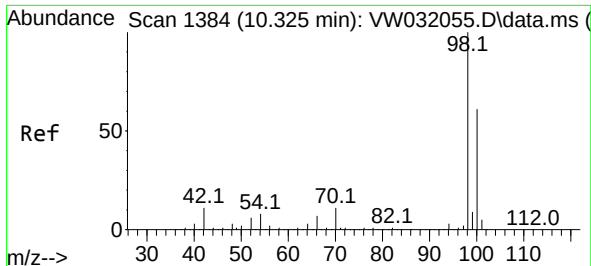

#50
Toluene-d8
Concen: 49.250 ug/l
RT: 10.325 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW032058.D
Acq: 11 Aug 2025 11:30




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 424673
Ion Ratio Lower Upper
98 100
100 65.2 51.1 76.7

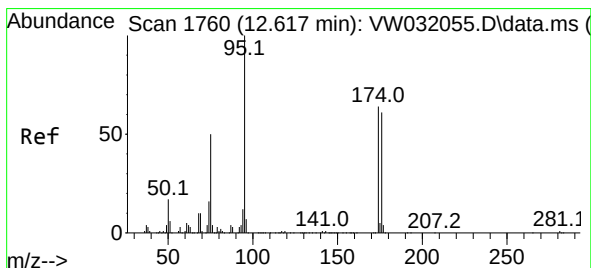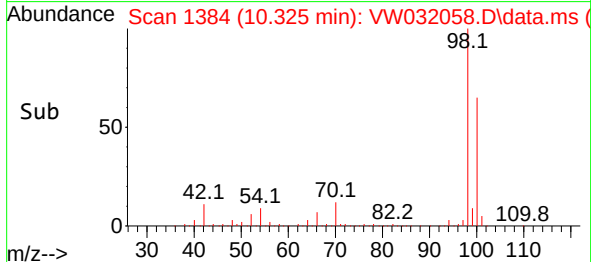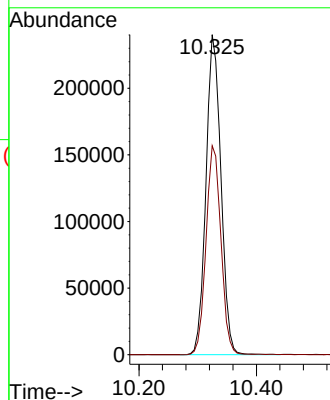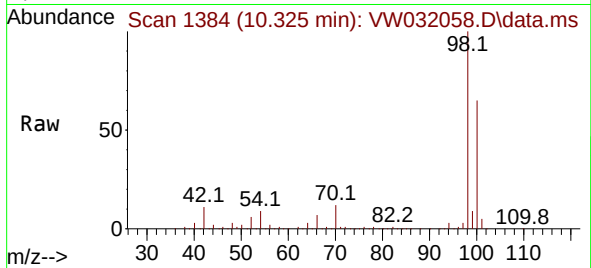

#62
4-Bromofluorobenzene
Concen: 48.123 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. -0.000 min
Lab File: VW032058.D
Acq: 11 Aug 2025 11:30

Tgt Ion: 95 Resp: 152918
Ion Ratio Lower Upper
95 100
174 64.7 0.0 129.0
176 64.3 0.0 124.6


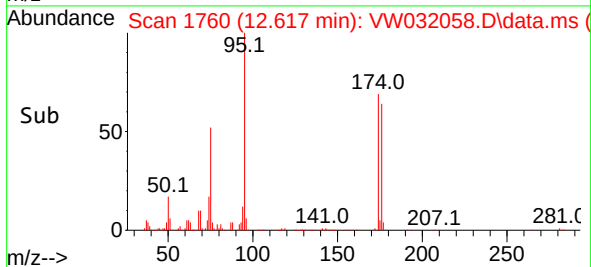
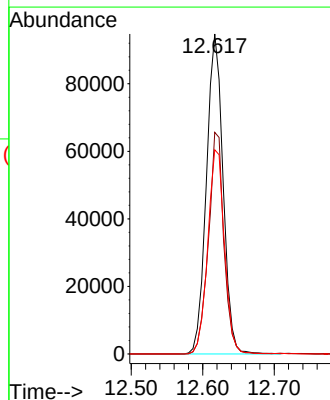
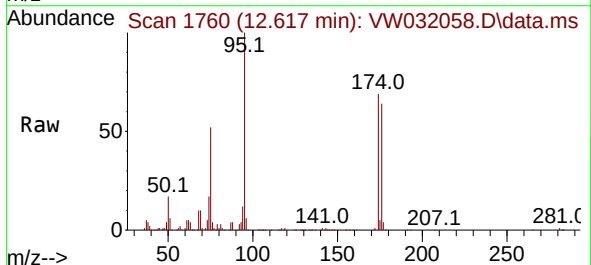


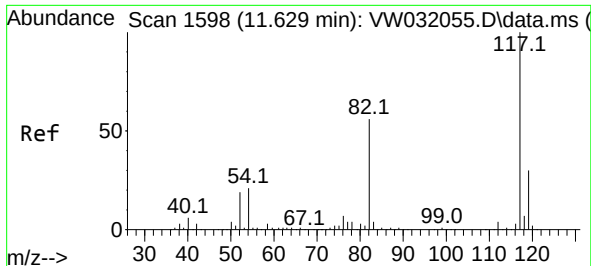

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.629 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW032058.D
Acq: 11 Aug 2025 11:30

Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 330434
Ion Ratio Lower Upper
117 100
82 60.5 45.0 67.4
119 31.6 24.2 36.4

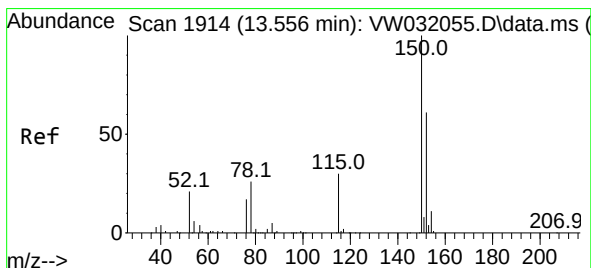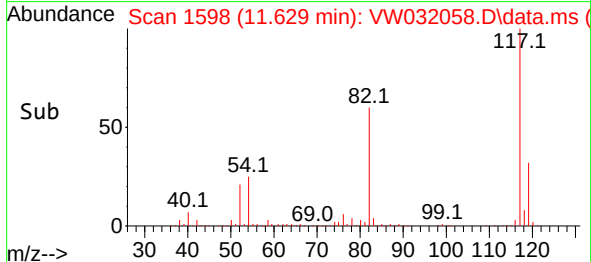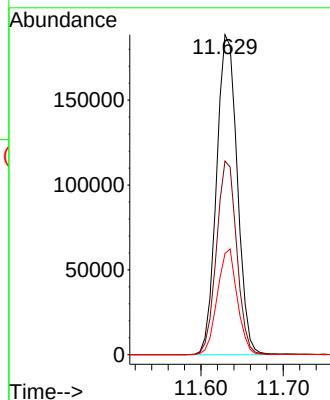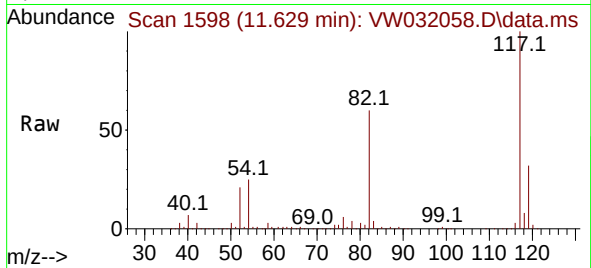

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. -0.000 min
Lab File: VW032058.D
Acq: 11 Aug 2025 11:30

Tgt Ion:152 Resp: 156308
Ion Ratio Lower Upper
152 100
115 64.9 32.6 97.8
150 157.8 0.0 359.4

