

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081324\
 Data File : VW029898.D
 Acq On : 13 Aug 2024 15:31
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 14 01:05:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 14 01:04:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	232236	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	214619	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	97826	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	78794	23.899	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.600%
7) Chloroethane-d5	2.899	69	65312	27.747	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.000%
11) 1,1-Dichloroethene-d2	4.021	65	33875	22.508	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.040%
21) 2-Butanone-d5	7.081	46	30108	33.318	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.640%
24) Chloroform-d	7.648	84	152552	25.375	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.520%
26) 1,2-Dichloroethane-d4	8.307	65	84569	24.697	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.800%
32) Benzene-d6	8.276	84	292545	25.228	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.920%
36) 1,2-Dichloropropane-d6	9.270	67	87330	23.585	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.360%
41) Toluene-d8	10.325	98	267757	25.968	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.880%
43) trans-1,3-Dichloroprop...	10.575	79	34938	23.318	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.280%
47) 2-Hexanone-d5	10.922	63	22602	37.019	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.040%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	67431	24.526	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.120%
66) 1,2-Dichlorobenzene-d4	13.849	152	87893	28.935	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	115.760%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	2877	0.490	ug/L	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081324\
Data File : VW029898.D
Acq On : 13 Aug 2024 15:31
Operator : SY/MD
Sample : VIBLK
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 14 01:05:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 14 01:04:35 2024
Response via : Initial Calibration

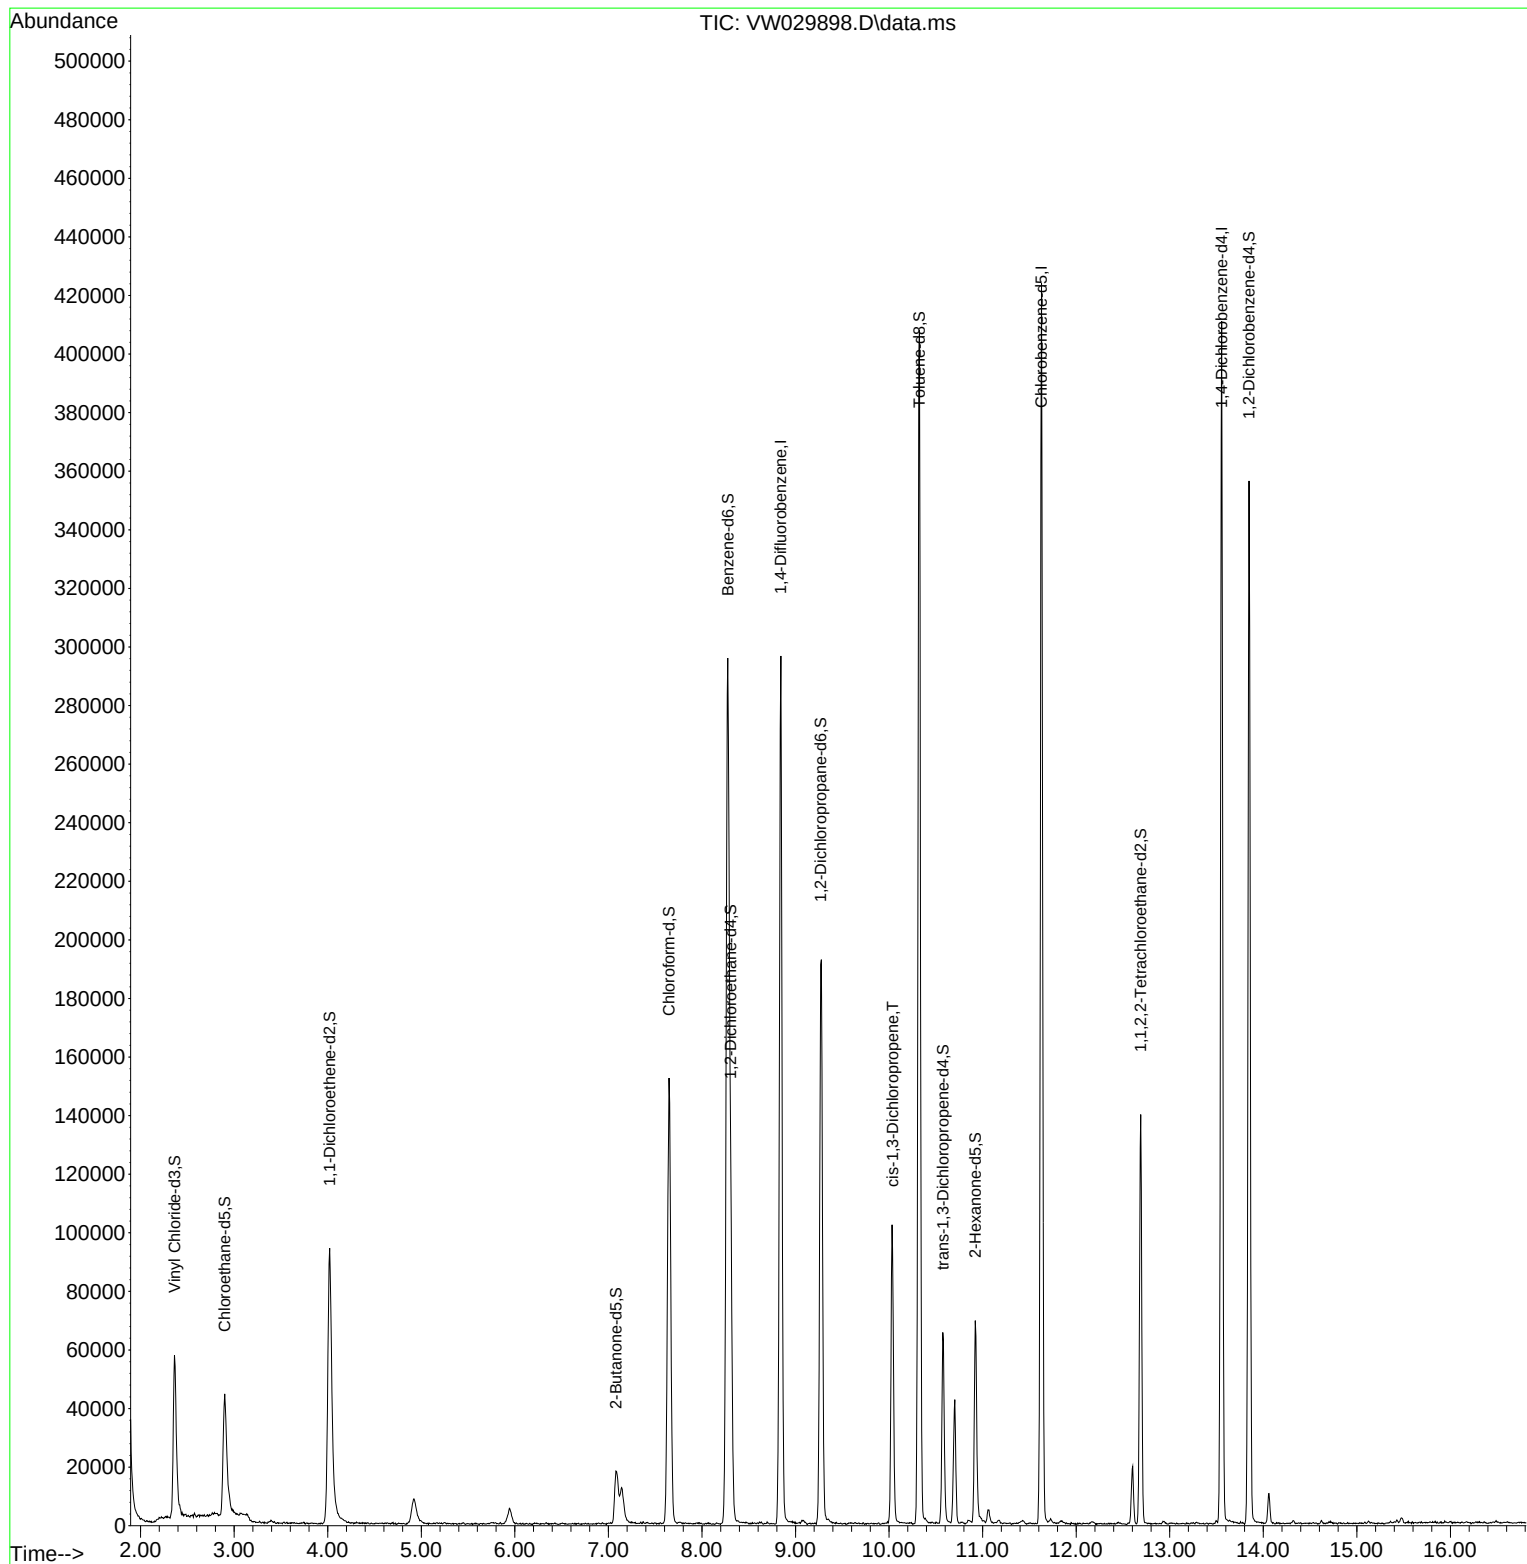

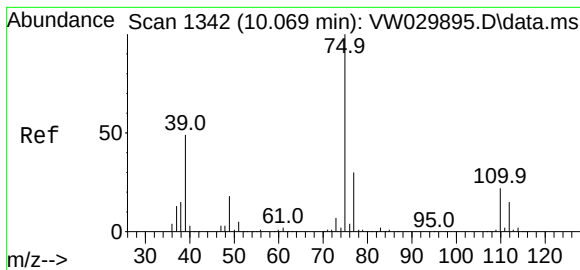

#39
cis-1,3-Dichloropropene
Concen: 0.490 ug/L
RT: 10.038 min Scan# 14
Delta R.T. -0.031 min
Lab File: VW029898.D
Acq: 13 Aug 2024 15:31

Instrument :
MSVOA_W
ClientSampleId :

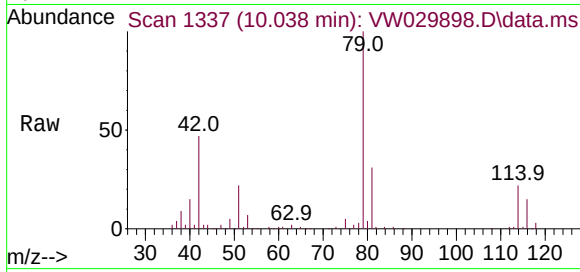

Tgt Ion: 75 Resp: 2877
Ion Ratio Lower Upper
75 100
77 44.8 20.8 38.6#

