

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_W\DATA\VW081418\
 Data File : VW004654.D
 Acq On : 13 Aug 2018 18:27
 Operator : SY/AP
 Sample : J4450-05
 Misc : 5.70G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAB04

Quant Time: Aug 14 01:21:32 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 14 01:20:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	785231	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	804933	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	342523	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	228361	23.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.52%
7) Chloroethane-d5	2.89	69	190886	23.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.92%
10) 1,1-Dichloroethene-d2	4.01	63	336163	16.95	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.80%
20) 2-Butanone-d5	7.09	46	299251	69.49	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	138.98%#
24) Chloroform-d	7.65	84	494329	23.25	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.00%
26) 1,2-Dichloroethane-d4	8.31	65	310546	26.20	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.80%
29) Benzene-d6	8.28	84	943077	22.02	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.08%
33) 1,2-Dichloropropane-d6	9.28	67	321607	22.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.92%
37) Toluene-d8	10.33	98	796418	21.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.40%
38) trans-1,3-Dichloropropene-	10.59	79	131942	22.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.72%
39) 2-Hexanone-d5	10.93	63	241063	70.76	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	141.52%#
48) 1,1,2,2-Tetrachloroethane-	12.70	84	426919	28.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.52%
61) 1,2-Dichlorobenzene-d4	13.86	152	328534	25.54	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.16%


Target Compounds					Qvalue
40) 1,2-Dichloropropane	9.27	63	32696	2.488 ug/L #	90
59) 1,2,3-Trichloropropane	13.57	75	39862	3.599 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_W\DATA\VW081418\
Data File : VW004654.D
Acq On : 13 Aug 2018 18:27
Operator : SY/AP
Sample : J4450-05
Misc : 5.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAB04

Quant Time: Aug 14 01:21:32 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 14 01:20:10 2018
Response via : Initial Calibration

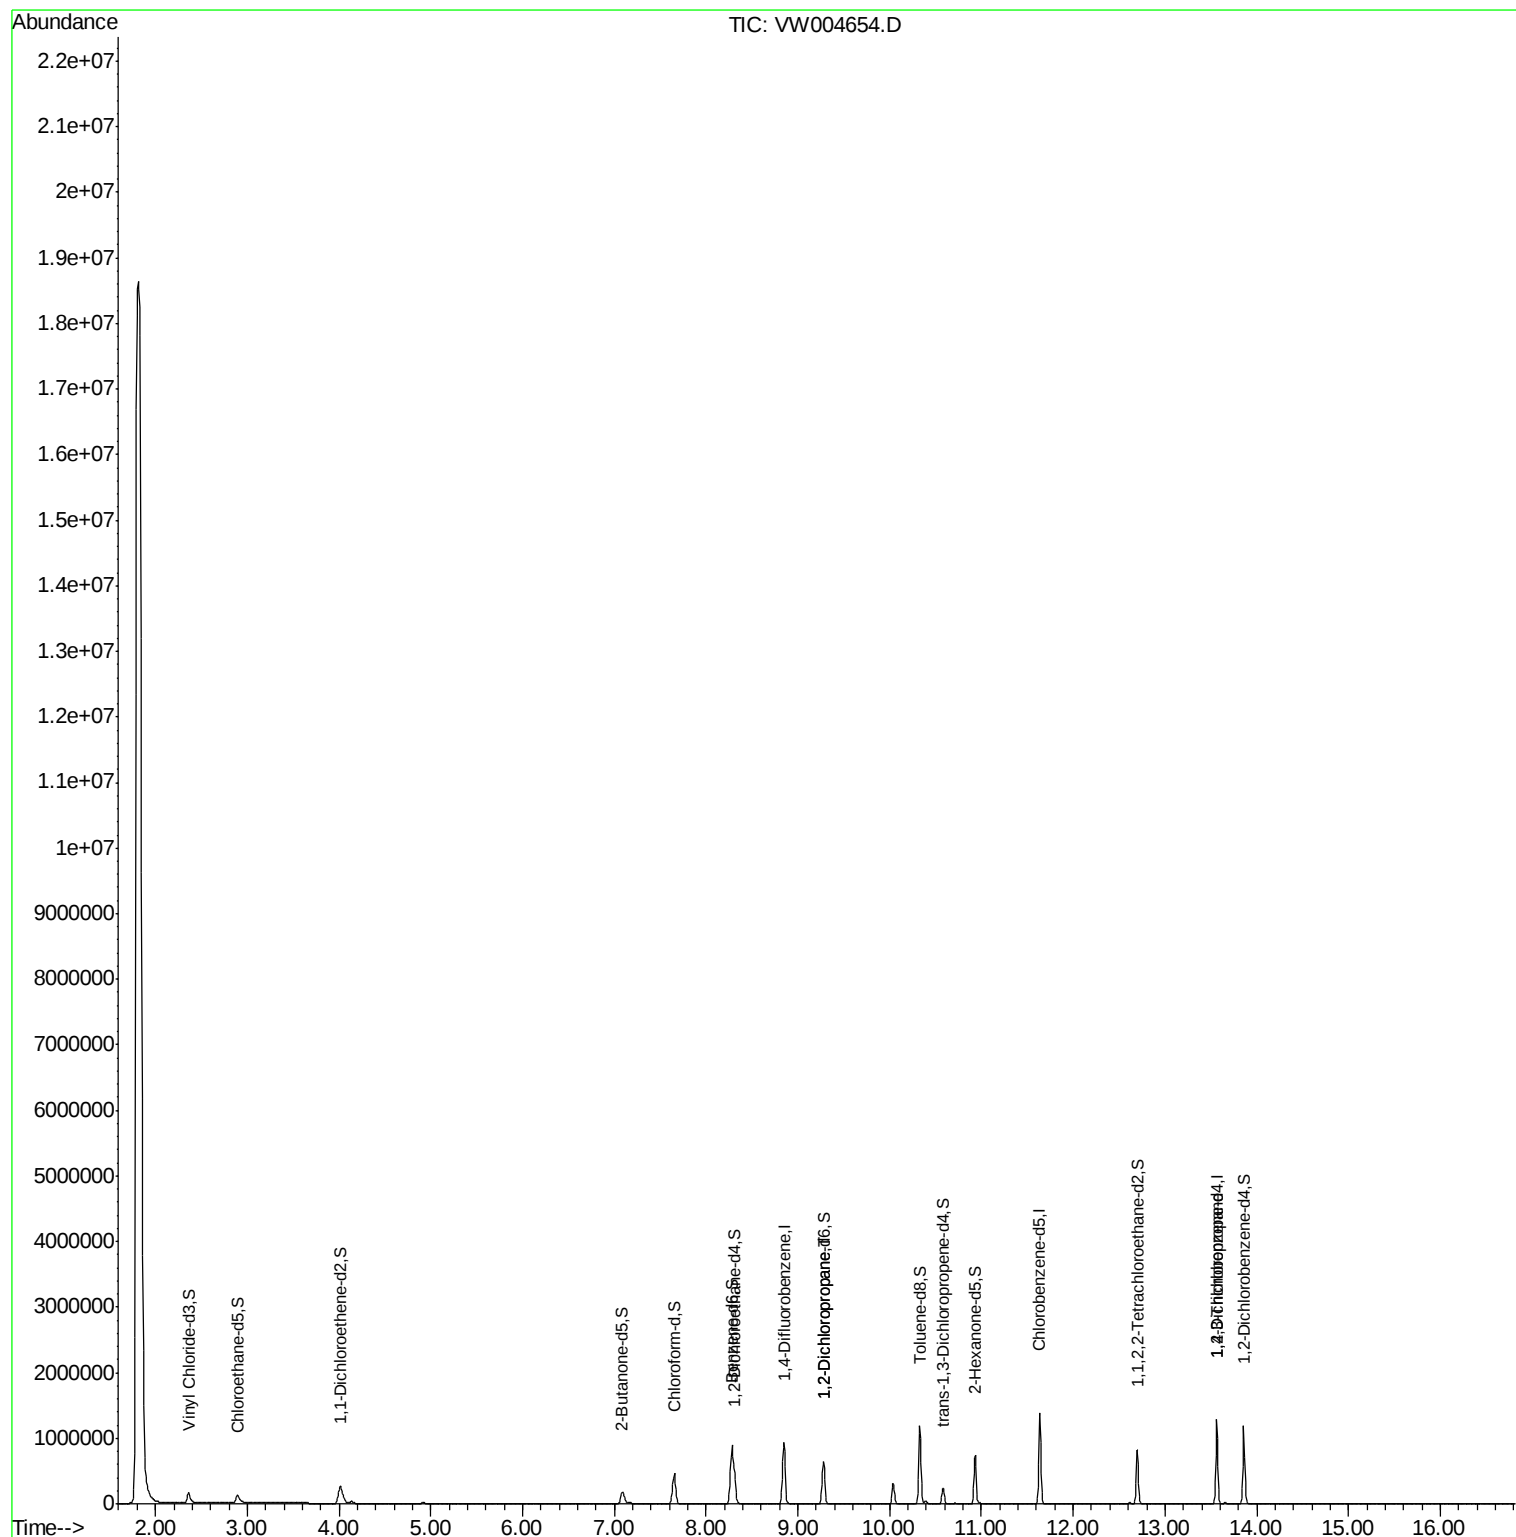

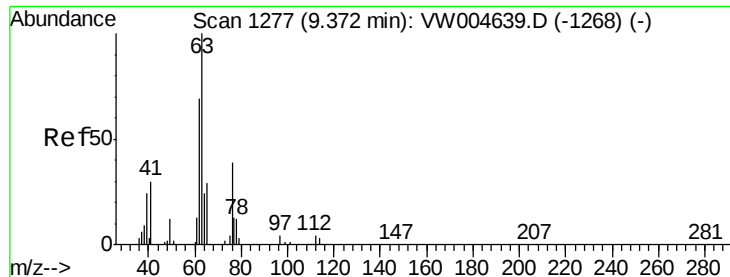

#40

1,2-Dichloropropane

Concen: 2.488 ug/L

RT: 9.27 min Scan# 1261

Delta R.T. -0.10 min

Lab File: VW004654.D

Acq: 13 Aug 2018 18:27

Instrument :

MSVOA_W

ClientSampleId :


GAB04

Tgt Ion: 63 Resp: 32696

Ion Ratio Lower Upper




63 100

112 0.5 3.0 4.6#

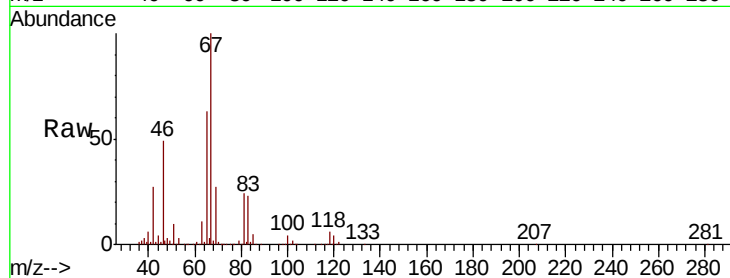

Abundance Ion 63.00 (62.70 to 63.70): VW

Ion 112.00 (111.70 to 112.70): V

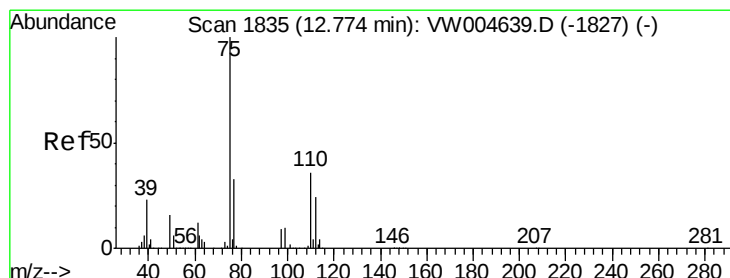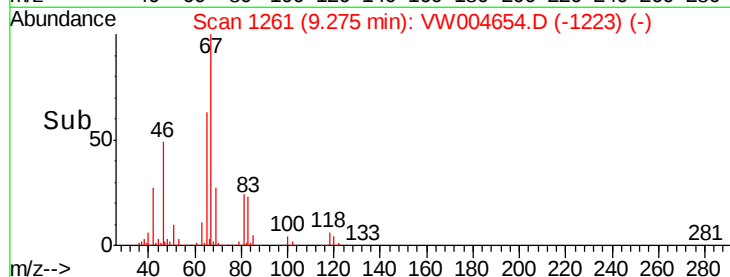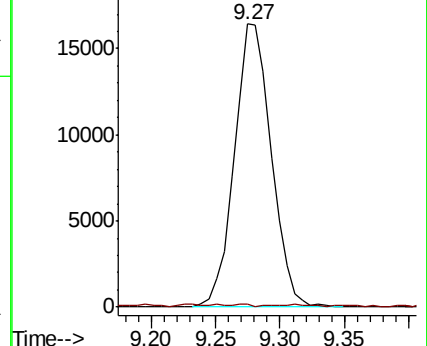

#59

1,2,3-Trichloropropane

Concen: 3.599 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW004654.D


Acq: 13 Aug 2018 18:27

Tgt Ion: 75 Resp: 39862

Ion Ratio Lower Upper

75 100

77 37.5 25.3 37.9

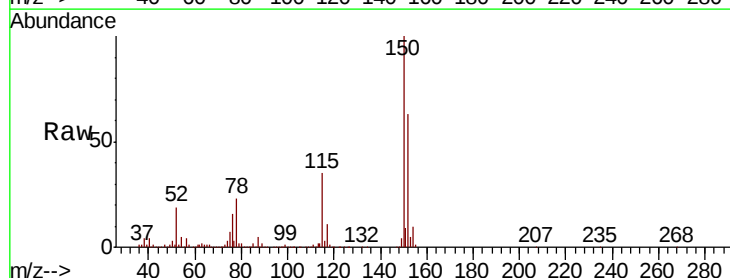

Abundance Ion 75.00 (74.70 to 75.70): VW

Ion 77.00 (76.70 to 77.70): VW

