

Data Path : \\74.0.250.170\terastorage\voasrv\HPCHEM1\MSVOA_W\Data\VW081418\
 Data File : VW004654.D
 Acq On : 13 Aug 2018 18:27
 Operator : SY/AP
 Sample : J4450-05
 Misc : 5.70G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 GAB04

Quant Time: Aug 14 06:39:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 14 01:20:10 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/14/2018 5:56:49 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	785231	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	804933	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	342523	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	228361	23.38	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.52%		
7) Chloroethane-d5	2.89	69	190886	23.23	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.92%		
10) 1,1-Dichloroethene-d2	4.01	63	336163	16.95	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.80%		
20) 2-Butanone-d5	7.09	46	299251	69.49	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	138.98%#		
24) Chloroform-d	7.65	84	494329	23.25	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.00%		
26) 1,2-Dichloroethane-d4	8.31	65	310546	26.20	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	104.80%		
29) Benzene-d6	8.28	84	943077	22.02	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.08%		
33) 1,2-Dichloropropane-d6	9.28	67	321607	22.98	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.92%		
37) Toluene-d8	10.33	98	796418	21.10	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.40%		
38) trans-1,3-Dichloropropene-	10.59	79	131942	22.93	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.72%		
39) 2-Hexanone-d5	10.93	63	241063	70.76	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	141.52%#		
48) 1,1,2,2-Tetrachloroethane-	12.70	84	426919	28.13	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	112.52%		
61) 1,2-Dichlorobenzene-d4	13.86	152	328534	25.54	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	102.16%		

Target Compounds

13) Acetone	4.14	43	47597m	12.757	ug/L	Qvalue 08/22/18 sy
-------------	------	----	--------	--------	------	--------------------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\terastorage\voasrv\HPCHEM1\MSVOA_W\Data\VW081418\
Data File : VW004654.D
Acq On : 13 Aug 2018 18:27
Operator : SY/AP
Sample : J4450-05
Misc : 5.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 06:39:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 14 01:20:10 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
GAB04

Manual Integrations
APPROVED

MMDadoda
8/14/2018 5:56:49 PM

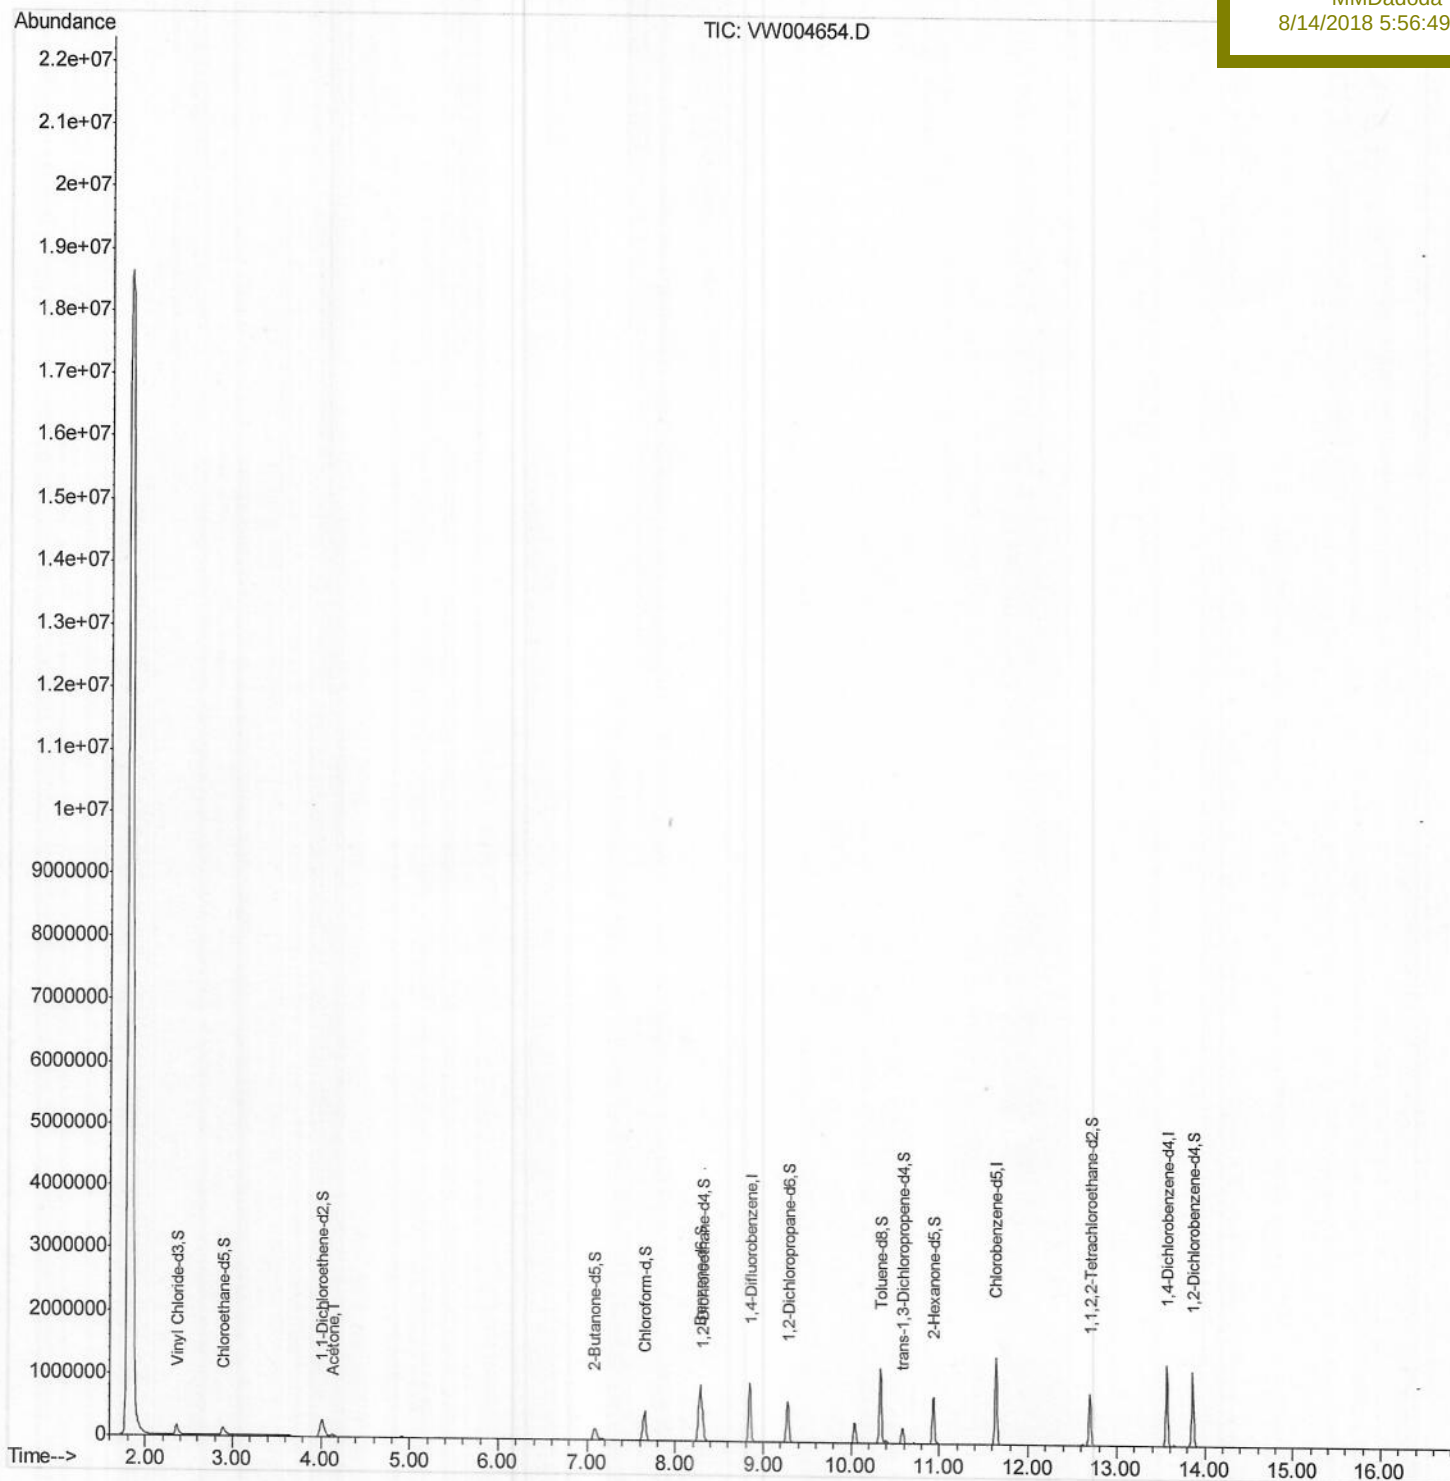




Data Path : \\74.0.250.170\terastorage\voasrv\HPCHEM1\MSVOA_W\Data\VW081418\
Data File : VW004654.D
Acq On : 13 Aug 2018 18:27
Operator : SY/AP
Sample : J4450-05
Misc : 5.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 02:25:22 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 14 01:20:10 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
GAB04

Manual Integrations
APPROVED

MMDadoda
8/14/2018 5:56:49 PM

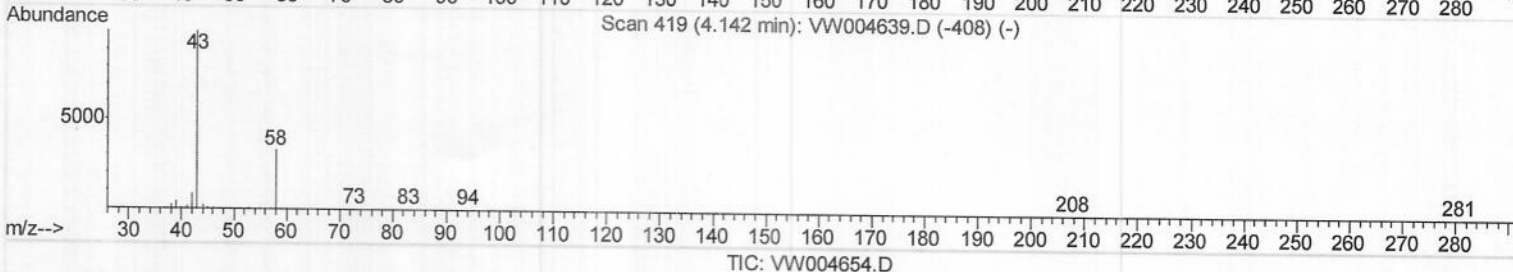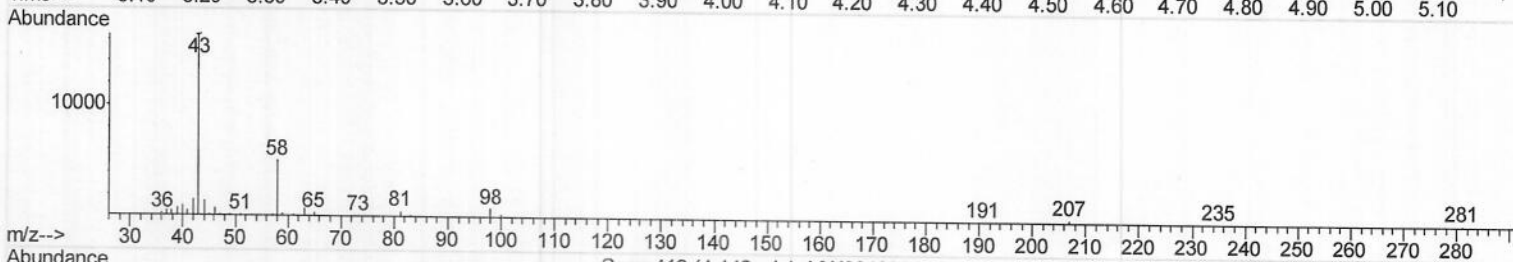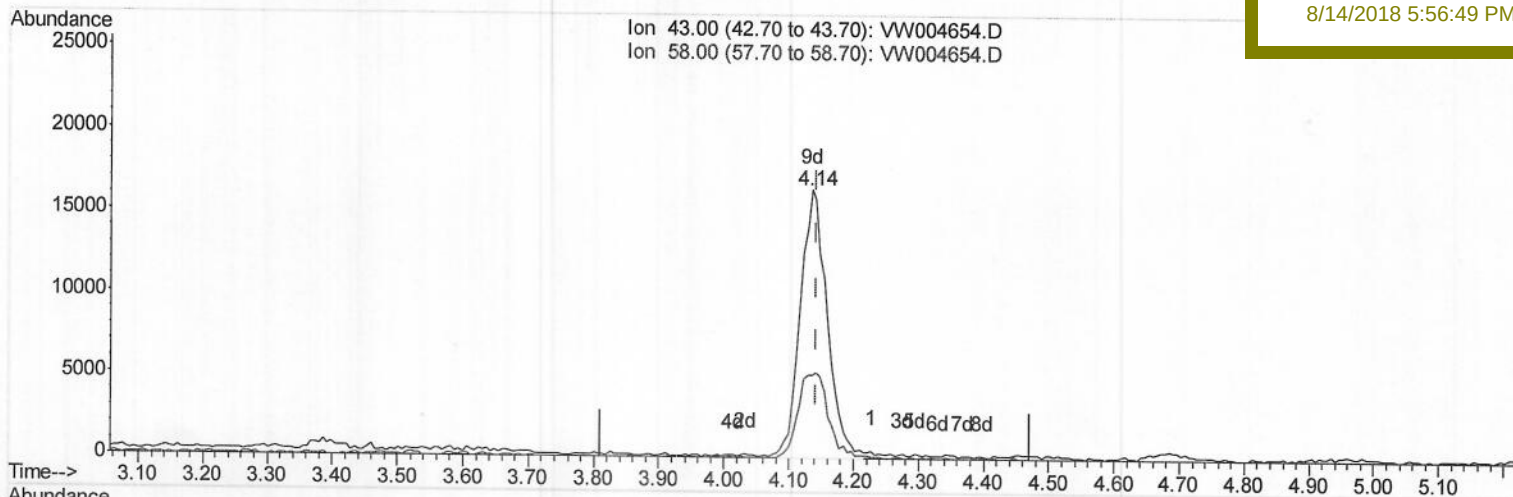

(13) Acetone (T)

4.136min (-0.006) 12.76ug/L m 208/22/18 sy

response 47597

Ion	Exp%	Act%
43.00	100	100
58.00	33.20	0.17
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : \\74.0.250.170\terastorage\voasrv\HPCHEM1\MSVOA_W\Data\VW081418\
 Data File : VW004654.D
 Acq On : 13 Aug 2018 18:27
 Operator : SY/AP
 Sample : J4450-05
 Misc : 5.70G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 02:25:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM080218S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 14 01:20:10 2018
 Response via : Initial Calibration

Instrument :
 MSVOA_W
 ClientSampled :
 GAB04

Manual Integrations
 APPROVED

MMDadoda
 8/14/2018 5:56:49 PM

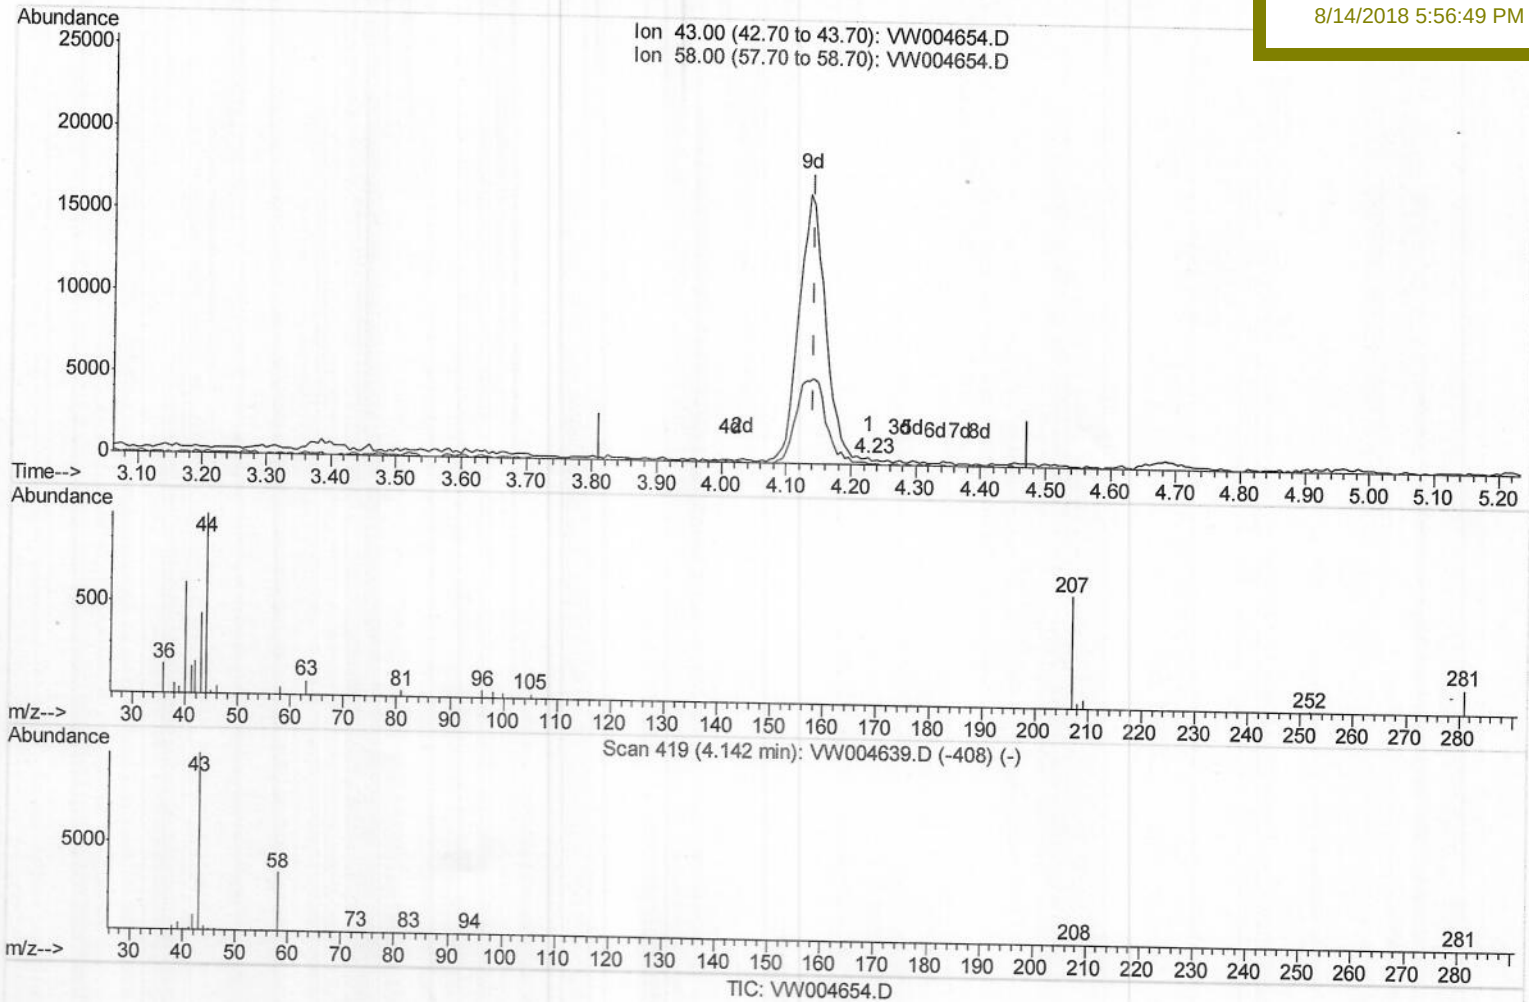

(13) Acetone (T)

4.227min (+0.085) 0.08ug/L

response 285

Ion	Exp%	Act%
43.00	100	100
58.00	33.20	28.42
0.00	0.00	0.00
0.00	0.00	0.00