




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
 Data File : VW026723.D
 Acq On : 14 Aug 2023 09:53
 Operator : SY/MD
 Sample : VW0814SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK548

Manual IntegrationsAPPROVED

Quant Time: Aug 14 23:24:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 14 23:23:26 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/15/2023
 Supervised By :Mahesh Dadoda 08/15/2023

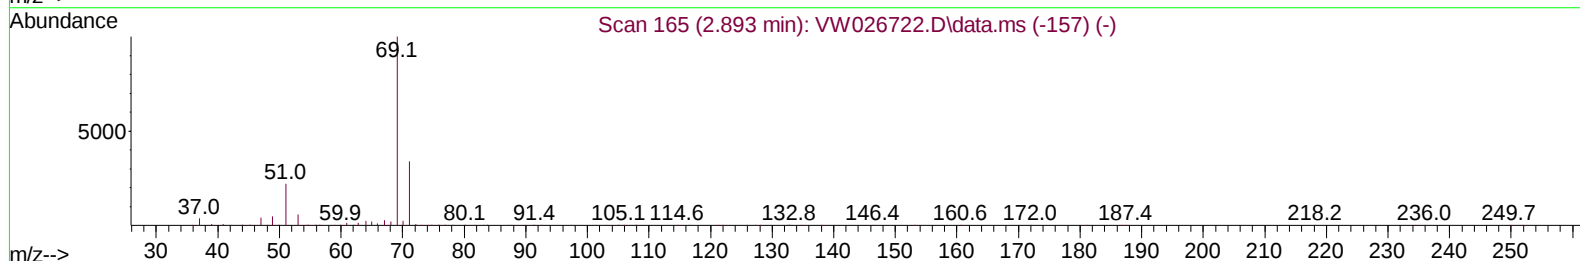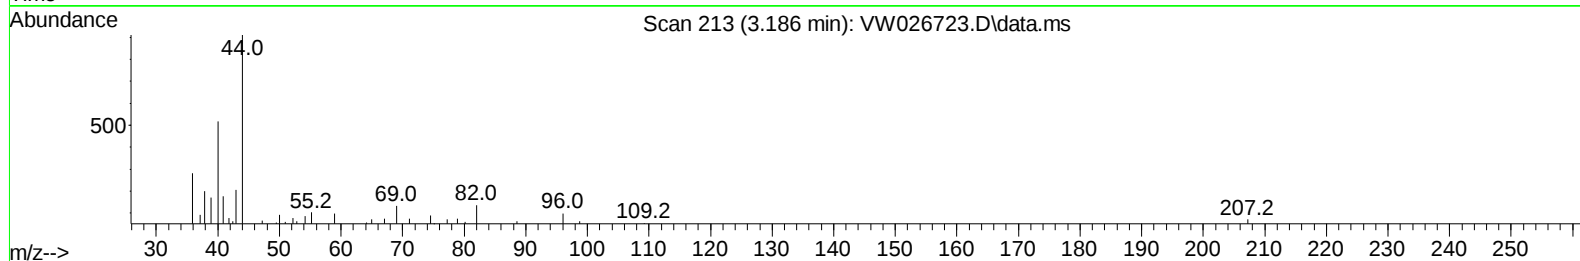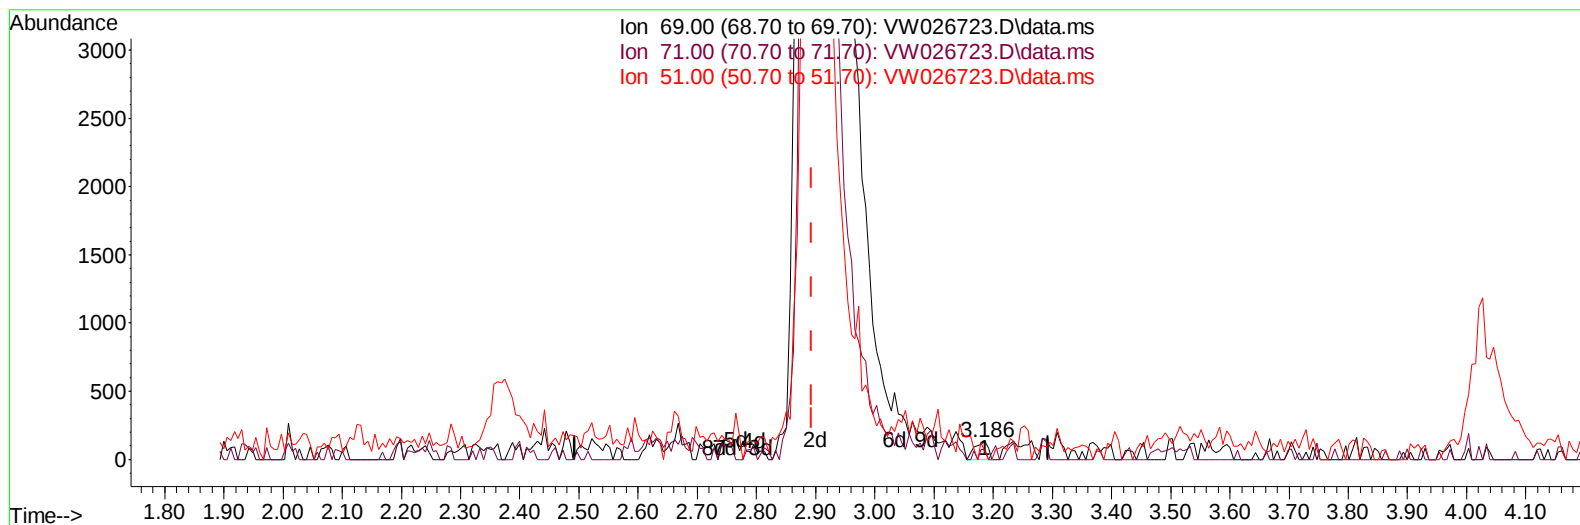

TIC: VW026723.D\data.ms

(7) Chloroethane-d5 (S)

3.186min (+ 0.293) 0.03 ug/L

response 210

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	25.71
51.00	28.30	32.38
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
 Data File : VW026723.D
 Acq On : 14 Aug 2023 09:53
 Operator : SY/MD
 Sample : VW0814SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK548

Manual IntegrationsAPPROVED

Quant Time: Aug 14 23:24:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 14 23:23:26 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/15/2023
 Supervised By :Mahesh Dadoda 08/15/2023

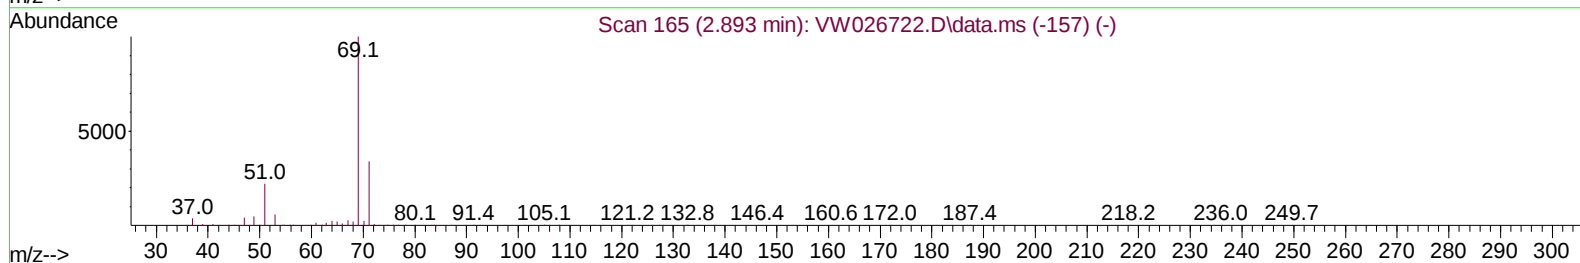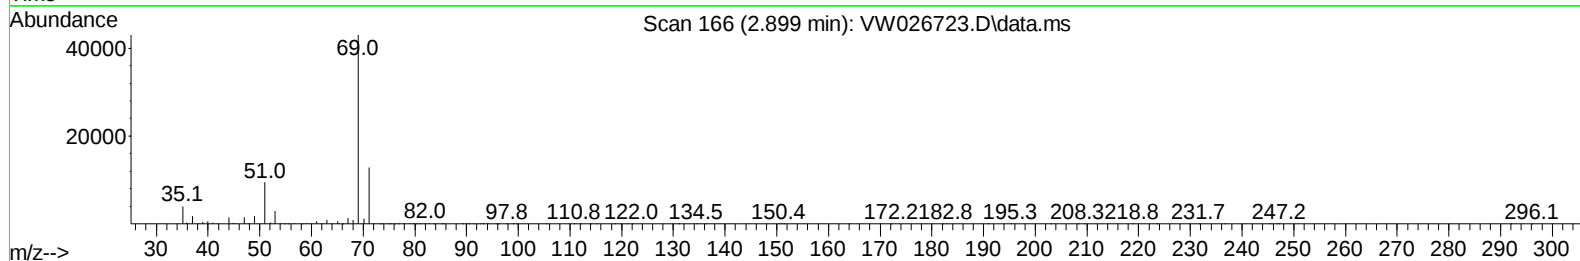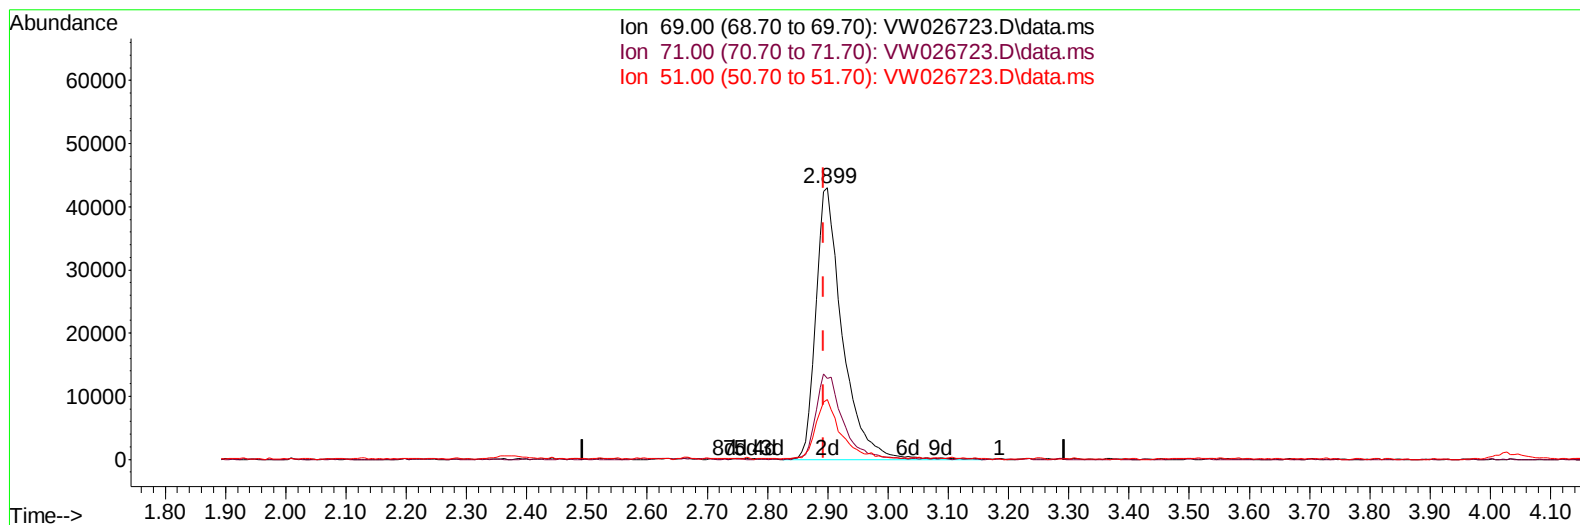

TIC: VW026723.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (+ 0.006) 20.45 ug/L m

response 131744

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	0.04#
51.00	28.30	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
 Data File : VW026723.D
 Acq On : 14 Aug 2023 09:53
 Operator : SY/MD
 Sample : VW0814SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK548

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/15/2023
 Supervised By :Mahesh Dadoda 08/15/2023

Quant Time: Aug 14 23:24:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 14 23:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		526930	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		515372	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		239402	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		158541	18.303	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.200%	
7) Chloroethane-d5	2.899	69		131744m	20.453	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.800%	
11) 1,1-Dichloroethene-d2	4.021	65		96637	22.683	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.720%	
21) 2-Butanone-d5	7.075	46		111408	44.748	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.500%	
24) Chloroform-d	7.648	84		435188	24.607	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.440%	
26) 1,2-Dichloroethane-d4	8.307	65		248600	25.472	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.880%	
32) Benzene-d6	8.276	84		875740	24.655	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.640%	
36) 1,2-Dichloropropane-d6	9.270	67		280753	25.376	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.520%	
41) Toluene-d8	10.325	98		771970	25.319	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.280%	
43) trans-1,3-Dichloroprop...	10.575	79		109880	24.054	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.200%	
47) 2-Hexanone-d5	10.922	63		52016	44.743	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.480%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		216459	24.774	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.080%	
66) 1,2-Dichlorobenzene-d4	13.849	152		241318	28.162	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	112.640%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
Data File : VW026723.D
Acq On : 14 Aug 2023 09:53
Operator : SY/MD
Sample : VW0814SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK548

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/15/2023
Supervised By :Mahesh Dadoda 08/15/2023

Quant Time: Aug 14 23:24:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 14 23:23:26 2023
Response via : Initial Calibration

