




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
 Data File : VW026739.D
 Acq On : 14 Aug 2023 16:30
 Operator : SY/MD
 Sample : 03968-36
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48Z4

Manual IntegrationsAPPROVED

Quant Time: Aug 14 23:28:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 14 23:23:26 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/15/2023
 Supervised By :Mahesh Dadoda 08/15/2023

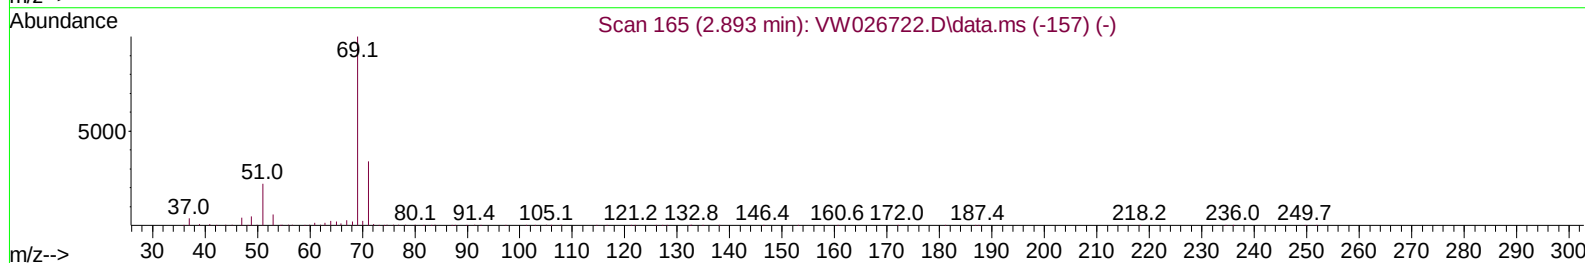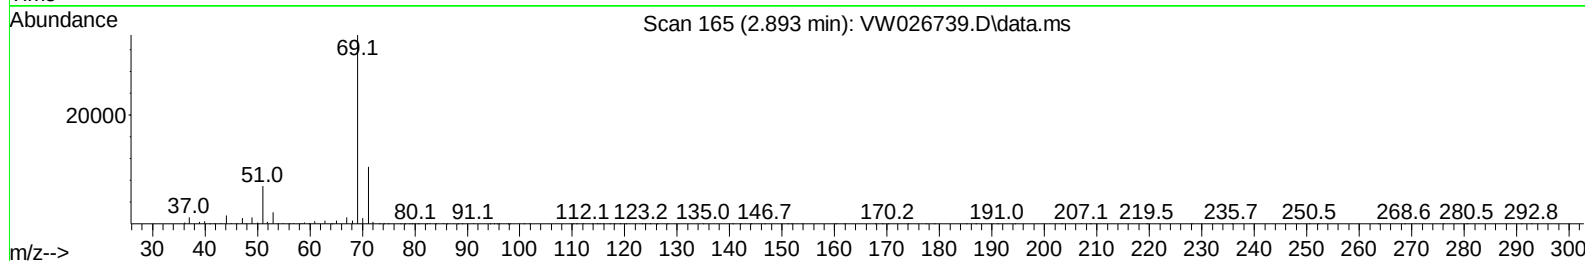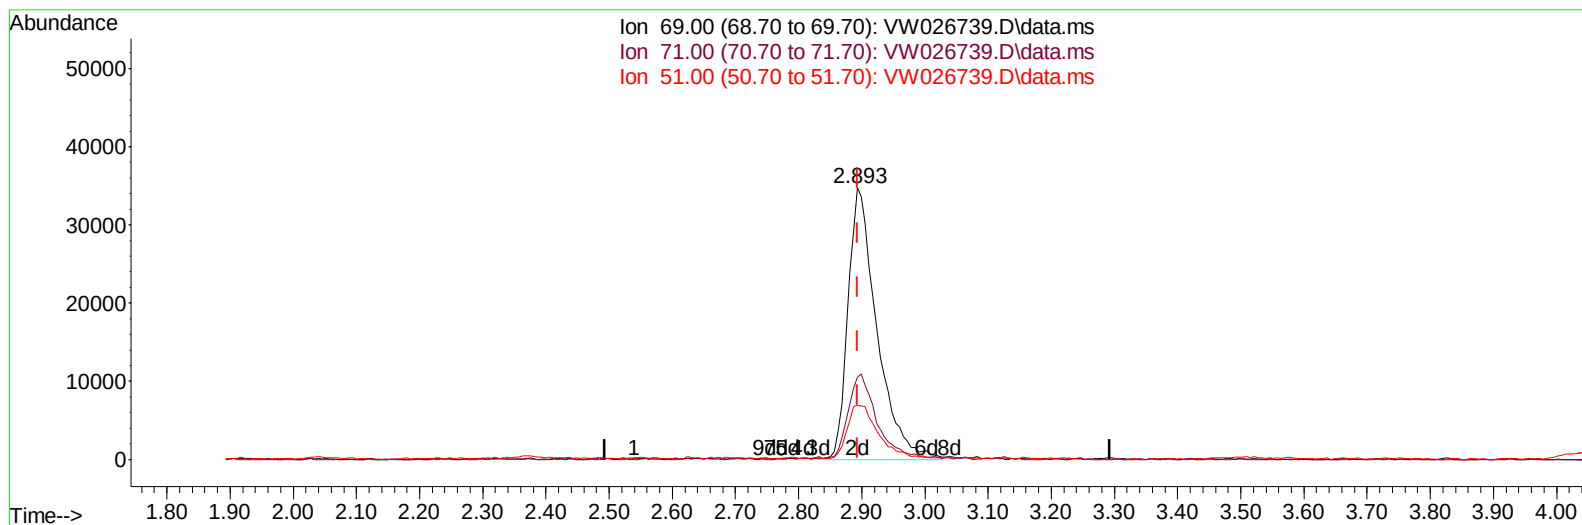

TIC: VW026739.D\data.ms

(7) Chloroethane-d5 (S)

2.893min (0.000) 18.26 ug/L m

response 110752

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	0.04#
51.00	28.30	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
 Data File : VW026739.D
 Acq On : 14 Aug 2023 16:30
 Operator : SY/MD
 Sample : 03968-36
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48Z4

Manual IntegrationsAPPROVED

Quant Time: Aug 14 23:28:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 14 23:23:26 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/15/2023
 Supervised By :Mahesh Dadoda 08/15/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	496096	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	502351	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	234704	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	128266	15.728	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	62.920%	
7) Chloroethane-d5	2.893	69	110752m	18.263	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	73.040%	
11) 1,1-Dichloroethene-d2	4.021	65	81962	20.434	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	81.720%	
21) 2-Butanone-d5	7.075	46	124838	53.259	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	106.520%	
24) Chloroform-d	7.648	84	392769	23.589	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	94.360%	
26) 1,2-Dichloroethane-d4	8.307	65	236567	25.746	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.000%	
32) Benzene-d6	8.276	84	784673	22.664	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.640%	
36) 1,2-Dichloropropane-d6	9.270	67	258869	24.004	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	96.000%	
41) Toluene-d8	10.325	98	660524	22.225	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	88.920%	
43) trans-1,3-Dichloroprop...	10.581	79	99936	22.444	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.760%	
47) 2-Hexanone-d5	10.922	63	57968	51.155	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	102.320%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	226895	26.641	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	106.560%	
66) 1,2-Dichlorobenzene-d4	13.848	152	212097	25.248	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	101.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
Data File : VW026739.D
Acq On : 14 Aug 2023 16:30
Operator : SY/MD
Sample : 03968-36
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A48Z4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/15/2023
Supervised By :Mahesh Dadoda 08/15/2023

Quant Time: Aug 14 23:28:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 14 23:23:26 2023
Response via : Initial Calibration

