

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
 Data File : VW026731.D
 Acq On : 14 Aug 2023 13:17
 Operator : SY/MD
 Sample : 03968-27
 Misc : 4.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A48P4

Quant Time: Aug 14 23:26:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 14 23:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	666093	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	629570	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	273387	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	155647	14.215	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.840%
7) Chloroethane-d5	2.893	69	127972	15.717	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.880%
11) 1,1-Dichloroethene-d2	4.015	65	95162	17.670	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.680%
21) 2-Butanone-d5	7.082	46	155152	49.299	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.600%
24) Chloroform-d	7.648	84	469455	20.999	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.000%
26) 1,2-Dichloroethane-d4	8.307	65	293771	23.812	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.240%
32) Benzene-d6	8.276	84	941392	21.696	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.800%
36) 1,2-Dichloropropane-d6	9.270	67	312030	23.087	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.360%
41) Toluene-d8	10.325	98	786731	21.123	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.480%
43) trans-1,3-Dichloroprop...	10.575	79	118891	21.305	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.240%
47) 2-Hexanone-d5	10.922	63	74365	52.364	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.720%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	275313	25.794	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.160%
66) 1,2-Dichlorobenzene-d4	13.849	152	222053	22.693	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.760%
Target Compounds						
13) Acetone	4.125	43	10896	3.482	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081423\
Data File : VW026731.D
Acq On : 14 Aug 2023 13:17
Operator : SY/MD
Sample : 03968-27
Misc : 4.85g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A48P4

Quant Time: Aug 14 23:26:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 14 23:23:26 2023
Response via : Initial Calibration

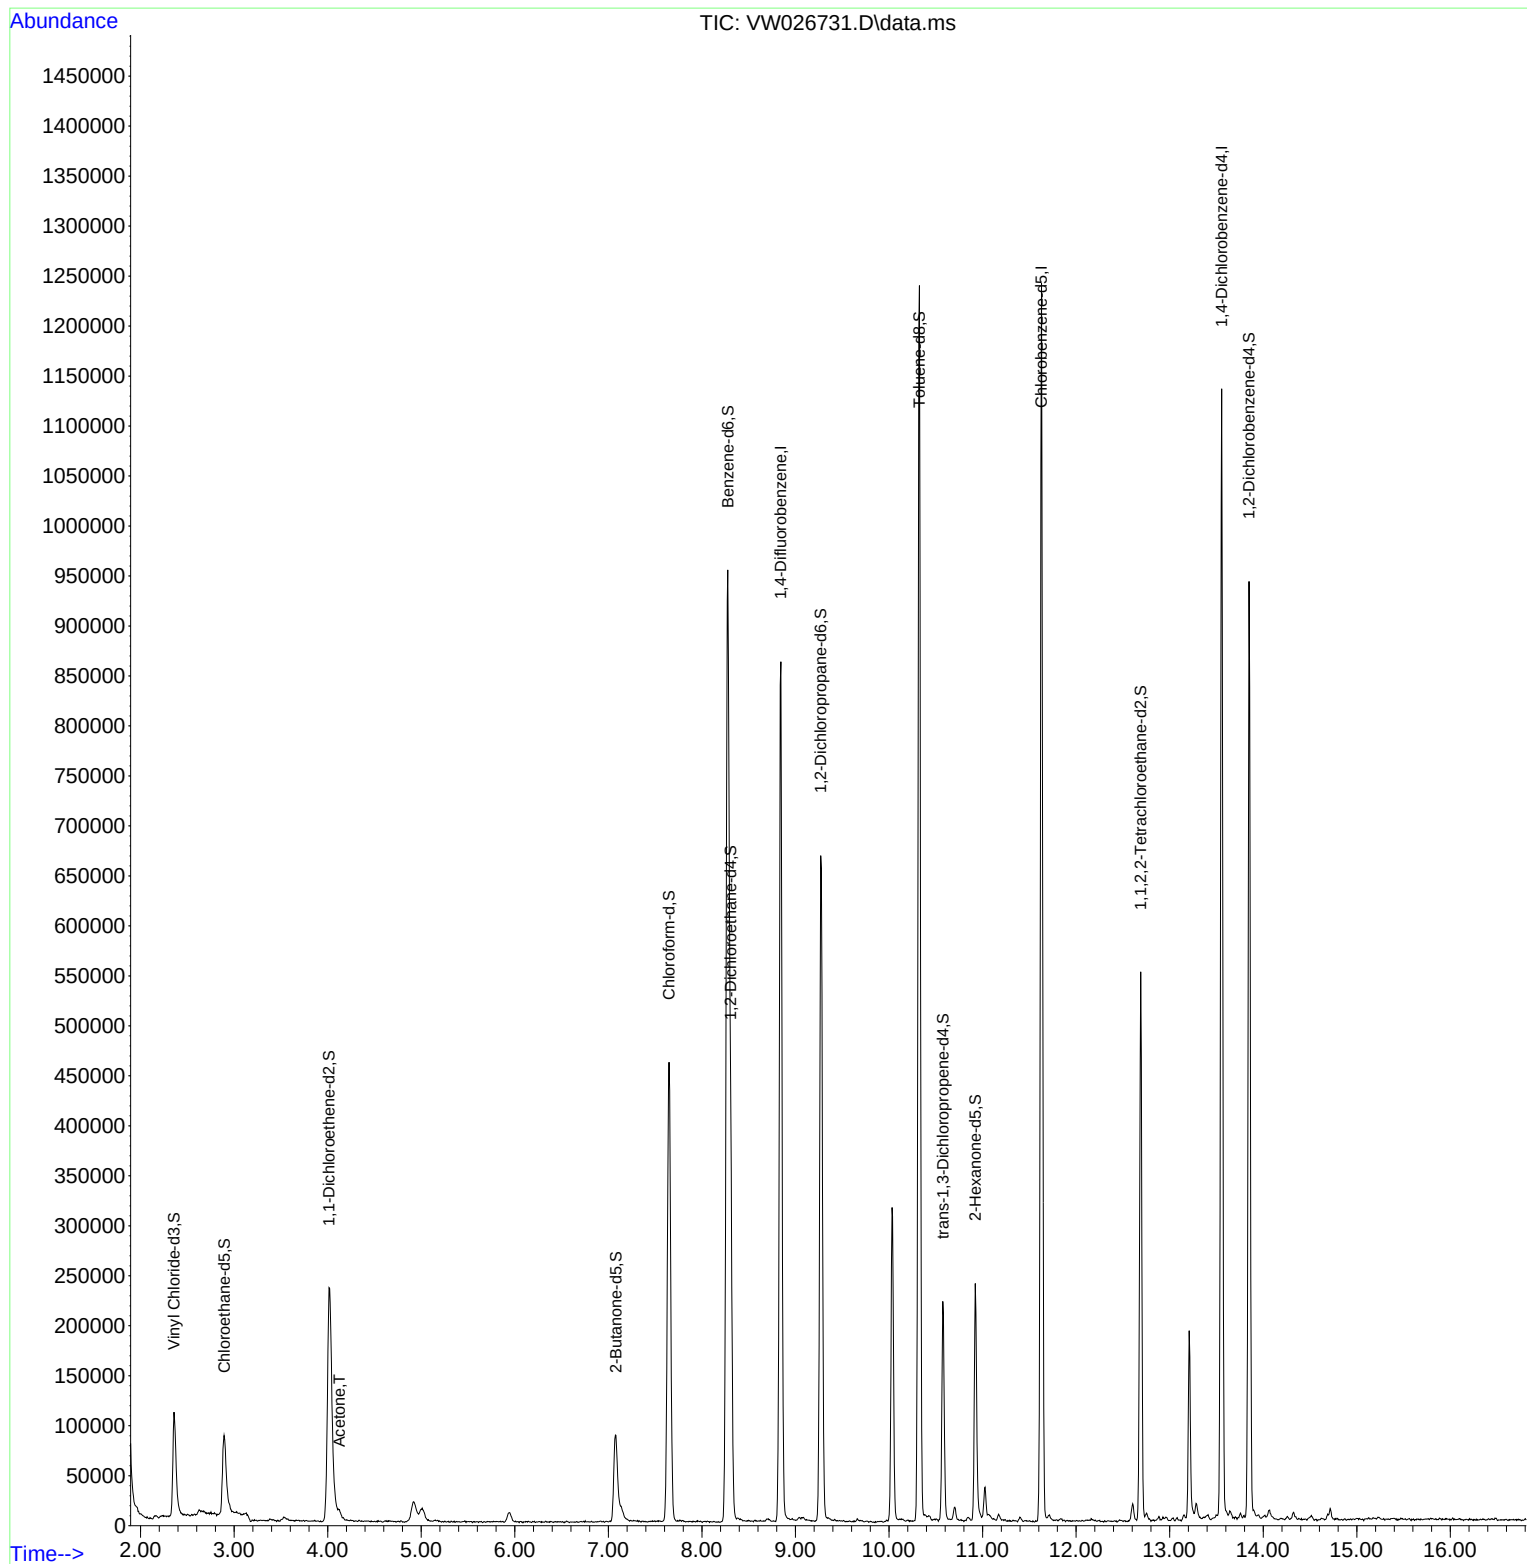

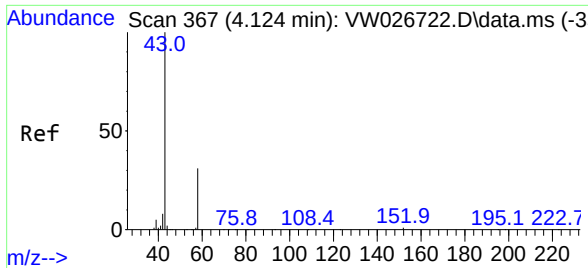

#13
 Acetone
 Concen: 3.482 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW026731.D
 Acq: 14 Aug 2023 13:17

Instrument :
 MSVOA_W
 ClientSampleId :
 A48P4

Tgt Ion: 43 Resp: 10896
 Ion Ratio Lower Upper
 43 100
 58 28.1 0.0 57.4

