

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081524\
 Data File : VW029913.D
 Acq On : 15 Aug 2024 18:20
 Operator : SY/MD
 Sample : P3504-06
 Misc : 3.99g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 16 01:16:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 16 01:14:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	351068	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	323589	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	133443	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	77386	15.527	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	62.120%		
7) Chloroethane-d5	2.899	69	68074	19.131	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	76.520%		
11) 1,1-Dichloroethene-d2	4.021	65	32948	14.482	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.920%		
21) 2-Butanone-d5	7.069	46	39051	28.587	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	57.180%		
24) Chloroform-d	7.654	84	170226	18.731	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	74.920%		
26) 1,2-Dichloroethane-d4	8.307	65	95669	18.482	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	73.920%		
32) Benzene-d6	8.276	84	312648	17.882	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	71.520%		
36) 1,2-Dichloropropane-d6	9.270	67	99940	17.901	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	71.600%		
41) Toluene-d8	10.319	98	284324	18.289	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	73.160%		
43) trans-1,3-Dichloroprop...	10.575	79	38995	17.262	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	69.040%		
47) 2-Hexanone-d5	10.922	63	30957	33.629	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	67.260%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	81546	19.672	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	78.680%		
66) 1,2-Dichlorobenzene-d4	13.848	152	93650	22.602	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.400%		
Target Compounds						Qvalue
13) Acetone	4.118	43	10741	6.327	ug/L	96
39) cis-1,3-Dichloropropene	10.032	75	3166	0.358	ug/L #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081524\
Data File : VW029913.D
Acq On : 15 Aug 2024 18:20
Operator : SY/MD
Sample : P3504-06
Misc : 3.99g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Aug 16 01:16:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 16 01:14:23 2024
Response via : Initial Calibration

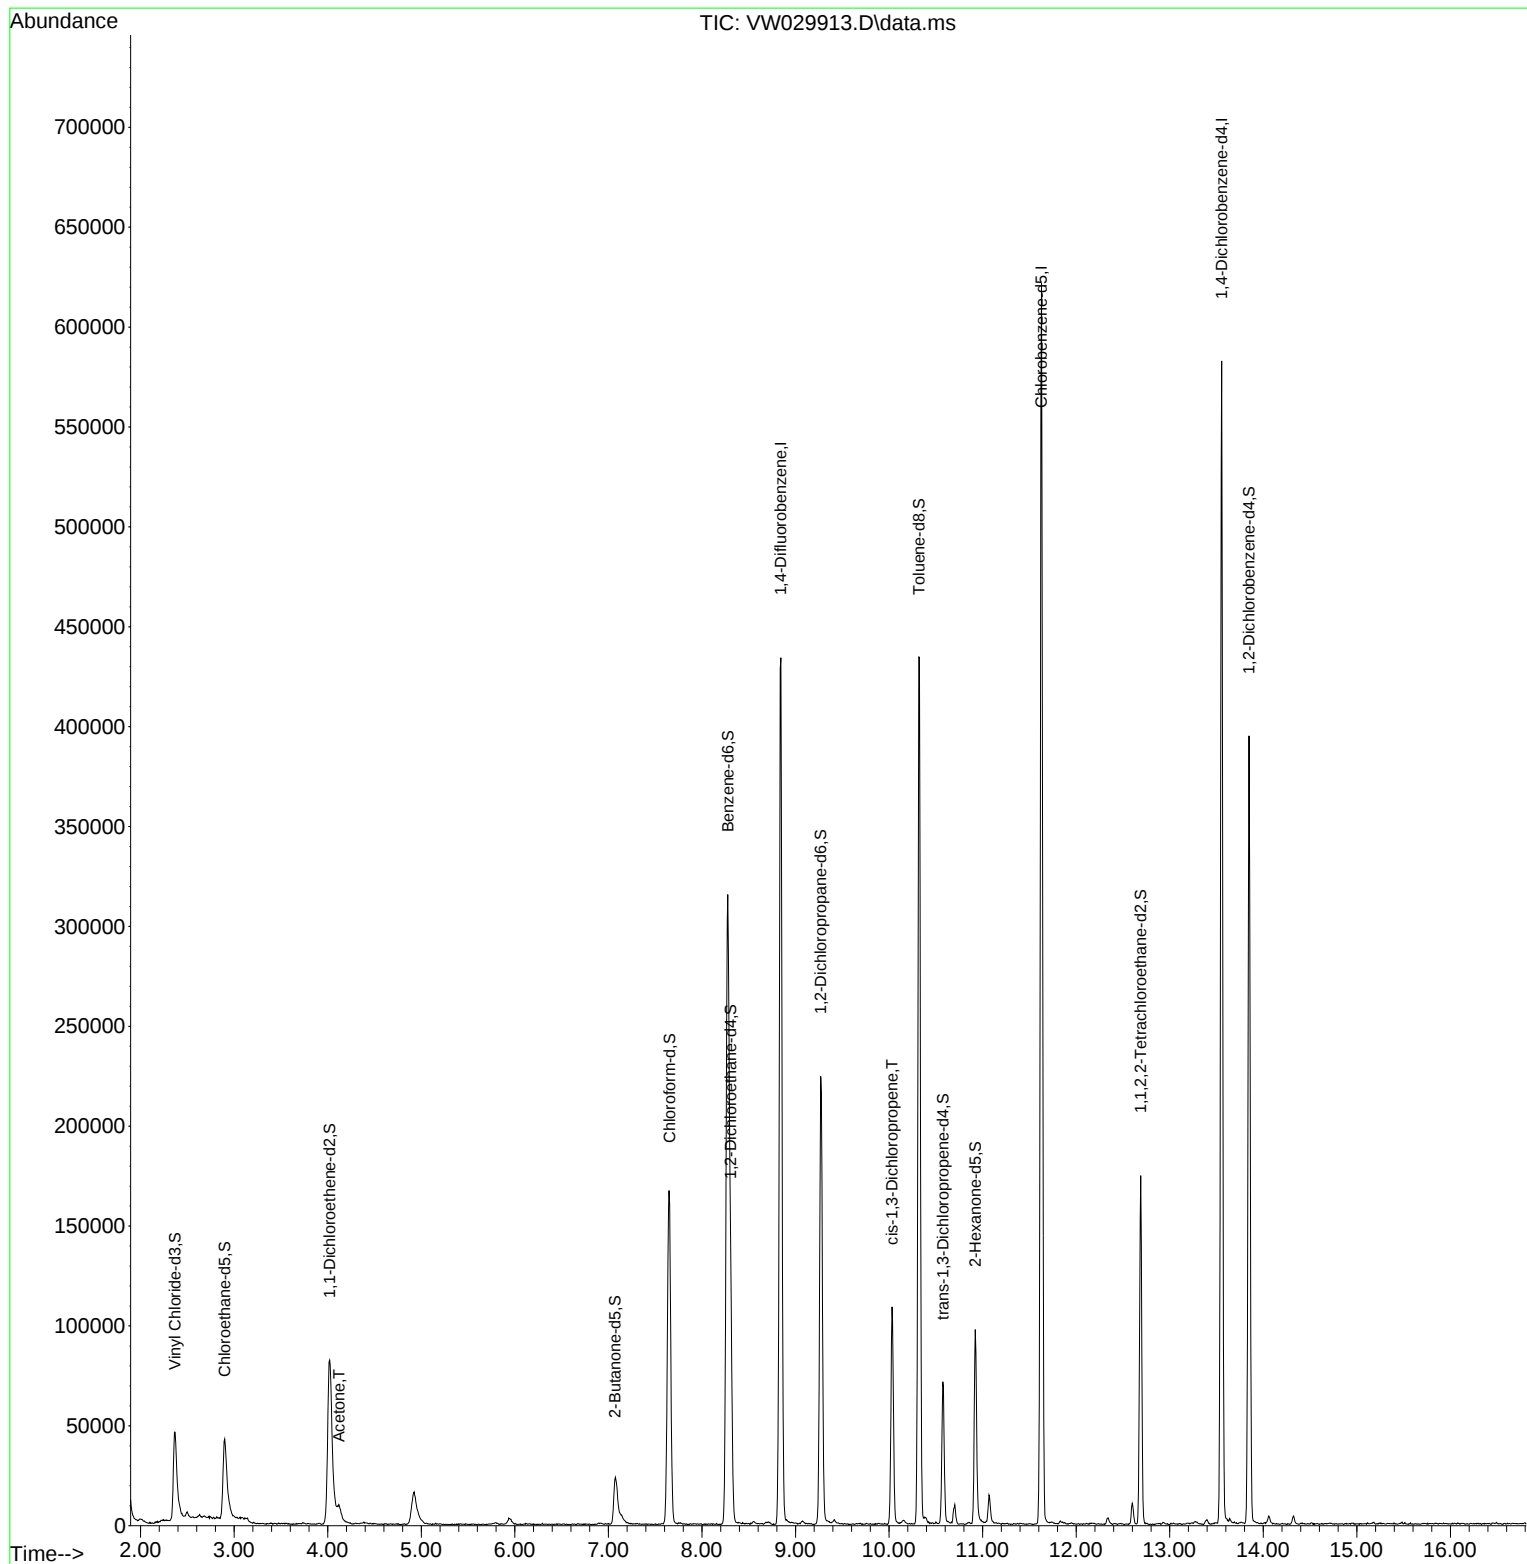



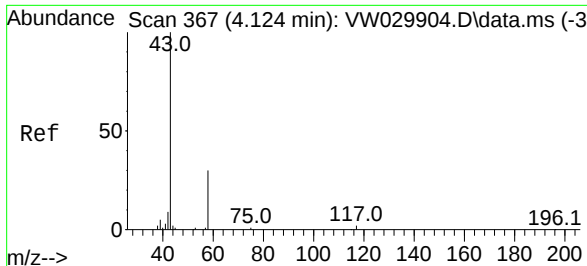


#13
Acetone
Concen: 6.327 ug/L
RT: 4.118 min Scan# 30
Delta R.T. -0.006 min
Lab File: VW029913.D
Acq: 15 Aug 2024 18:20

Instrument :
MSVOA_W
ClientSampleId :

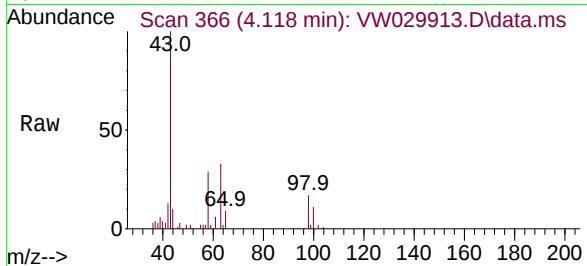

Tgt Ion: 43 Resp: 10741
Ion Ratio Lower Upper
43 100
58 30.7 0.0 57.6

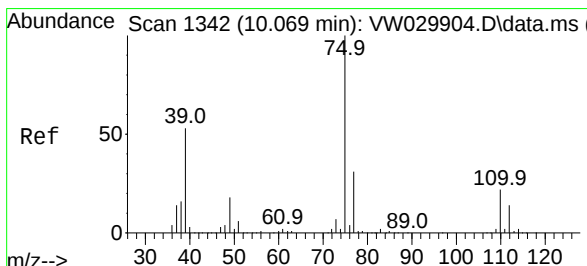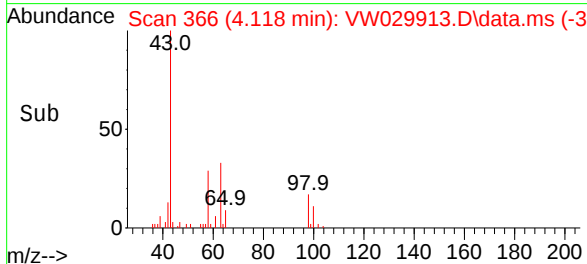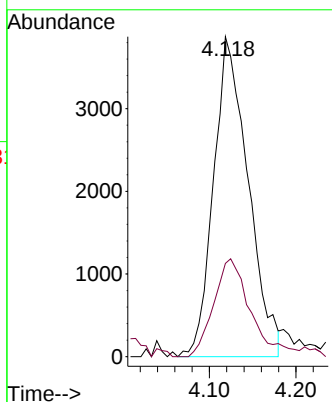

#39
cis-1,3-Dichloropropene
Concen: 0.358 ug/L
RT: 10.032 min Scan# 1336
Delta R.T. -0.037 min
Lab File: VW029913.D
Acq: 15 Aug 2024 18:20

Tgt Ion: 75 Resp: 3166
Ion Ratio Lower Upper
75 100
77 42.9 20.8 38.6#

