




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081524\
 Data File : VW029909.D
 Acq On : 15 Aug 2024 16:43
 Operator : SY/MD
 Sample : P3626-04
 Misc : 3.36g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYD3

Manual IntegrationsAPPROVED

Quant Time: Aug 16 02:07:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 16 01:14:23 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/16/2024
 Supervised By :Mahesh Dadoda 08/21/2024

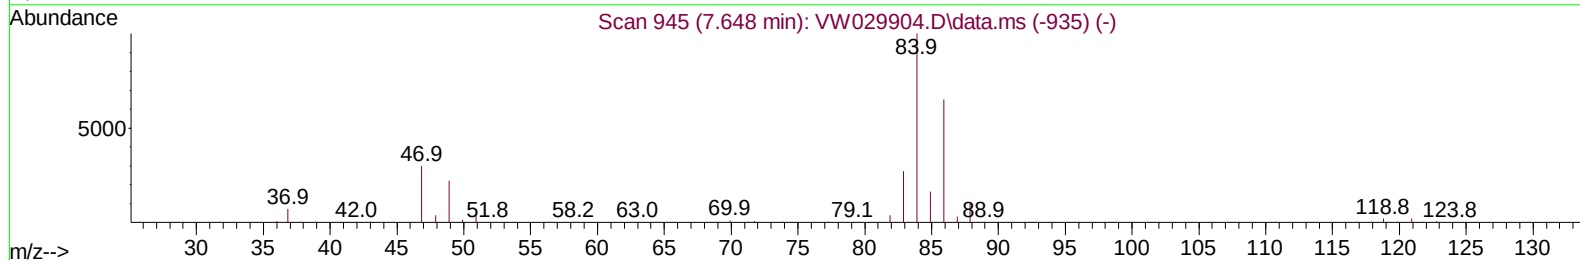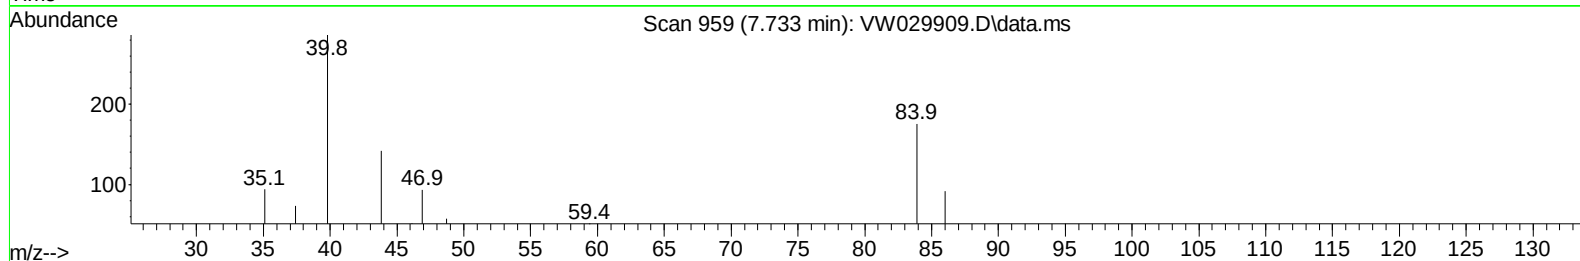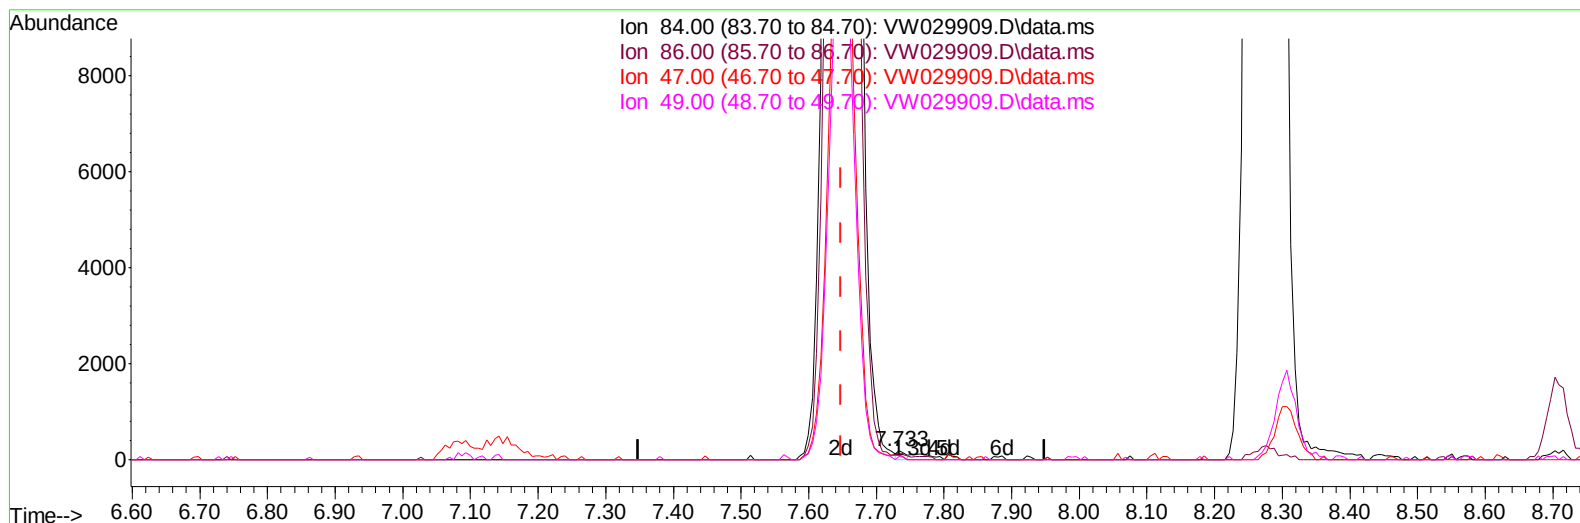

TIC: VW029909.D\data.ms

(24) Chloroform-d (S)

7.733min (+ 0.085) 0.02 ug/L

response 145

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.90	44.14
47.00	57.60	58.62
49.00	31.80	27.59




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081524\
Data File : VW029909.D
Acq On : 15 Aug 2024 16:43
Operator : SY/MD
Sample : P3626-04
Misc : 3.36g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYD3

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:15:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 16 01:14:23 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/16/2024
Supervised By :Mahesh Dadoda 08/21/2024

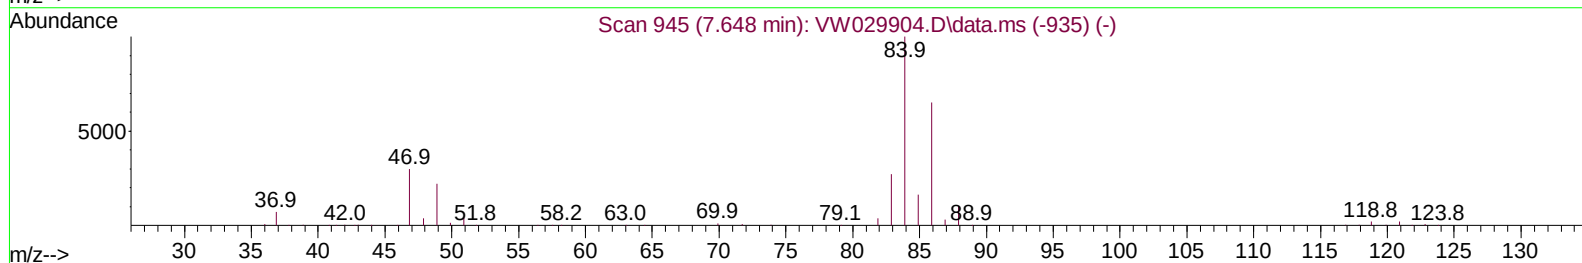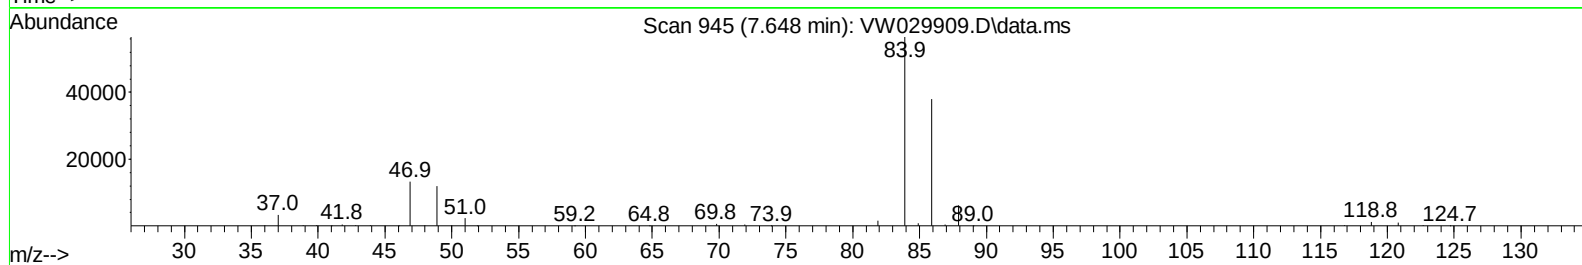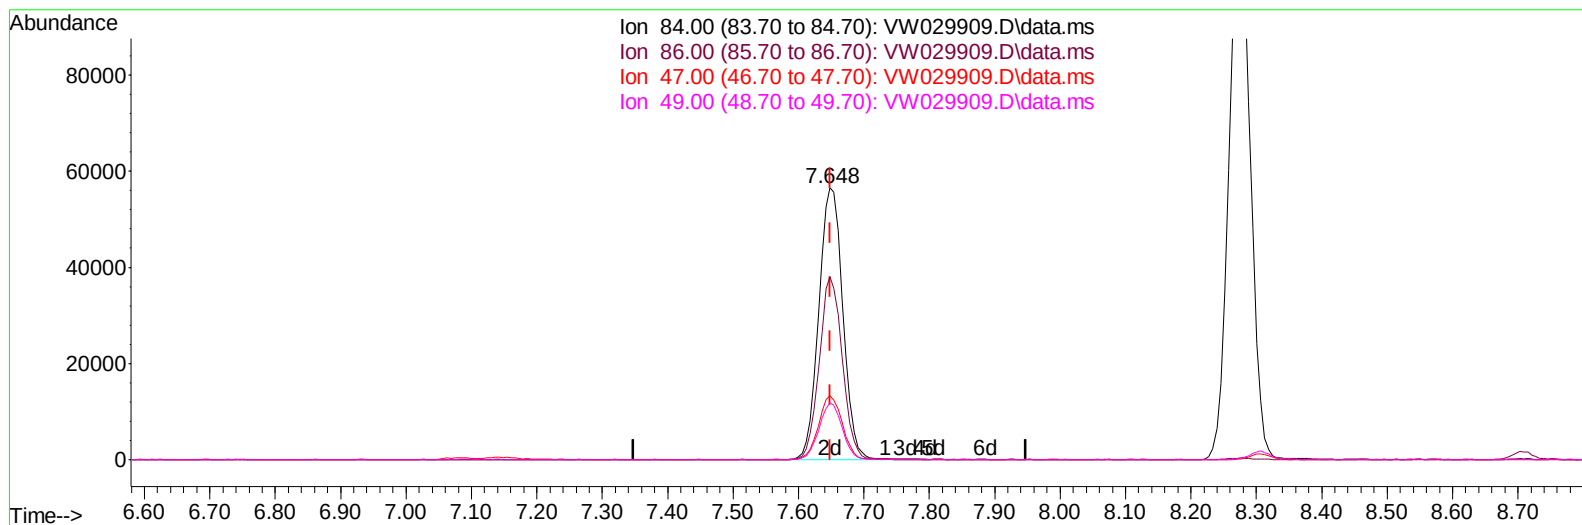

TIC: VW029909.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 18.93 ug/L m

response 144366

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.90	0.04#
47.00	57.60	0.06#
49.00	31.80	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081524\
 Data File : VW029909.D
 Acq On : 15 Aug 2024 16:43
 Operator : SY/MD
 Sample : P3626-04
 Misc : 3.36g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYD3

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:15:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 16 01:14:23 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/16/2024
 Supervised By :Mahesh Dadoda 08/21/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		294554	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		238810	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		86266	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		75272	18.000	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	72.000%		
7) Chloroethane-d5	2.899	69		63507	21.272	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	85.080%		
11) 1,1-Dichloroethene-d2	4.027	65		29425	15.415	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	61.640%		
21) 2-Butanone-d5	7.087	46		39389	34.367	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135		Recovery =	68.740%		
24) Chloroform-d	7.648	84		144366m	18.933	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	75.720%		
26) 1,2-Dichloroethane-d4	8.307	65		83656	19.262	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	77.040%		
32) Benzene-d6	8.276	84		259782	20.133	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	80.520%		
36) 1,2-Dichloropropane-d6	9.276	67		83790	20.337	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	81.360%		
41) Toluene-d8	10.324	98		225256	19.633	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	78.520%		
43) trans-1,3-Dichloroprop...	10.574	79		32512	19.501	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	78.000%		
47) 2-Hexanone-d5	10.922	63		29694	43.708	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	87.420%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		67334	22.010	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	88.040%		
66) 1,2-Dichlorobenzene-d4	13.848	152		51183	19.108	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	76.440%		
Target Compounds							
13) Acetone	4.137	43		39732	27.895	ug/L	97
42) Toluene	10.385	91		5816	0.348	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081524\
Data File : VW029909.D
Acq On : 15 Aug 2024 16:43
Operator : SY/MD
Sample : P3626-04
Misc : 3.36g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCYD3

Manual IntegrationsAPPROVED

Quant Time: Aug 16 01:15:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 16 01:14:23 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/16/2024
Supervised By :Mahesh Dadoda 08/21/2024

