

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081524\
 Data File : VW029906.D
 Acq On : 15 Aug 2024 15:31
 Operator : SY/MD
 Sample : P3626-01
 Misc : 4.58g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYB5

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 08/16/2024
 Supervised By :Mahesh Dadoda 08/21/2024

Quant Time: Aug 16 01:32:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 16 01:14:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	331630	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	315782	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	140633	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	82744	17.575	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.320%		
7) Chloroethane-d5	2.899	69	68473m	20.371	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.480%		
11) 1,1-Dichloroethene-d2	4.015	65	33768	15.712	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.840%		
21) 2-Butanone-d5	7.075	46	40349	31.268	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	62.540%		
24) Chloroform-d	7.648	84	170296	19.837	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	79.360%		
26) 1,2-Dichloroethane-d4	8.301	65	96129m	19.659	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	78.640%		
32) Benzene-d6	8.270	84	305494	17.905	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	71.600%		
36) 1,2-Dichloropropane-d6	9.270	67	97595	17.914	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	71.640%		
41) Toluene-d8	10.319	98	284138	18.729	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	74.920%		
43) trans-1,3-Dichloroprop...	10.575	79	40388	18.320	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	73.280%		
47) 2-Hexanone-d5	10.922	63	31644	35.225	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	70.440%		
56) 1,1,2,2-Tetrachloroeth...	12.684	84	82366	20.361	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	81.440%		
66) 1,2-Dichlorobenzene-d4	13.848	152	90643	20.758	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	83.040%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	34044	21.229	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081524\
Data File : VW029906.D
Acq On : 15 Aug 2024 15:31
Operator : SY/MD
Sample : P3626-01
Misc : 4.58g/10mL/MSVOA_W/SOIL/A
ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DCYB5

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 08/16/2024
Supervised By :Mahesh Dadoda 08/21/2024


Quant Time: Aug 16 01:32:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 16 01:14:23 2024
Response via : Initial Calibration

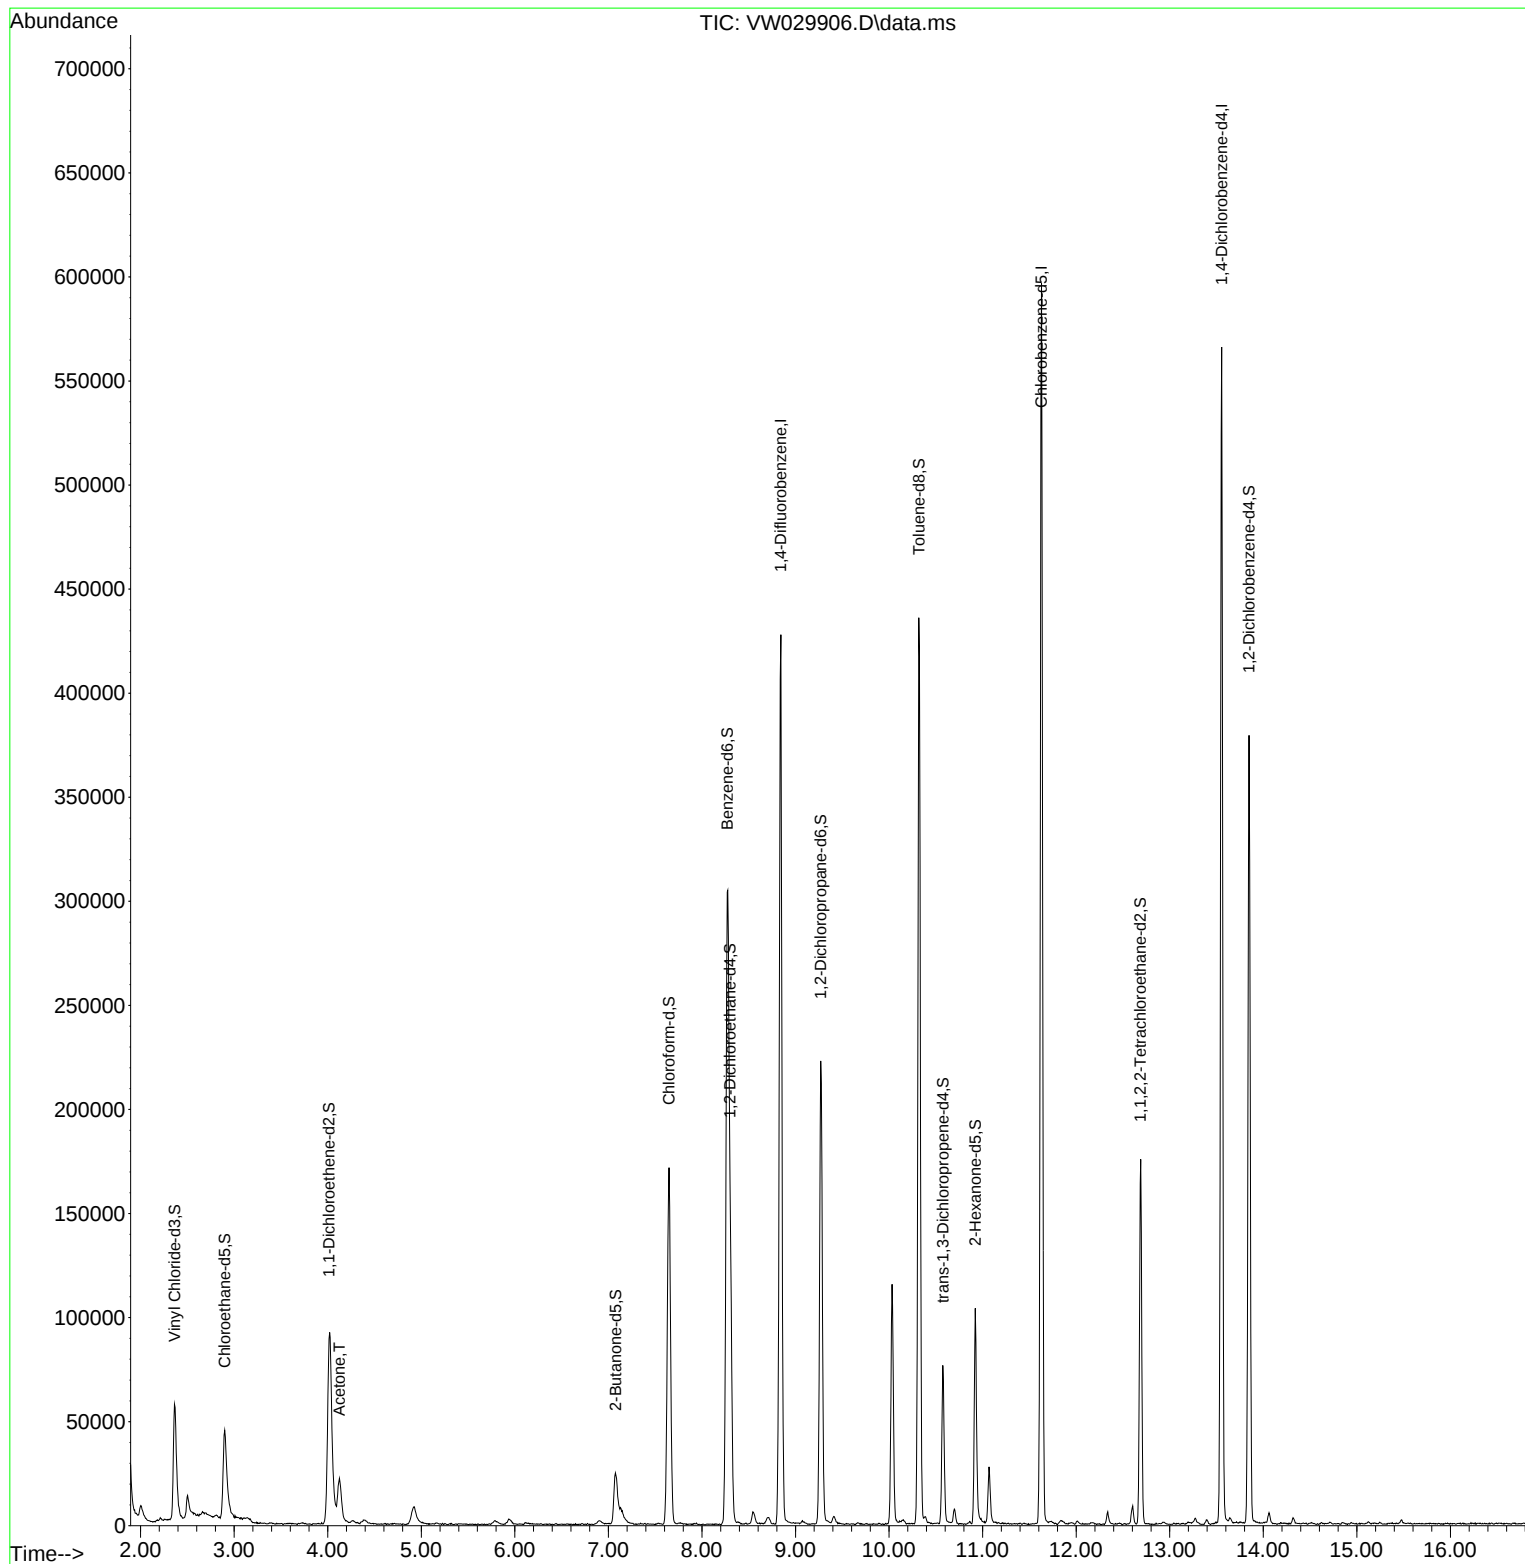

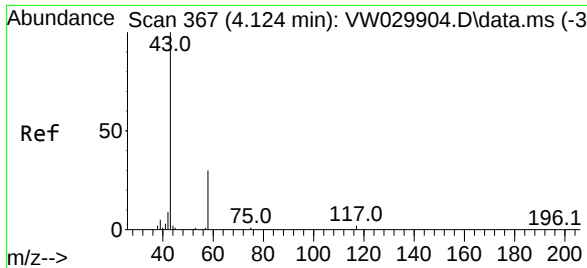

#13
 Acetone
 Concen: 21.229 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW029906.D
 Acq: 15 Aug 2024 15:31

Instrument :
 MSVOA_W
 ClientSampleId :
 DCYB5

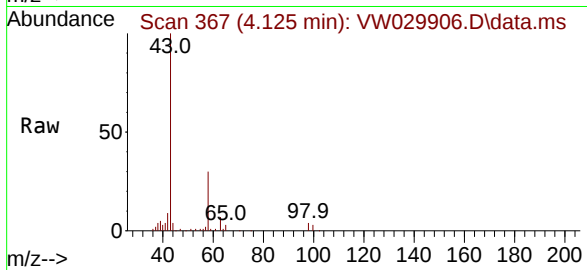

Tgt Ion: 43 Resp: 3404
 Ion Ratio Lower Upper
 43 100
 58 32.3 0.0 57.6

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 08/16/2024
 Supervised By :Mahesh Dadoda 08/21/2024

