


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081618\
Data File : VW004697.D
Acq On : 15 Aug 2018 14:57
Operator : SY/AP
Sample : J4485-01
Misc : 5.78G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BEY68

Manual Integrations
APPROVED

MMDadoda
8/16/2018 11:47:02 AM

Quant Time: Aug 16 04:27:51 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081418S.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 16 02:39:24 2018
Response via : Initial Calibration

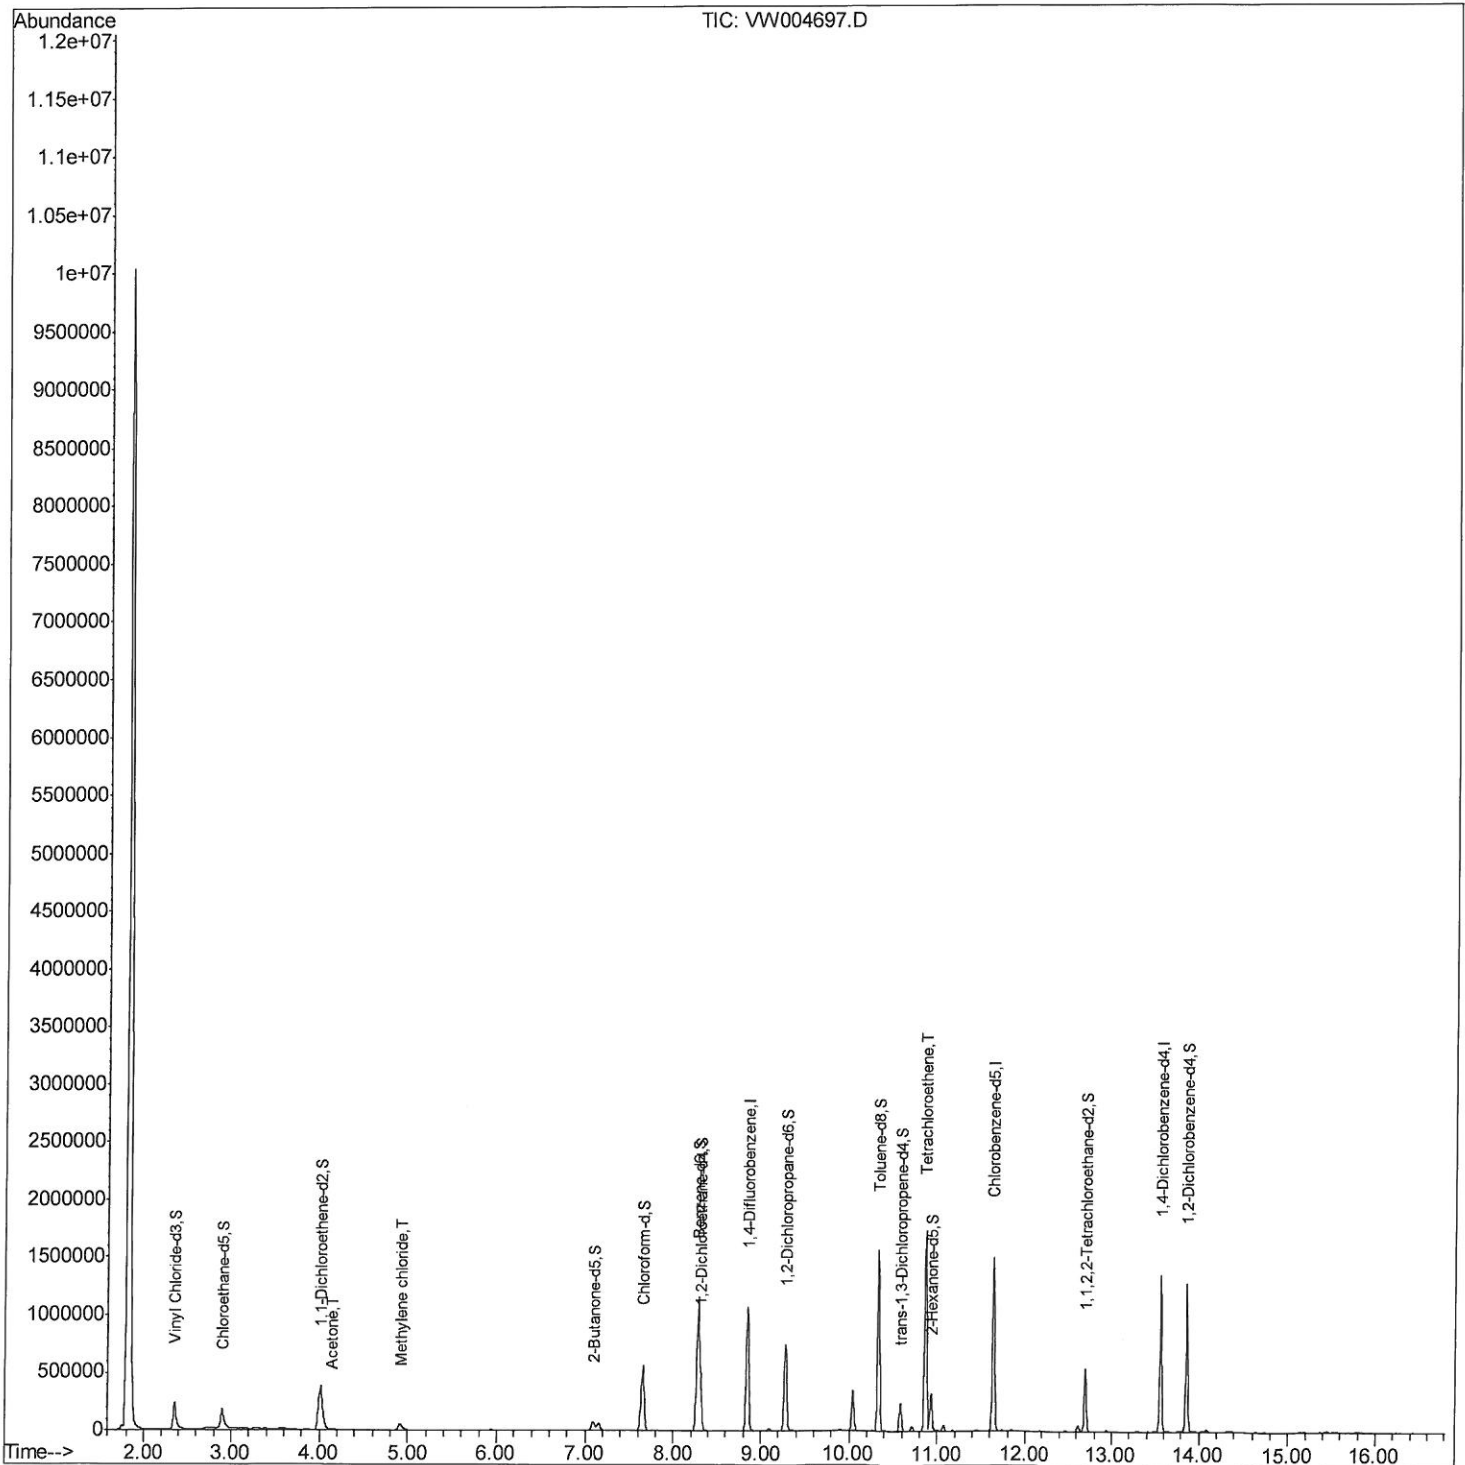

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081618\
 Data File : VW004697.D
 Acq On : 15 Aug 2018 14:57
 Operator : SY/AP
 Sample : J4485-01
 Misc : 5.78G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BEY68

Manual Integrations
 APPROVED

MMDadoda
 8/16/2018 11:47:02 AM

Quant Time: Aug 16 04:12:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081418S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 16 02:39:24 2018
 Response via : Initial Calibration

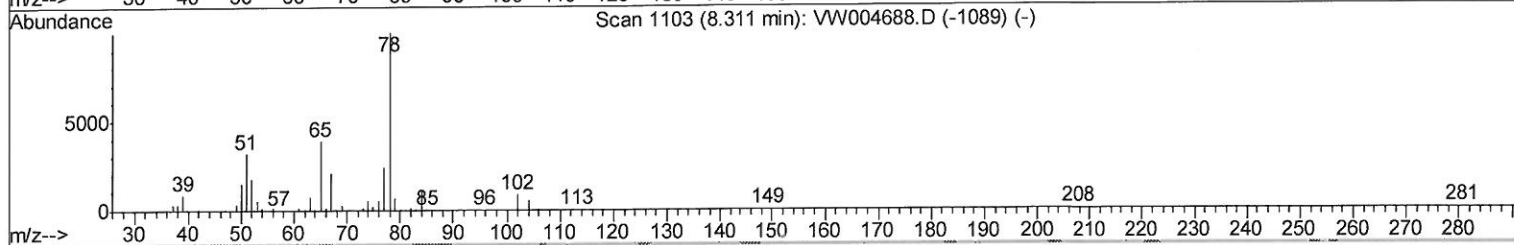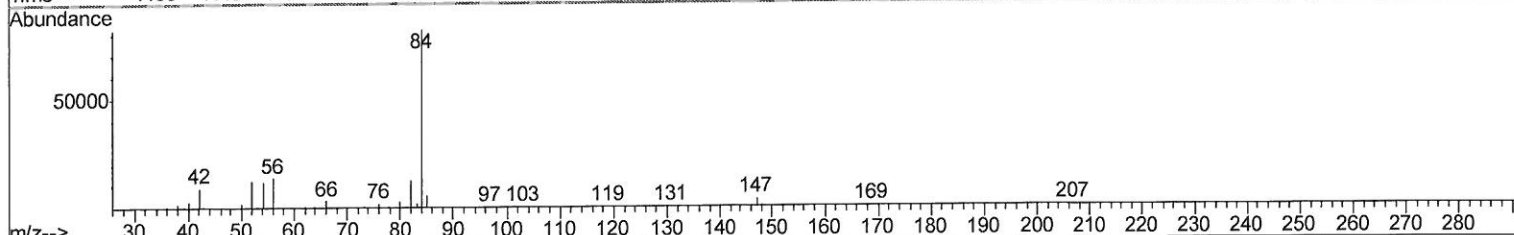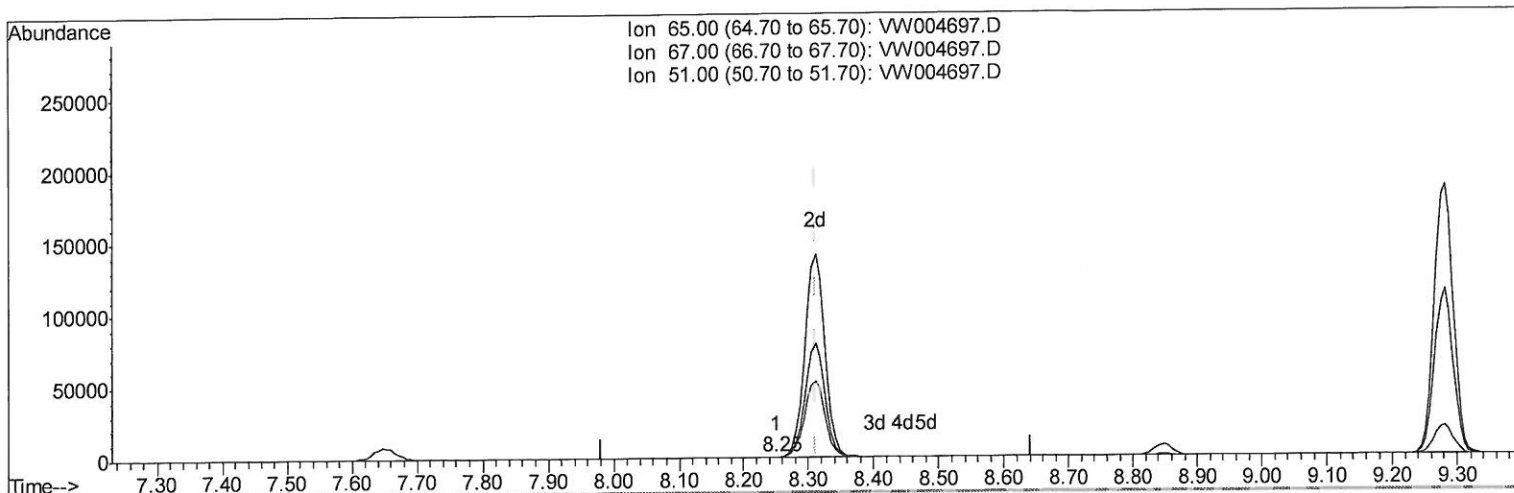

TIC: VW004697.D

(26) 1,2-Dichloroethane-d4 (S)

8.250min (-0.061) 0.01ug/L

response 162

Ion	Exp%	Act%
65.00	100	100
67.00	55.60	46.30
51.00	109.80	79.63
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081618\
 Data File : VW004697.D
 Acq On : 15 Aug 2018 14:57
 Operator : SY/AP
 Sample : J4485-01
 Misc : 5.78G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BEY68

Manual Integrations
 APPROVED

MMDadoda
 8/16/2018 11:47:02 AM

Quant Time: Aug 16 04:12:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081418S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 16 02:39:24 2018
 Response via : Initial Calibration

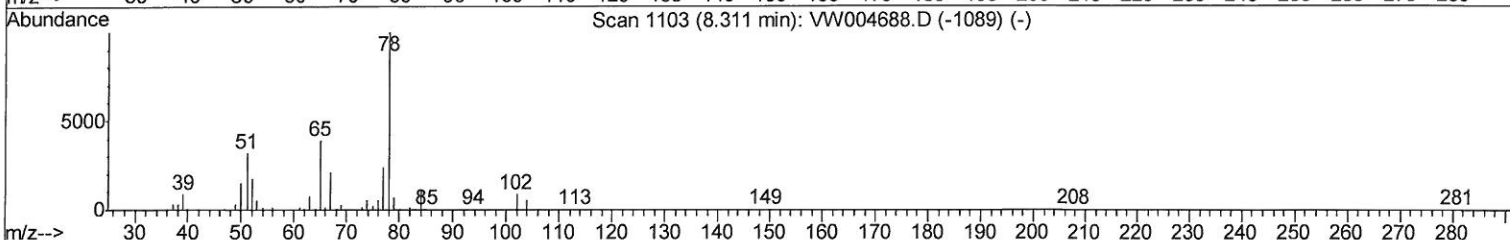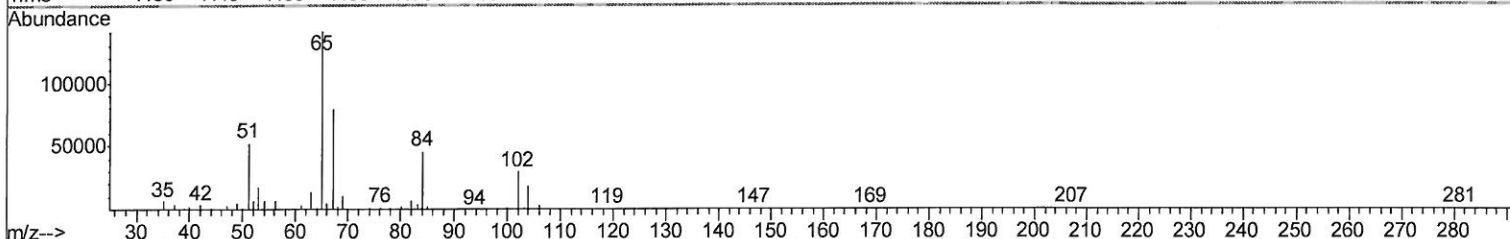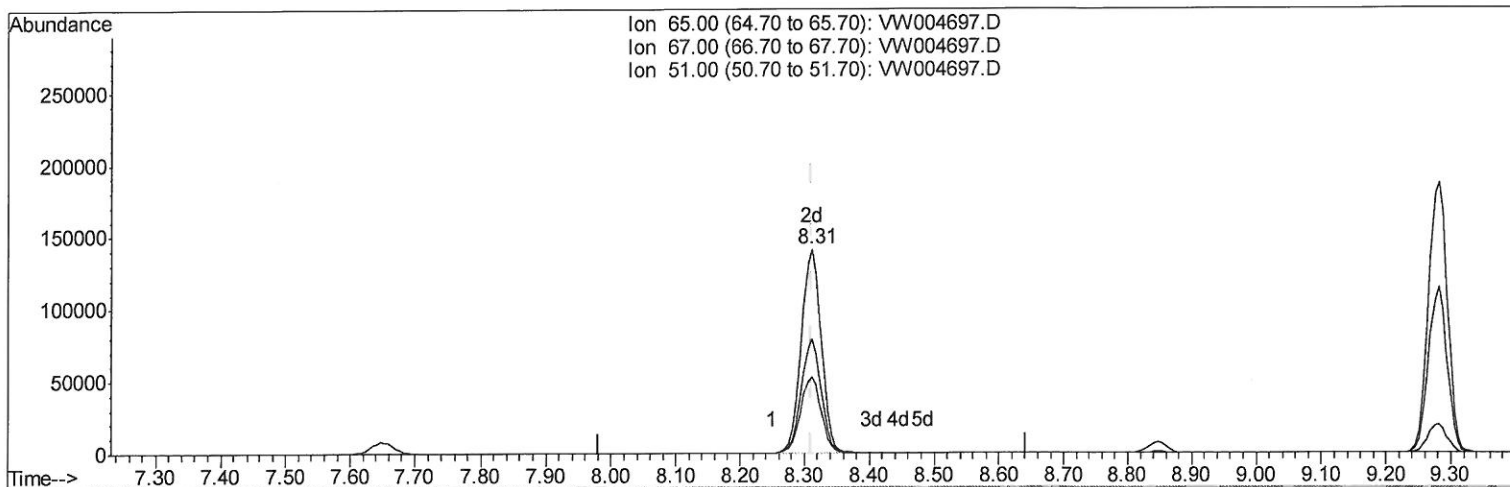

TIC: VW004697.D

(26) 1,2-Dichloroethane-d4 (S)

8.311min (-0.000) 23.83ug/L m

response 302573

Ion	Exp%	Act%
65.00	100	100
67.00	55.60	0.02#
51.00	109.80	0.04#
0.00	0.00	0.00

>08/17/18 Sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081618\
 Data File : VW004697.D
 Acq On : 15 Aug 2018 14:57
 Operator : SY/AP
 Sample : J4485-01
 Misc : 5.78G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BEY68

Manual Integrations
 APPROVED

MMDadoda
 8/16/2018 11:47:02 AM

Quant Time: Aug 16 04:27:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081418S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 16 02:39:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	894211	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	869846	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	362961	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	343582	24.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.68%
7) Chloroethane-d5	2.89	69	269561	24.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.12%
10) 1,1-Dichloroethane-d2	4.01	63	474575	18.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.04%
20) 2-Butanone-d5	7.09	46	134206	34.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.80%
24) Chloroform-d	7.65	84	601342	25.09	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.36%
26) 1,2-Dichloroethane-d4	8.31	65	302573m	23.83	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.32%
29) Benzene-d6	8.28	84	1196451	24.53	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.12%
33) 1,2-Dichloropropane-d6	9.28	67	378260	24.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.84%
37) Toluene-d8	10.33	98	1043411	23.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.36%
38) trans-1,3-Dichloropropene-	10.59	79	132300	21.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.00%
39) 2-Hexanone-d5	10.93	63	107341	35.45	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.90%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	279850	19.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	78.76%
61) 1,2-Dichlorobenzene-d4	13.86	152	355220	25.80	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.20%

Target Compounds					Ovalue
13) Acetone	4.14	43	9319	2.641 ug/L	100
16) Methylene chloride	4.92	84	47990	2.686 ug/L	95
47) Tetrachloroethene	10.87	164	401598	34.739 ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

28/17/18 24